

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
 Data File : VU053801.D
 Acq On : 20 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02340-21 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	90	rBV	54883	62938	11.51%	1.435%
2	1.912	169	178	190	rVB	50128	67403	12.32%	1.536%
3	2.568	367	382	398	rBV3	107616	205355	37.54%	4.681%
4	3.041	518	529	544	rBV2	14665	28717	5.25%	0.655%
5	3.864	776	785	797	rVB3	5700	12609	2.31%	0.287%
6	4.623	1008	1021	1054	rBV2	62842	177283	32.41%	4.041%
7	5.057	1140	1156	1178	rVB2	88892	198310	36.26%	4.520%
8	5.311	1225	1235	1247	rBV3	3478	6816	1.25%	0.155%
9	5.719	1341	1362	1383	rBV3	166566	439418	80.34%	10.016%
10	6.243	1508	1525	1552	rBV	156779	299973	54.84%	6.837%
11	6.536	1603	1616	1637	rBV	288466	546966	100.00%	12.467%
12	6.684	1650	1662	1679	rVB2	107203	205509	37.57%	4.684%
13	7.562	1924	1935	1952	rBV2	45520	81183	14.84%	1.850%
14	7.893	2026	2038	2054	rBV	207791	356592	65.19%	8.128%
15	8.176	2114	2126	2146	rBV	29413	48745	8.91%	1.111%
16	8.549	2231	2242	2255	rBV3	35833	59248	10.83%	1.350%
17	8.629	2255	2267	2299	rBV	219755	408977	74.77%	9.322%
18	9.414	2497	2511	2535	rBV	215767	362426	66.26%	8.261%
19	10.751	2915	2927	2940	rBV	87335	138885	25.39%	3.166%
20	11.809	3243	3256	3275	rBV	215497	346829	63.41%	7.905%
21	12.189	3359	3374	3394	rBV	201883	333129	60.90%	7.593%




Sum of corrected areas: 4387311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053801.D
Acq On : 20 Apr 2023 13:10
Operator : JC/MD
Sample : 02340-21 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

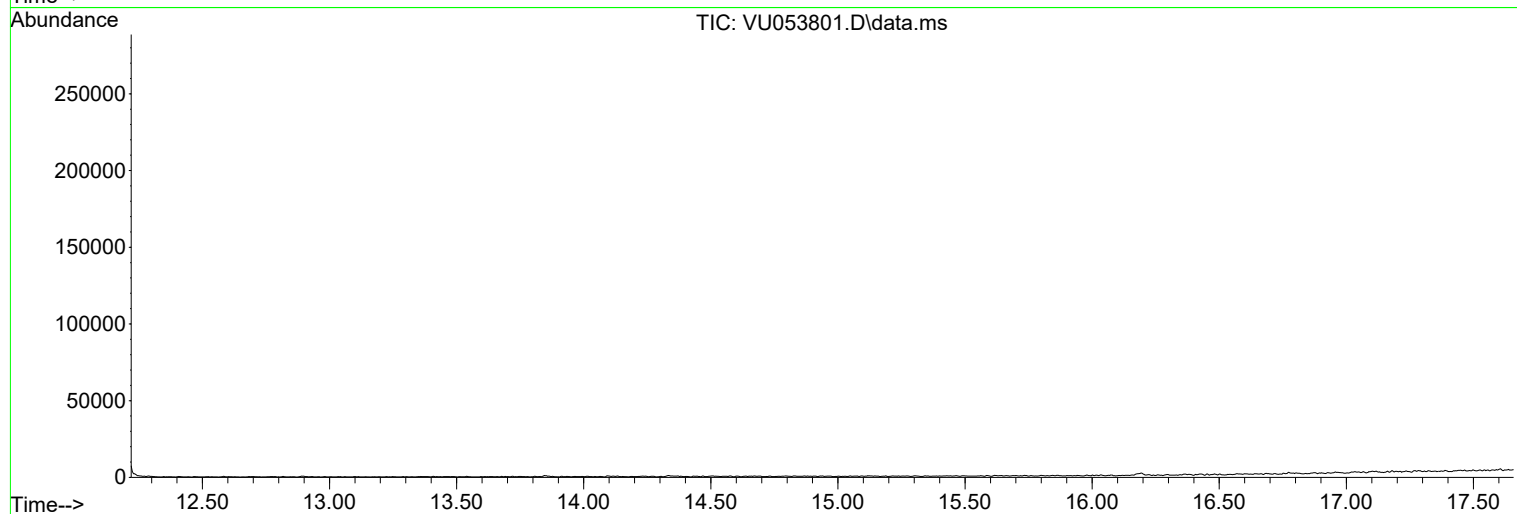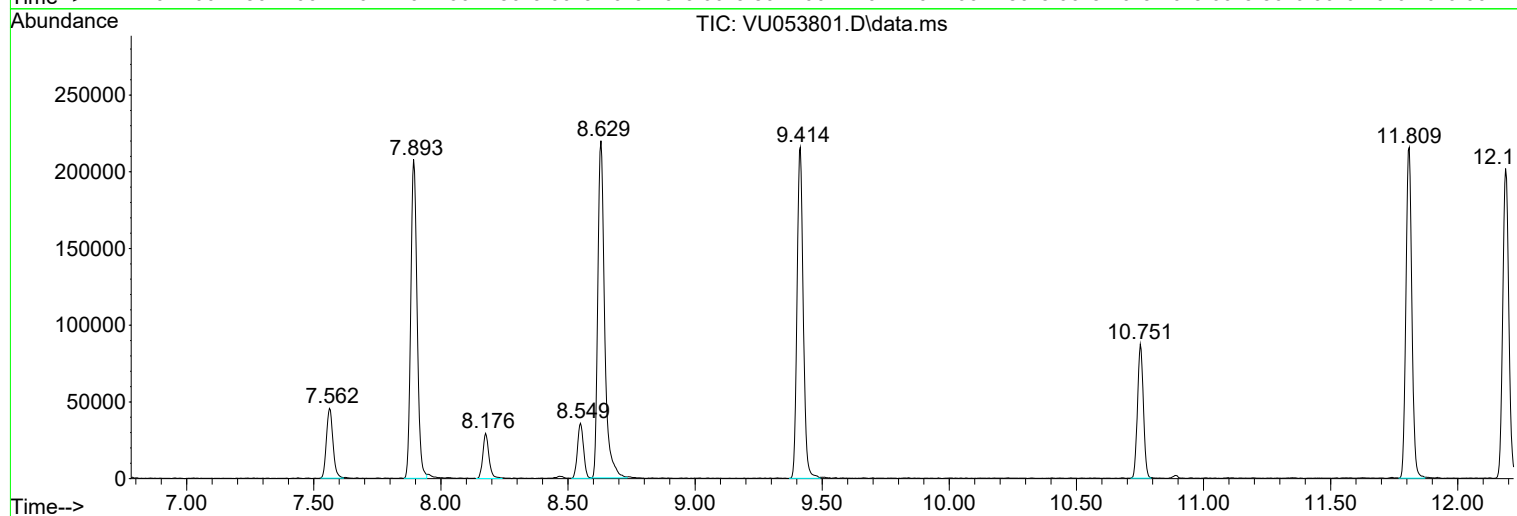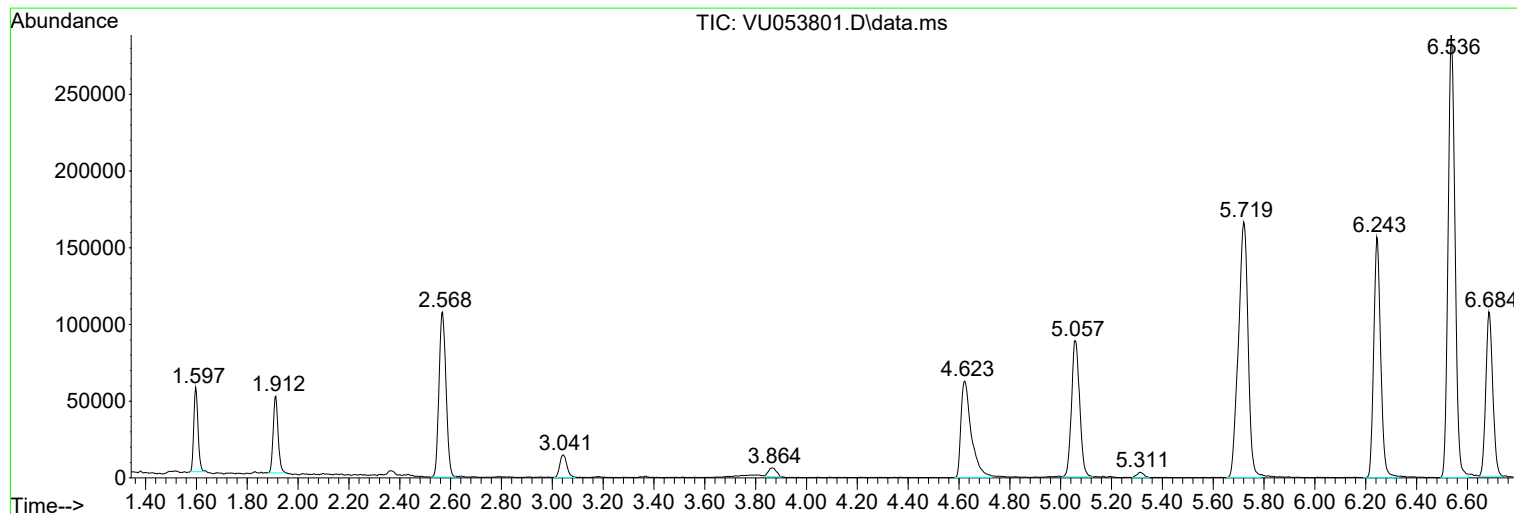

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053801.D
Acq On : 20 Apr 2023 13:10
Operator : JC/MD
Sample : 02340-21 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053801.D
Acq On : 20 Apr 2023 13:10
Operator : JC/MD
Sample : 02340-21 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------