

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
 Data File : VU053813.D
 Acq On : 20 Apr 2023 17:59
 Operator : JC/MD
 Sample : 02396-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB	63109	73552	17.02%	2.025%
2	1.916	170	179	191	rBV	52100	69351	16.05%	1.909%
3	2.565	369	381	402	rVB	100212	164184	38.00%	4.520%
4	3.044	520	530	540	rBV2	4477	8081	1.87%	0.222%
5	3.182	560	573	585	rBV	5209	10589	2.45%	0.291%
6	4.639	1011	1026	1061	rBV	43573	150733	34.88%	4.149%
7	5.057	1141	1156	1174	rVB	87844	191186	44.25%	5.263%
8	5.722	1343	1363	1385	rBV3	168097	432097	100.00%	11.895%
9	6.247	1512	1526	1545	rBV	153949	300497	69.54%	8.272%
10	6.687	1645	1663	1686	rBV	102071	199549	46.18%	5.493%
11	7.562	1923	1935	1957	rBV	50086	88891	20.57%	2.447%
12	7.893	2024	2038	2060	rBV	213067	371871	86.06%	10.237%
13	8.179	2116	2127	2145	rBV	28743	49463	11.45%	1.362%
14	8.468	2207	2217	2225	rBV3	5091	9480	2.19%	0.261%
15	8.632	2256	2268	2298	rBV2	181667	355470	82.27%	9.785%
16	9.414	2499	2511	2526	rBV	217558	361486	83.66%	9.951%
17	10.751	2916	2927	2944	rVB	74841	118953	27.53%	3.274%
18	10.889	2960	2970	2982	rVB2	6981	11502	2.66%	0.317%
19	11.809	3243	3256	3274	rBV	216739	357447	82.72%	9.840%
20	12.188	3360	3374	3395	rBV	186665	308326	71.36%	8.487%




Sum of corrected areas: 3632708

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053813.D
Acq On : 20 Apr 2023 17:59
Operator : JC/MD
Sample : 02396-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

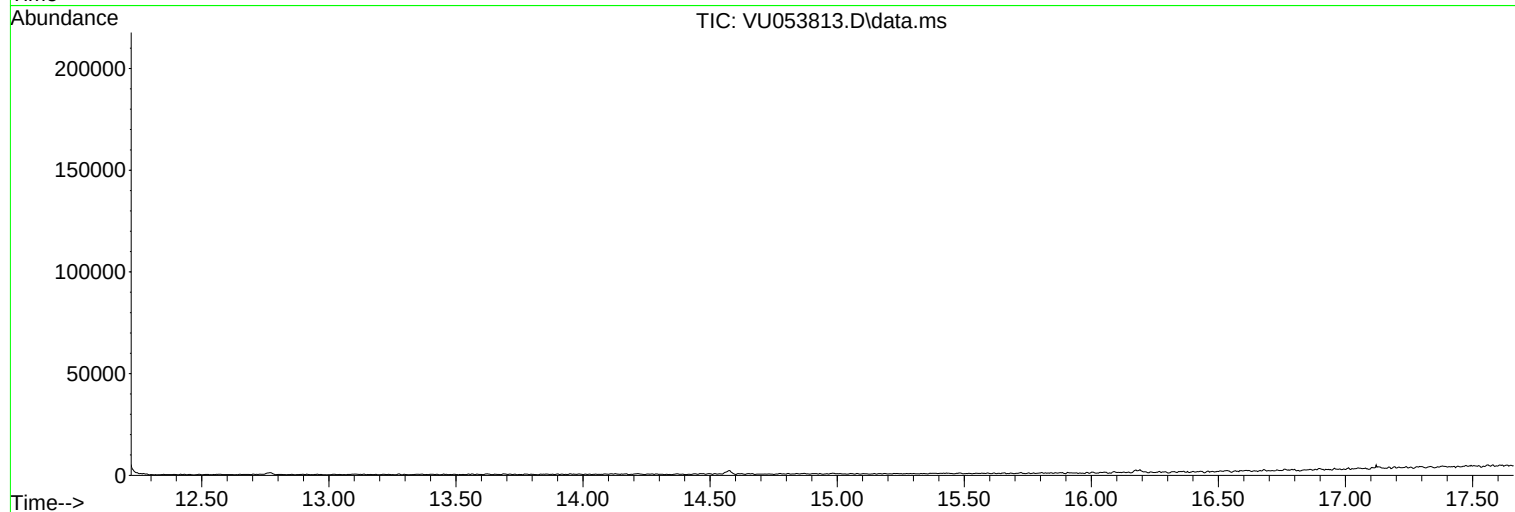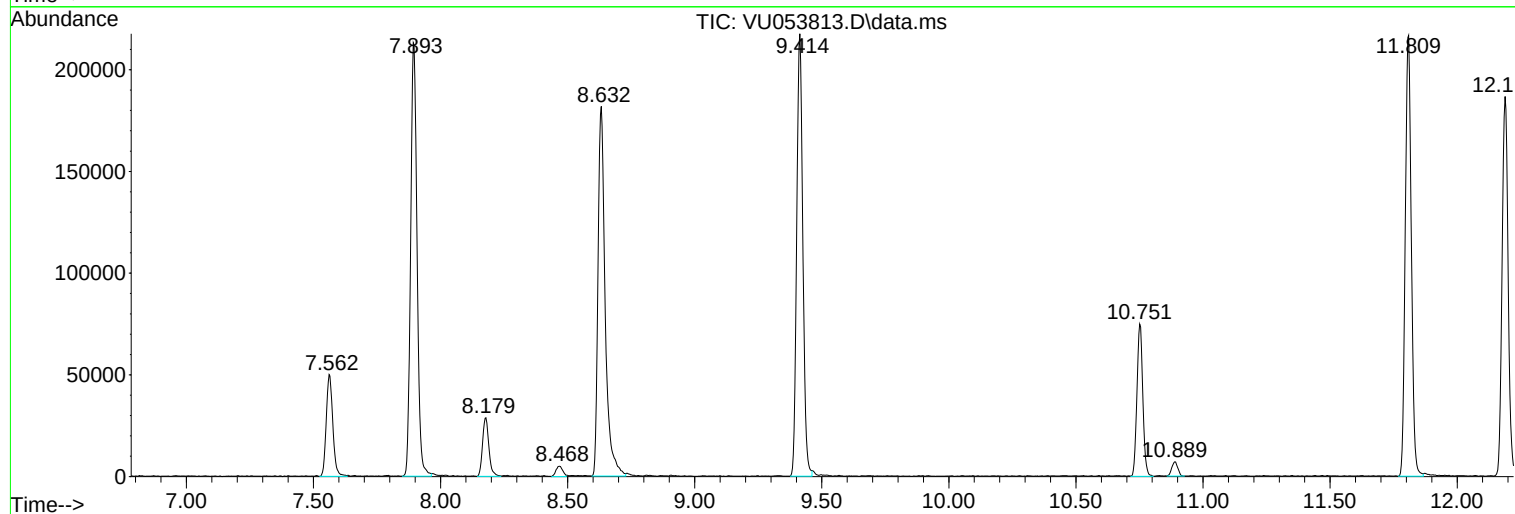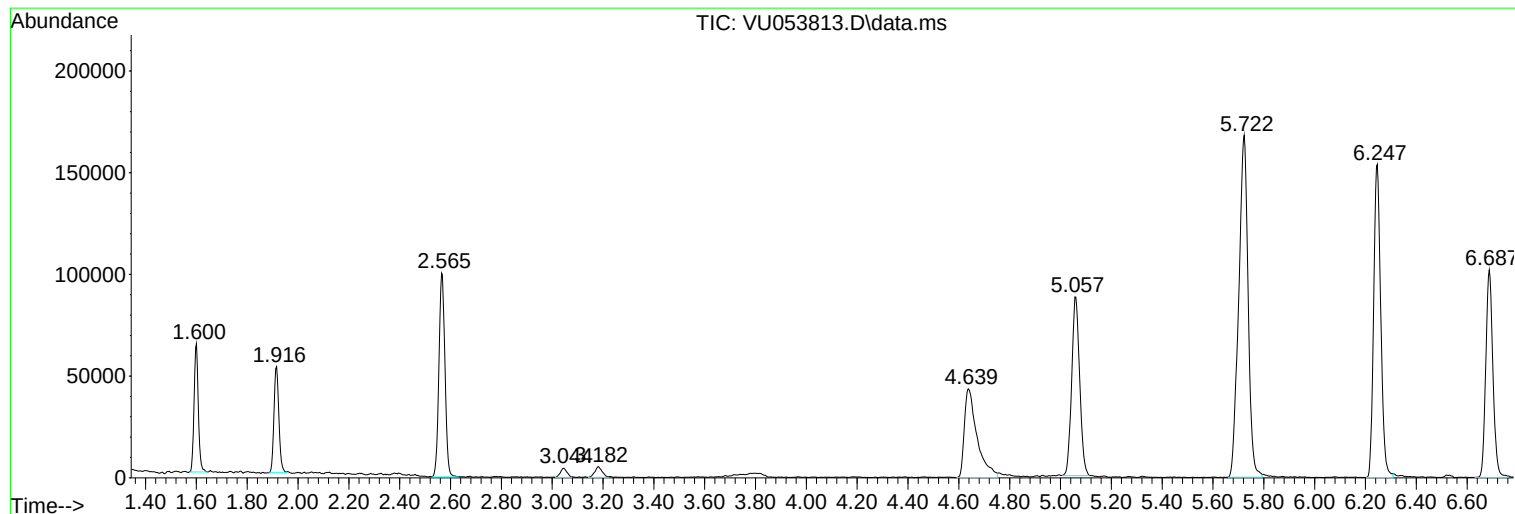

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053813.D
Acq On : 20 Apr 2023 17:59
Operator : JC/MD
Sample : 02396-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053813.D
Acq On : 20 Apr 2023 17:59
Operator : JC/MD
Sample : 02396-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc