

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
 Data File : VU053815.D
 Acq On : 20 Apr 2023 18:47
 Operator : JC/MD
 Sample : 02392-07 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rVB	57492	69312	17.16%	1.970%
2	1.912	170	178	188	rBV	48867	63773	15.79%	1.812%
3	2.565	369	381	399	rBV	92072	152110	37.67%	4.323%
4	3.047	520	531	543	rVB3	4721	8654	2.14%	0.246%
5	4.636	1010	1025	1055	rBV2	40567	134484	33.30%	3.822%
6	5.060	1141	1157	1177	rVB2	82133	184176	45.61%	5.234%
7	5.723	1344	1363	1389	rBV2	156217	403807	100.00%	11.475%
8	6.247	1512	1526	1546	rBV	163932	314097	77.78%	8.926%
9	6.539	1606	1617	1633	rVB4	21450	40890	10.13%	1.162%
10	6.687	1645	1663	1681	rBV	95144	188323	46.64%	5.352%
11	7.562	1925	1935	1954	rBV	44792	79476	19.68%	2.259%
12	7.893	2025	2038	2062	rBV	195597	344217	85.24%	9.782%
13	8.176	2115	2126	2138	rBV	27342	45342	11.23%	1.289%
14	8.552	2231	2243	2253	rBV3	6769	10843	2.69%	0.308%
15	8.632	2253	2268	2299	rBV3	169857	334441	82.82%	9.504%
16	9.414	2499	2511	2535	rBV	222219	376108	93.14%	10.688%
17	10.751	2915	2927	2943	rVB	69013	112656	27.90%	3.201%
18	11.809	3244	3256	3276	rBV	232009	370835	91.83%	10.538%
19	12.189	3362	3374	3387	rBV	173416	285397	70.68%	8.110%




Sum of corrected areas: 3518941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053815.D
Acq On : 20 Apr 2023 18:47
Operator : JC/MD
Sample : 02392-07 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

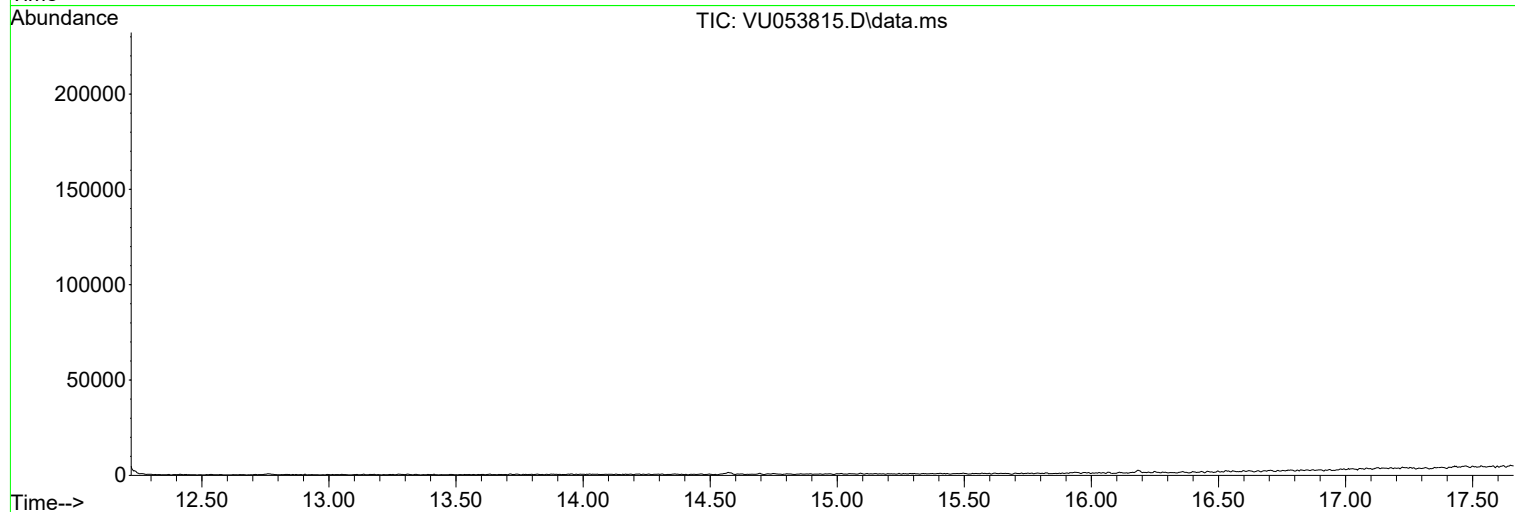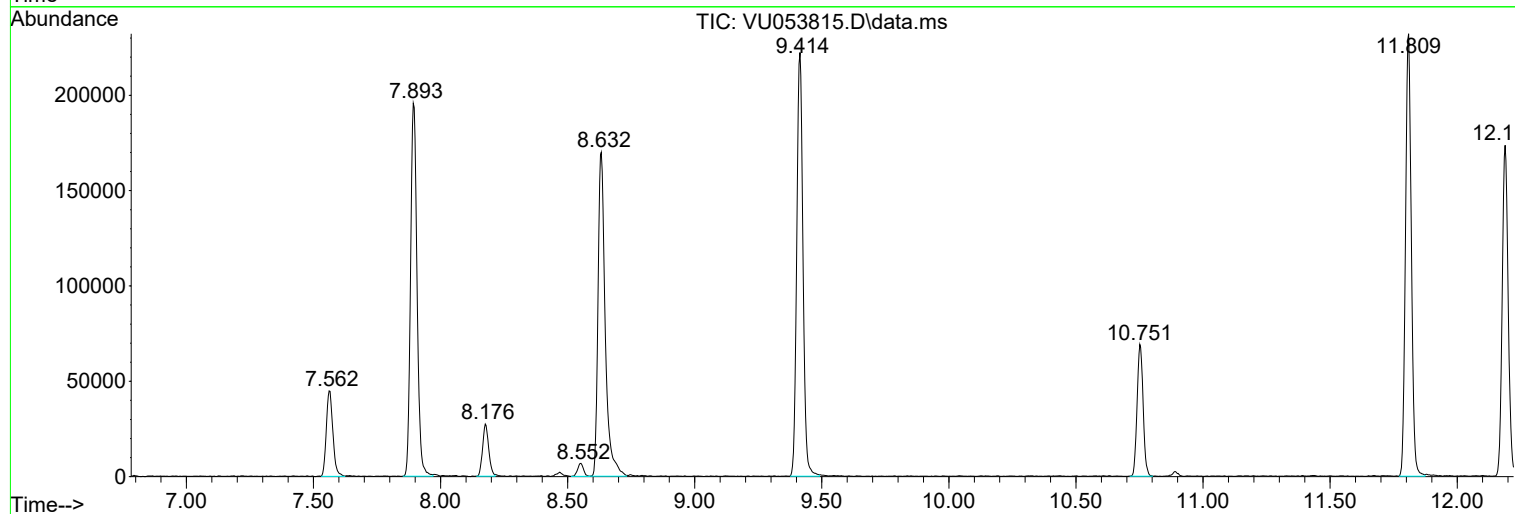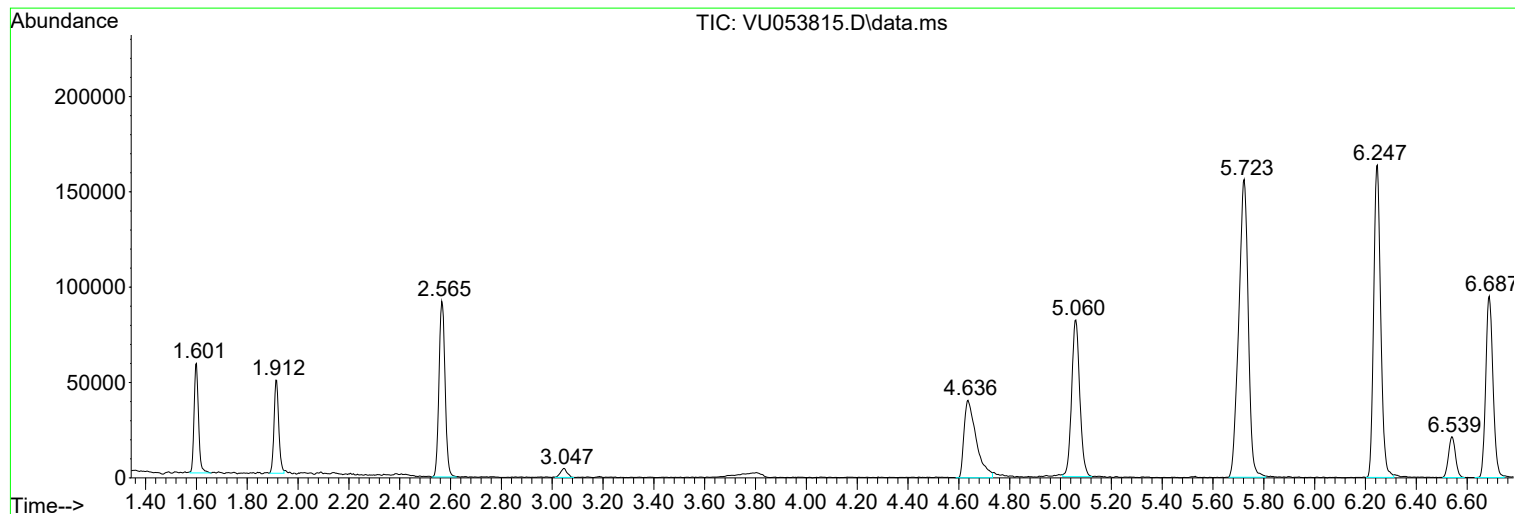

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053815.D
Acq On : 20 Apr 2023 18:47
Operator : JC/MD
Sample : 02392-07 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053815.D
Acq On : 20 Apr 2023 18:47
Operator : JC/MD
Sample : 02392-07 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------