

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
 Data File : VU053816.D
 Acq On : 20 Apr 2023 19:11
 Operator : JC/MD
 Sample : 02392-12 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	71	81	90	rBV	60569	72190	16.92%	1.913%
2	1.916	170	179	192	rBV	50289	68095	15.96%	1.805%
3	2.565	369	381	396	rBV	98377	163577	38.33%	4.335%
4	3.044	521	530	541	rVB2	4810	9239	2.17%	0.245%
5	4.639	1013	1026	1066	rBV2	40631	146487	34.33%	3.882%
6	5.057	1140	1156	1175	rVB	85285	184788	43.30%	4.897%
7	5.723	1343	1363	1380	rBV2	169516	426728	100.00%	11.309%
8	6.247	1512	1526	1551	rBV	153704	300245	70.36%	7.957%
9	6.539	1602	1617	1635	rBV3	40754	78603	18.42%	2.083%
10	6.687	1650	1663	1680	rBV	100530	196392	46.02%	5.205%
11	7.562	1924	1935	1950	rBV	48417	84630	19.83%	2.243%
12	7.893	2026	2038	2068	rBV	209655	370061	86.72%	9.807%
13	8.176	2115	2126	2148	rVB2	27954	48554	11.38%	1.287%
14	8.549	2229	2242	2257	rBV2	74143	121682	28.52%	3.225%
15	8.632	2257	2268	2301	rVV2	180197	359089	84.15%	9.516%
16	9.414	2496	2511	2537	rBV	215592	363445	85.17%	9.632%
17	10.751	2916	2927	2944	rBV2	75590	119658	28.04%	3.171%
18	11.806	3243	3255	3274	rBV	219813	352919	82.70%	9.353%
19	12.189	3361	3374	3394	rBV	184975	307017	71.95%	8.136%




Sum of corrected areas: 3773399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053816.D
Acq On : 20 Apr 2023 19:11
Operator : JC/MD
Sample : 02392-12 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

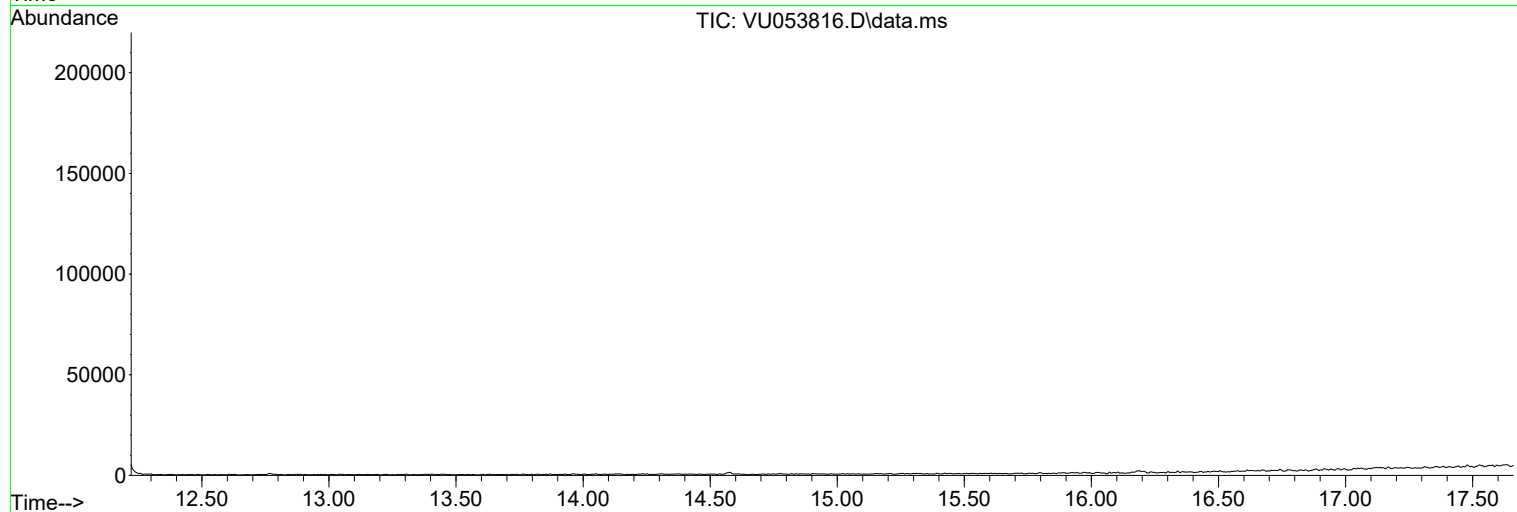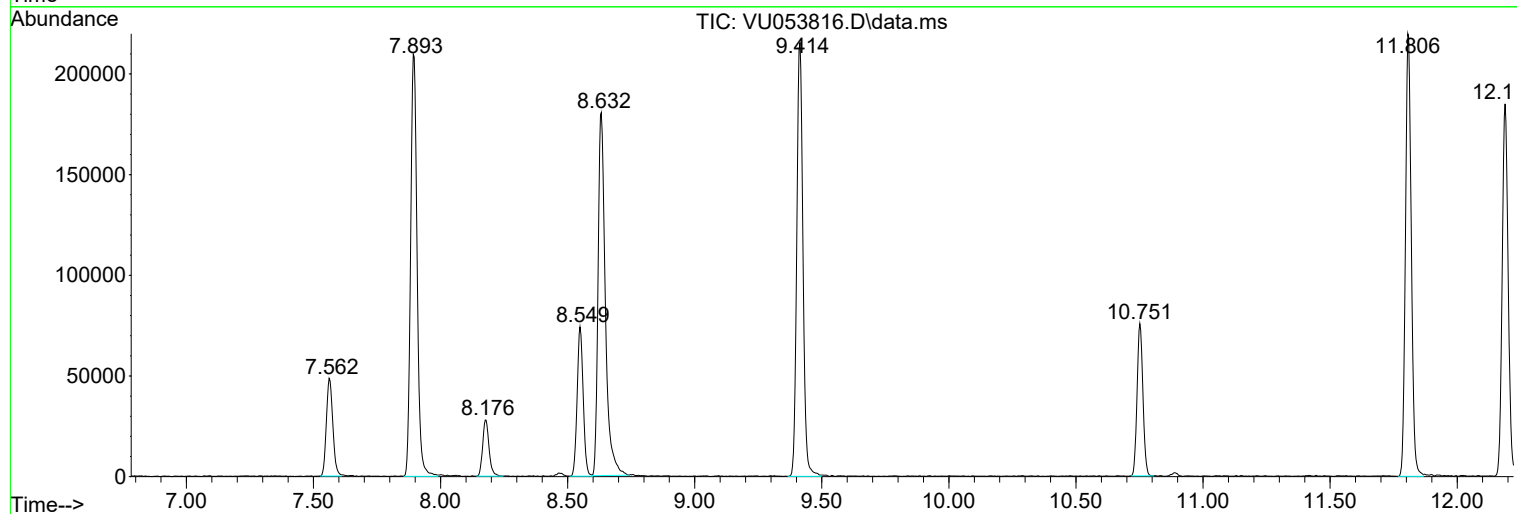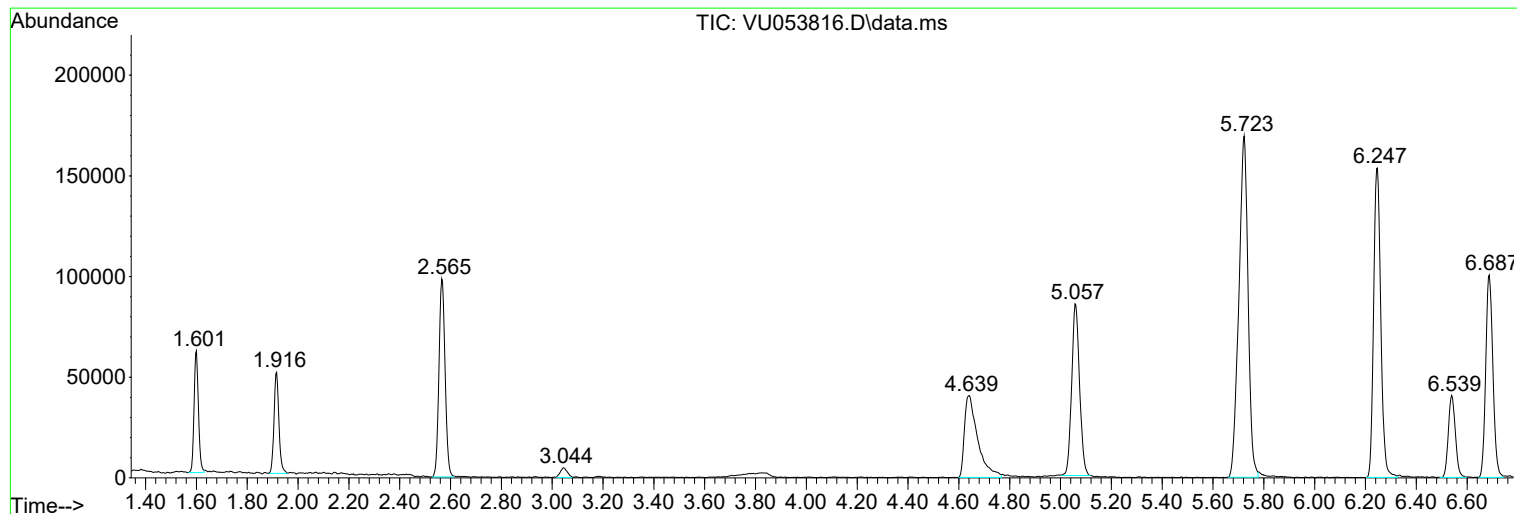

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053816.D
Acq On : 20 Apr 2023 19:11
Operator : JC/MD
Sample : 02392-12 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053816.D
Acq On : 20 Apr 2023 19:11
Operator : JC/MD
Sample : 02392-12 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------