

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
 Data File : VU053817.D
 Acq On : 20 Apr 2023 19:36
 Operator : JC/MD
 Sample : 02392-13 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rBV	59651	71789	17.05%	1.906%
2	1.916	169	179	192	rBV	51057	66679	15.84%	1.771%
3	2.565	367	381	399	rBV	96950	157590	37.43%	4.184%
4	3.044	521	530	543	rVB2	4704	8556	2.03%	0.227%
5	4.636	1012	1025	1062	rBV2	38749	137501	32.66%	3.651%
6	5.060	1141	1157	1187	rVB	86012	195044	46.32%	5.179%
7	5.722	1343	1363	1388	rBV3	161499	421054	100.00%	11.180%
8	6.247	1512	1526	1547	rBV	168112	323756	76.89%	8.597%
9	6.539	1606	1617	1632	rBV7	7603	15412	3.66%	0.409%
10	6.687	1650	1663	1686	rBV2	99408	197241	46.84%	5.237%
11	7.562	1922	1935	1953	rBV2	47472	84843	20.15%	2.253%
12	7.893	2021	2038	2063	rBV	207305	359322	85.34%	9.541%
13	8.176	2115	2126	2142	rBV	27417	46010	10.93%	1.222%
14	8.549	2230	2242	2257	rBV	88796	148108	35.18%	3.933%
15	8.632	2257	2268	2296	rBV2	176408	340644	80.90%	9.045%
16	9.414	2498	2511	2533	rBV	235094	396316	94.12%	10.523%
17	10.751	2916	2927	2941	rBV2	71969	115433	27.42%	3.065%
18	11.809	3244	3256	3273	rBV	240490	384990	91.43%	10.223%
19	12.188	3360	3374	3393	rBV	180382	295803	70.25%	7.854%




Sum of corrected areas: 3766091

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053817.D
Acq On : 20 Apr 2023 19:36
Operator : JC/MD
Sample : 02392-13 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

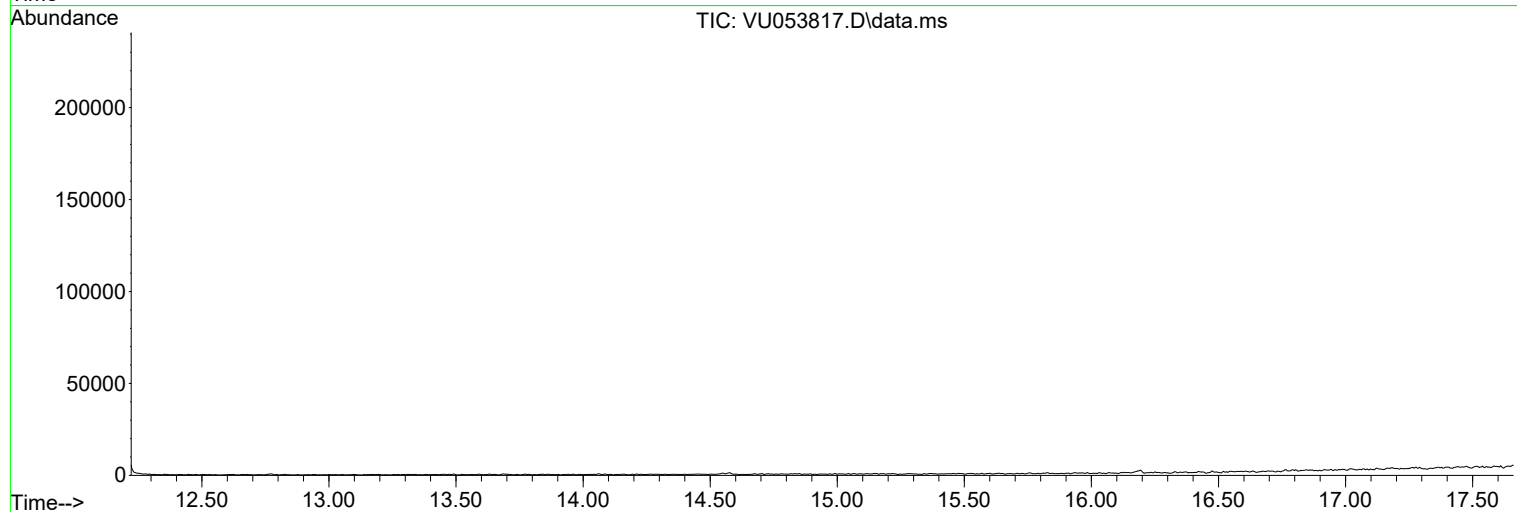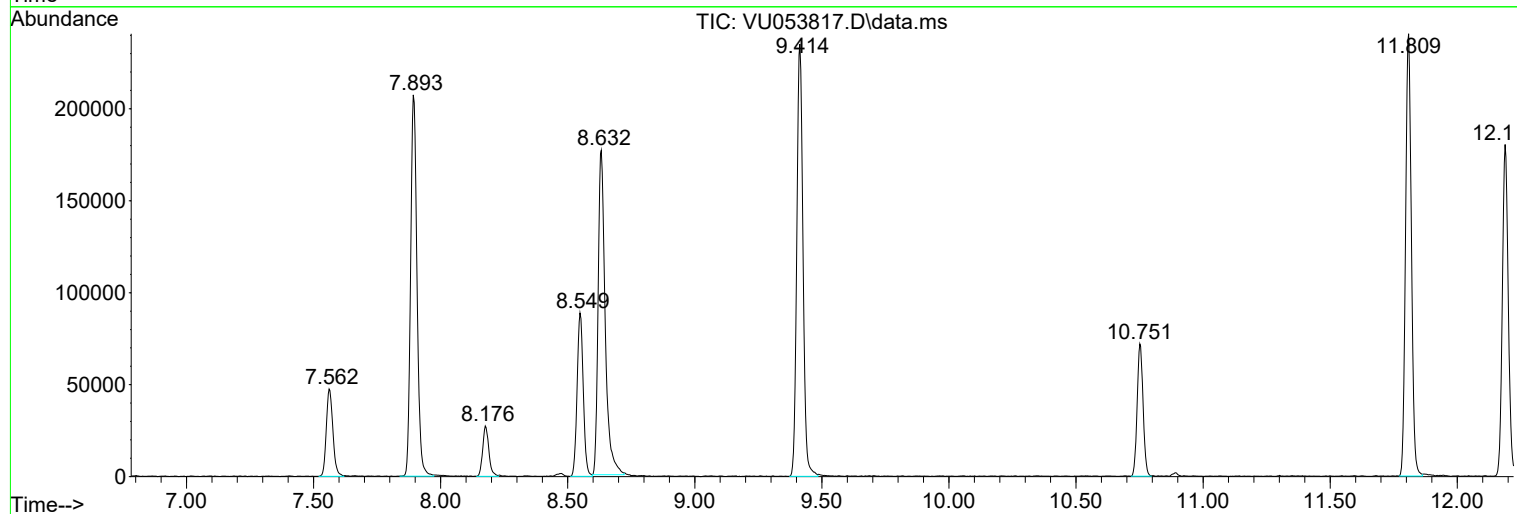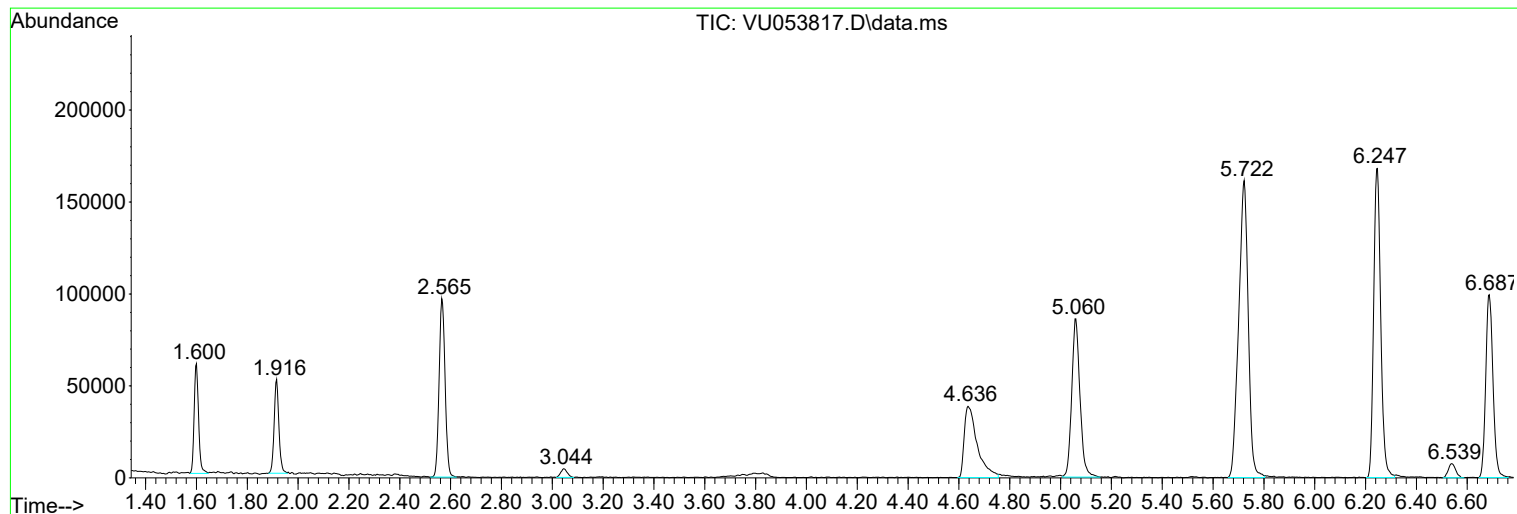

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053817.D
Acq On : 20 Apr 2023 19:36
Operator : JC/MD
Sample : 02392-13 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053817.D
Acq On : 20 Apr 2023 19:36
Operator : JC/MD
Sample : 02392-13 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------