
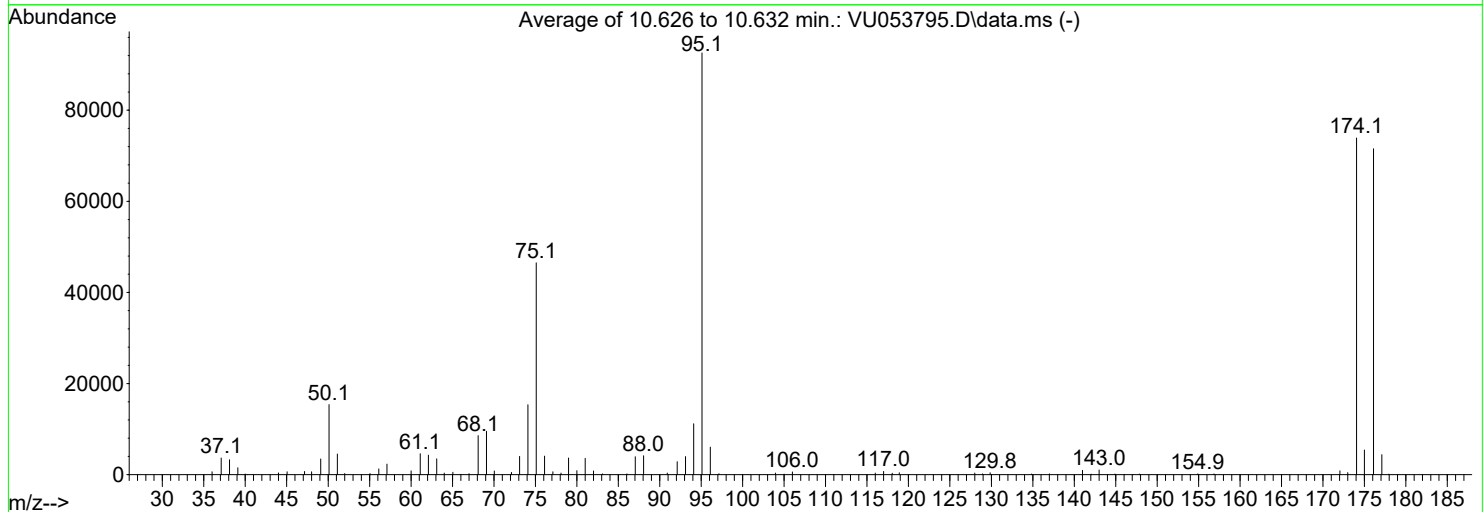


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053795.D
Acq On : 20 Apr 2023 09:10
Operator : JC/MD
Sample : BFB006
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB006

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 19 04:58:28 2023

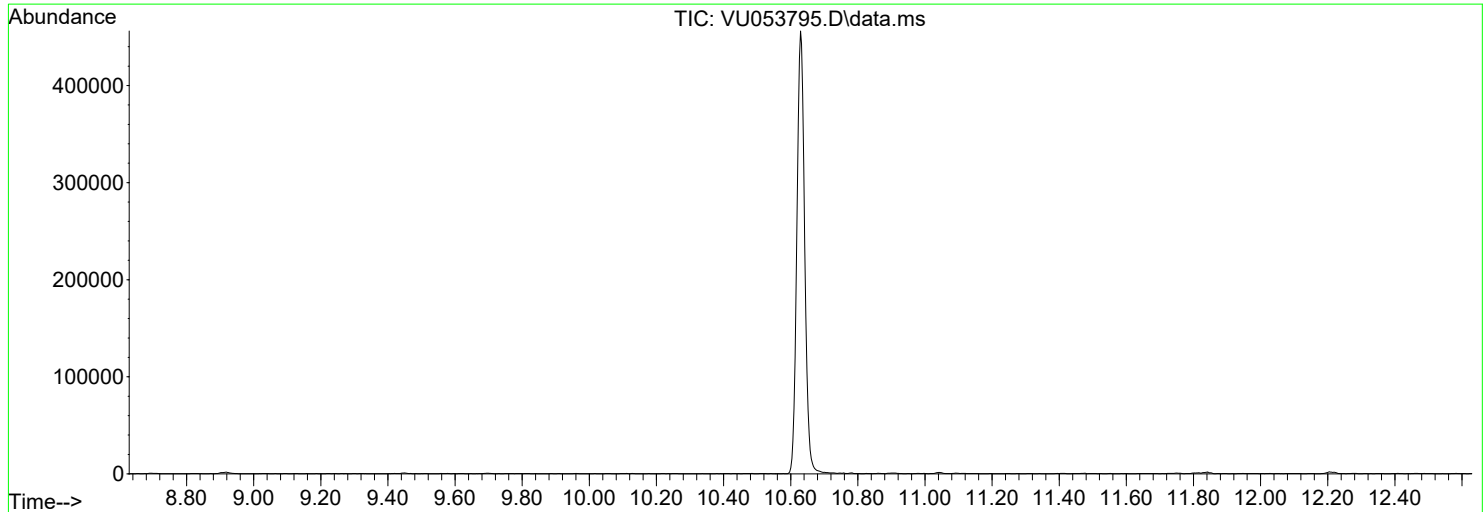

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	15377	PASS
75	95	30	80	50.2	46512	PASS
95	95	100	100	100.0	92600	PASS
96	95	5	9	6.5	6028	PASS
173	174	0.00	2	0.6	449	PASS
174	95	50	120	79.8	73915	PASS
175	174	5	9	7.3	5424	PASS
176	174	95	101	96.8	71547	PASS
177	176	5	9	6.1	4389	PASS

m/z	Abundance
43.90	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
36.00	661.0
37.10	3589.0
38.10	3455.0
39.10	1496.0
40.00	154.0
44.00	566.0
45.10	671.0
47.10	792.0
48.00	617.0
49.10	3326.0
50.10	15252.0
51.10	4481.0
52.00	242.0
55.00	228.0
56.10	1210.0
57.10	2507.0
60.00	878.0
61.10	4523.0
62.10	4317.0
63.10	3165.0
64.00	415.0
65.10	527.0
67.00	171.0
68.10	8264.0
69.10	9304.0
70.10	778.0
72.10	485.0
73.10	3878.0
74.10	15187.0
75.10	45312.0
76.10	3857.0
77.10	600.0
78.20	324.0
79.00	3704.0
80.00	845.0
81.00	3541.0
82.00	692.0
83.10	176.0
86.10	167.0
87.00	3821.0
88.00	3966.0
90.90	389.0
92.10	2683.0
93.10	3914.0
94.10	11080.0
95.10	89480.0
96.10	6110.0
97.20	193.0
104.00	317.0
105.00	164.0
106.00	547.0
116.00	325.0
117.00	760.0
118.00	324.0
118.90	460.0
128.00	313.0
129.00	217.0
129.90	427.0
134.90	136.0
137.00	175.0
141.00	933.0
142.00	158.0
143.00	1013.0
144.90	170.0
146.10	129.0
147.90	130.0
154.90	174.0
156.80	160.0
172.10	755.0
173.00	370.0
174.00	70888.0
175.00	5297.0
176.10	67256.0
177.10	4059.0
178.00	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
36.00	644.0
37.10	3736.0
38.10	3371.0
39.10	1568.0
40.00	165.0
44.10	627.0
45.10	673.0
47.20	741.0
48.00	689.0
49.10	3585.0
50.10	15996.0
51.10	4680.0
52.00	262.0
55.00	258.0
56.10	1248.0
57.10	2371.0
60.00	847.0
61.10	4816.0
62.10	4481.0
63.10	3544.0
64.00	353.0
65.10	510.0
66.00	103.0
67.00	233.0
68.10	8742.0
69.10	9860.0
70.00	838.0
72.10	521.0
73.10	4176.0
74.10	15885.0
75.10	47952.0
76.10	4256.0
77.10	651.0
78.10	363.0
79.00	3769.0
80.00	897.0
81.00	3679.0
82.00	835.0
83.10	175.0
86.10	172.0
87.10	4005.0
88.10	4252.0
90.90	377.0
92.10	2950.0
93.10	4071.0
94.10	11378.0
95.10	95784.0
96.10	6252.0
97.20	195.0
103.90	342.0
105.00	140.0
106.00	609.0
111.00	109.0
116.00	352.0
117.00	730.0
118.10	301.0
118.90	440.0
128.00	374.0
129.00	204.0
129.90	414.0
134.90	145.0
137.00	176.0
141.00	991.0
142.10	134.0
143.00	1078.0
144.90	155.0
146.00	105.0
147.90	144.0
154.90	194.0
156.90	174.0
172.00	931.0
173.00	458.0
174.00	75840.0
175.00	5594.0
176.10	73880.0
177.10	4461.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
36.00	568.0
37.10	3641.0
38.10	2982.0
39.10	1458.0
40.00	144.0
40.30	135.0
44.10	611.0
45.00	560.0
47.20	604.0
48.00	595.0
49.10	3430.0
50.10	14884.0
51.10	4462.0
52.00	205.0
55.10	243.0
56.10	1344.0
57.10	2037.0
60.00	784.0
61.10	4520.0
62.10	4091.0
63.10	3751.0
64.00	281.0
65.00	498.0
66.00	124.0
67.00	222.0
68.10	8748.0
69.10	9454.0
70.00	845.0
72.10	476.0
73.10	3994.0
74.10	14944.0
75.10	46272.0
76.10	4095.0
77.10	653.0
78.00	388.0
79.00	3522.0
80.00	893.0
81.00	3558.0
82.00	874.0
83.10	165.0
85.90	166.0
87.10	3956.0
88.10	4207.0
90.90	339.0
92.10	2894.0
93.10	3935.0
94.10	11091.0
95.10	92536.0
96.10	5722.0
97.10	216.0
103.90	364.0
106.00	596.0
111.00	137.0
116.00	410.0
117.00	635.0
118.10	290.0
118.90	426.0
128.00	359.0
128.90	145.0
129.80	428.0
134.80	179.0
137.00	152.0
141.00	957.0
143.00	995.0
144.90	134.0
147.10	135.0
147.80	180.0
154.90	211.0
156.90	180.0
172.00	902.0
173.00	518.0
174.10	75016.0
175.00	5381.0
176.10	73504.0
177.10	4646.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006