


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043261.D
Acq On : 21 Apr 2021 19:31
Operator : SY/MD
Sample : M2088-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4489

Manual Integrations
APPROVED

MMDadoda
4/23/2021 2:47:32 PM

Quant Time: Apr 22 04:46:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 22 04:40:57 2021
Response via : Initial Calibration

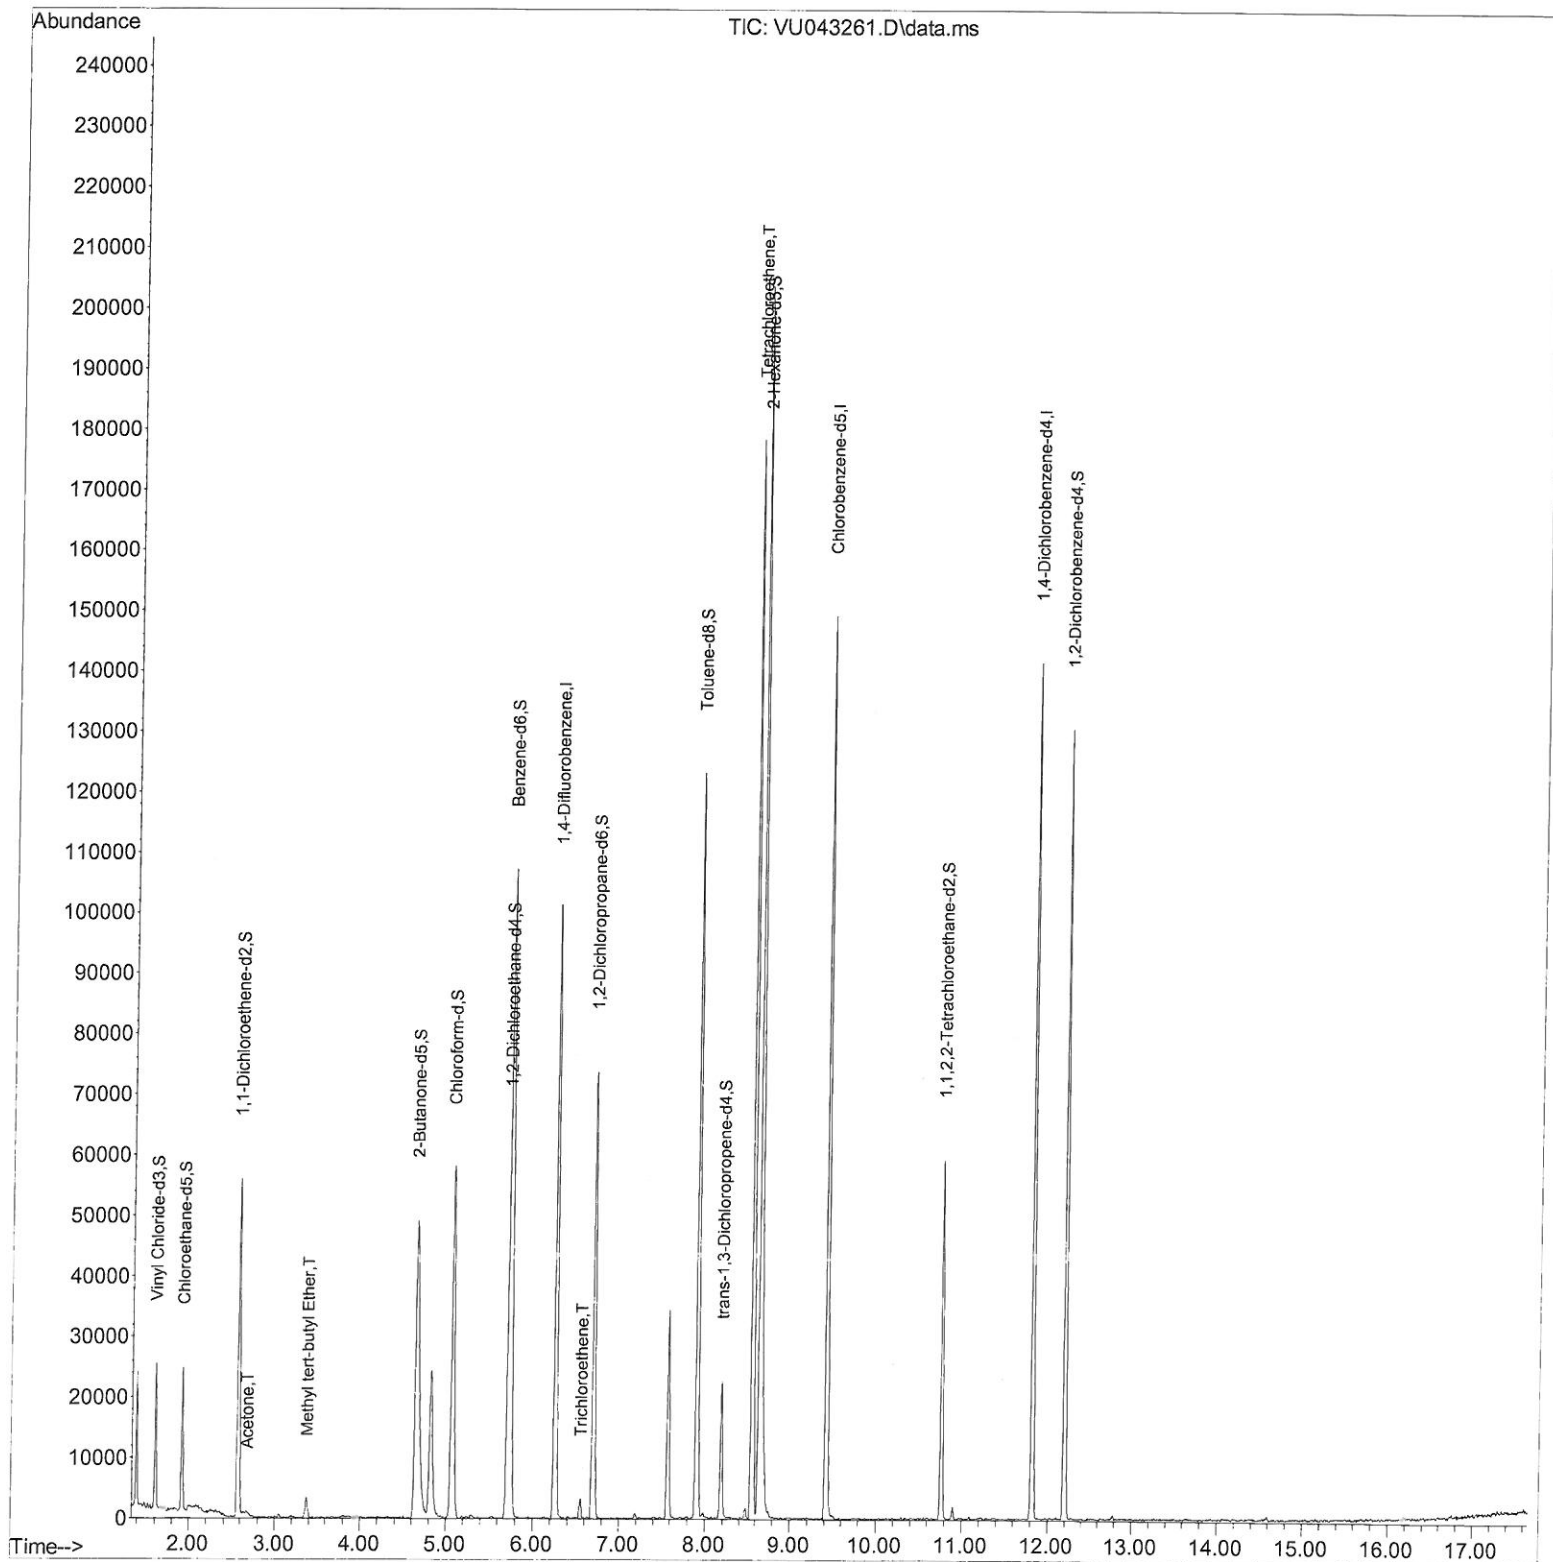



Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043261.D
 Acq On : 21 Apr 2021 19:31
 Operator : SY/MD
 Sample : M2088-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4489

Manual Integrations
 APPROVED

MMDadoda
 4/23/2021 2:47:32 PM

Quant Time: Apr 22 04:46:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 22 04:40:57 2021
 Response via : Initial Calibration

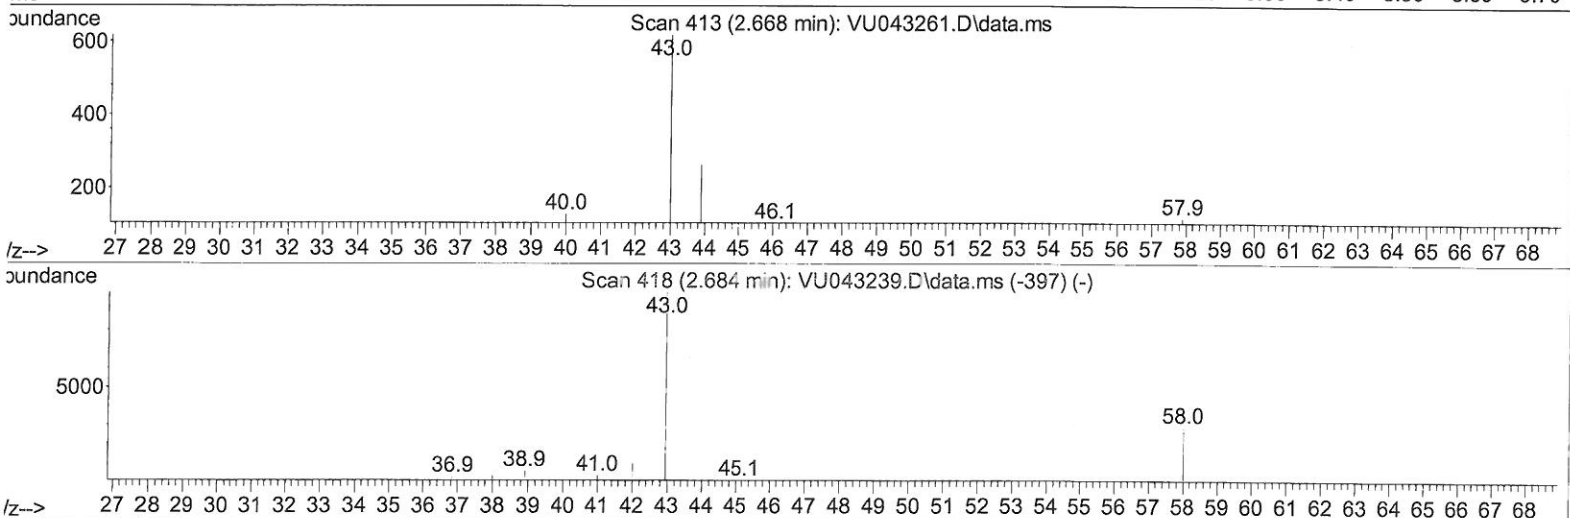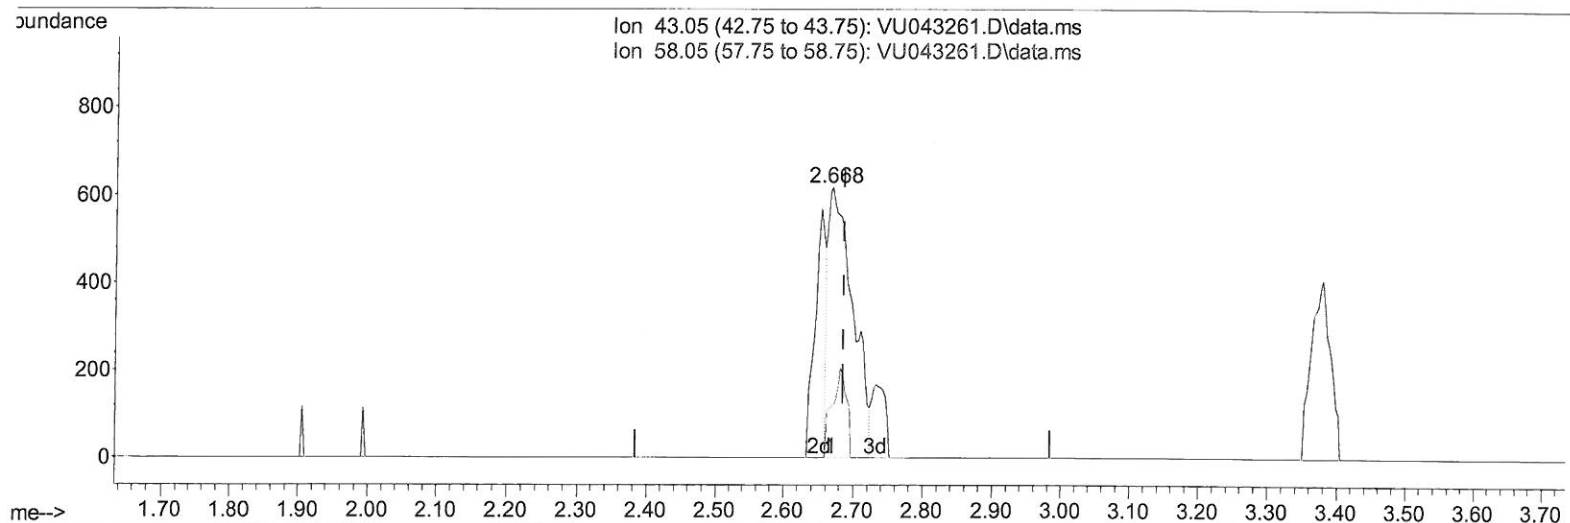

TIC: VU043261.D\data.ms

(13) Acetone (T)

2.668min (-0.017) 1.28 ug/L

response 1530

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.50	19.54
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043261.D
 Acq On : 21 Apr 2021 19:31
 Operator : SY/MD
 Sample : M2088-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4489

Manual Integrations
 APPROVED

MMDadoda
 4/23/2021 2:47:32 PM

Quant Time: Apr 22 04:46:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 22 04:40:57 2021
 Response via : Initial Calibration

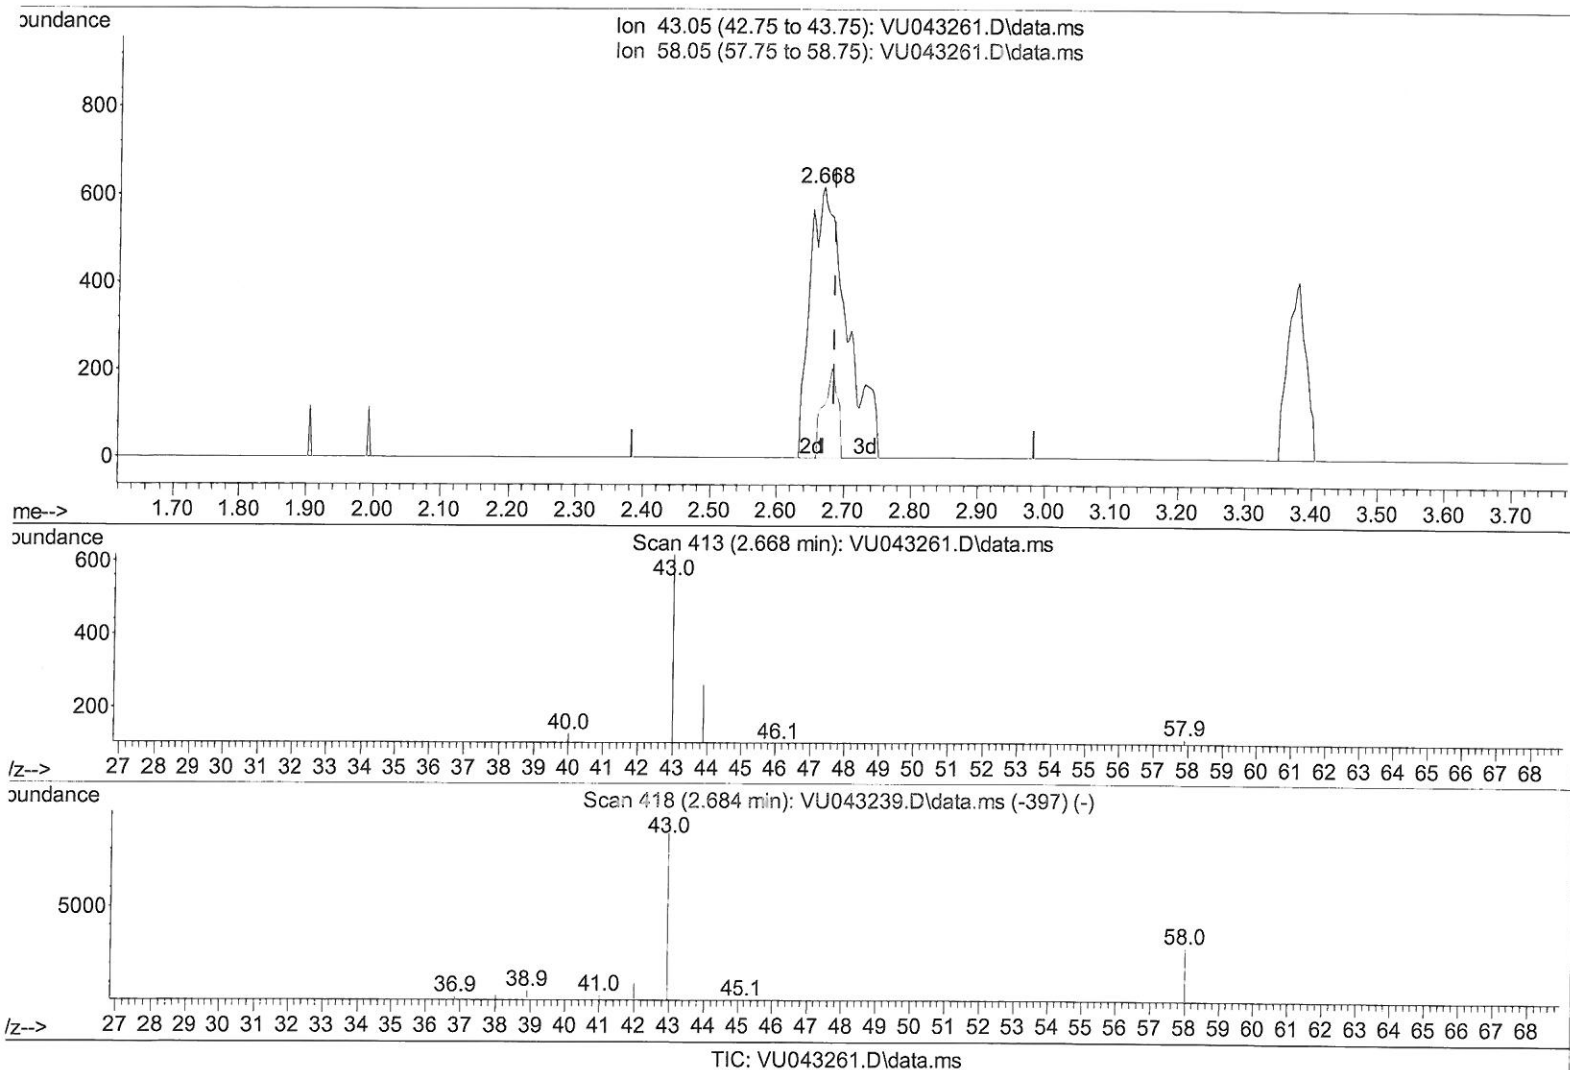

(13) Acetone (T)

2.668min (-0.017) 1.96 ug/L m

response 2343

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.50	12.76
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 4/27/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043261.D
 Acq On : 21 Apr 2021 19:31
 Operator : SY/MD
 Sample : M2088-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 H4489

Manual Integrations
 APPROVED

MMDadoda
 4/23/2021 2:47:32 PM

Quant Time: Apr 22 04:46:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 Last Update : Thu Apr 22 04:40:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	73033	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	74185	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	34753	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	16171	4.35	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.00%	
7) Chloroethane-d5	1.919	69	15529	4.44	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.80%	
11) 1,1-Dichloroethene-d2	2.575	65	10628	4.94	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	98.80%	
20) 2-Butanone-d5	4.648	46	103103	63.30	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	126.60%	
24) Chloroform-d	5.073	84	49972	5.29	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.80%	
26) 1,2-Dichloroethane-d4	5.713	65	33141	5.19	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.80%	
32) Benzene-d6	5.735	84	88448	5.12	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.40%	
36) 1,2-Dichloropropane-d6	6.700	67	30933	5.40	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.00%	
41) Toluene-d8	7.906	98	76164	4.24	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.80%	
43) trans-1,3-Dichloroprop...	8.189	79	11743	4.64	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.80%	
46) 2-Hexanone-d5	8.645	63	62009	49.15	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.30%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	26499	5.26	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.20%	
66) 1,2-Dichlorobenzene-d4	12.201	152	30838	5.18	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.60%	
Target Compounds						
13) Acetone	2.668	43	2343m	1.96	ug/L	Qvalue
17) Methyl tert-butyl Ether	3.378	73	3005	0.23	ug/L	# 89
34) Trichloroethene	6.555	95	1074	0.20	ug/L	87
47) Tetrachloroethene	8.562	164	37057	8.56	ug/L	96

7170
 4/27/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed