

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043245.D
 Acq On : 21 Apr 2021 13:05
 Operator : SY/MD
 Sample : M2057-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4540

Quant Time: Apr 22 04:42:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 22 04:40:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	79823	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	79962	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	38744	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	18531	4.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.40%
7) Chloroethane-d5	1.919	69	17186	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.00%
11) 1,1-Dichloroethene-d2	2.575	65	11915	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.40%
20) 2-Butanone-d5	4.652	46	109506	61.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.02%
24) Chloroform-d	5.073	84	55505	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.60%
26) 1,2-Dichloroethane-d4	5.713	65	35708	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.735	84	97648	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
36) 1,2-Dichloropropane-d6	6.700	67	33012	5.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.00%
41) Toluene-d8	7.906	98	85997	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloroprop...	8.185	79	12488	4.58	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.60%
46) 2-Hexanone-d5	8.642	63	65700	48.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.62%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	28633	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.40%
66) 1,2-Dichlorobenzene-d4	12.201	152	34772	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%
Target Compounds						
14) Carbon disulfide	2.806	76	1008	0.09	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043245.D
Acq On : 21 Apr 2021 13:05
Operator : SY/MD
Sample : M2057-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4540

Quant Time: Apr 22 04:42:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 22 04:40:57 2021
Response via : Initial Calibration

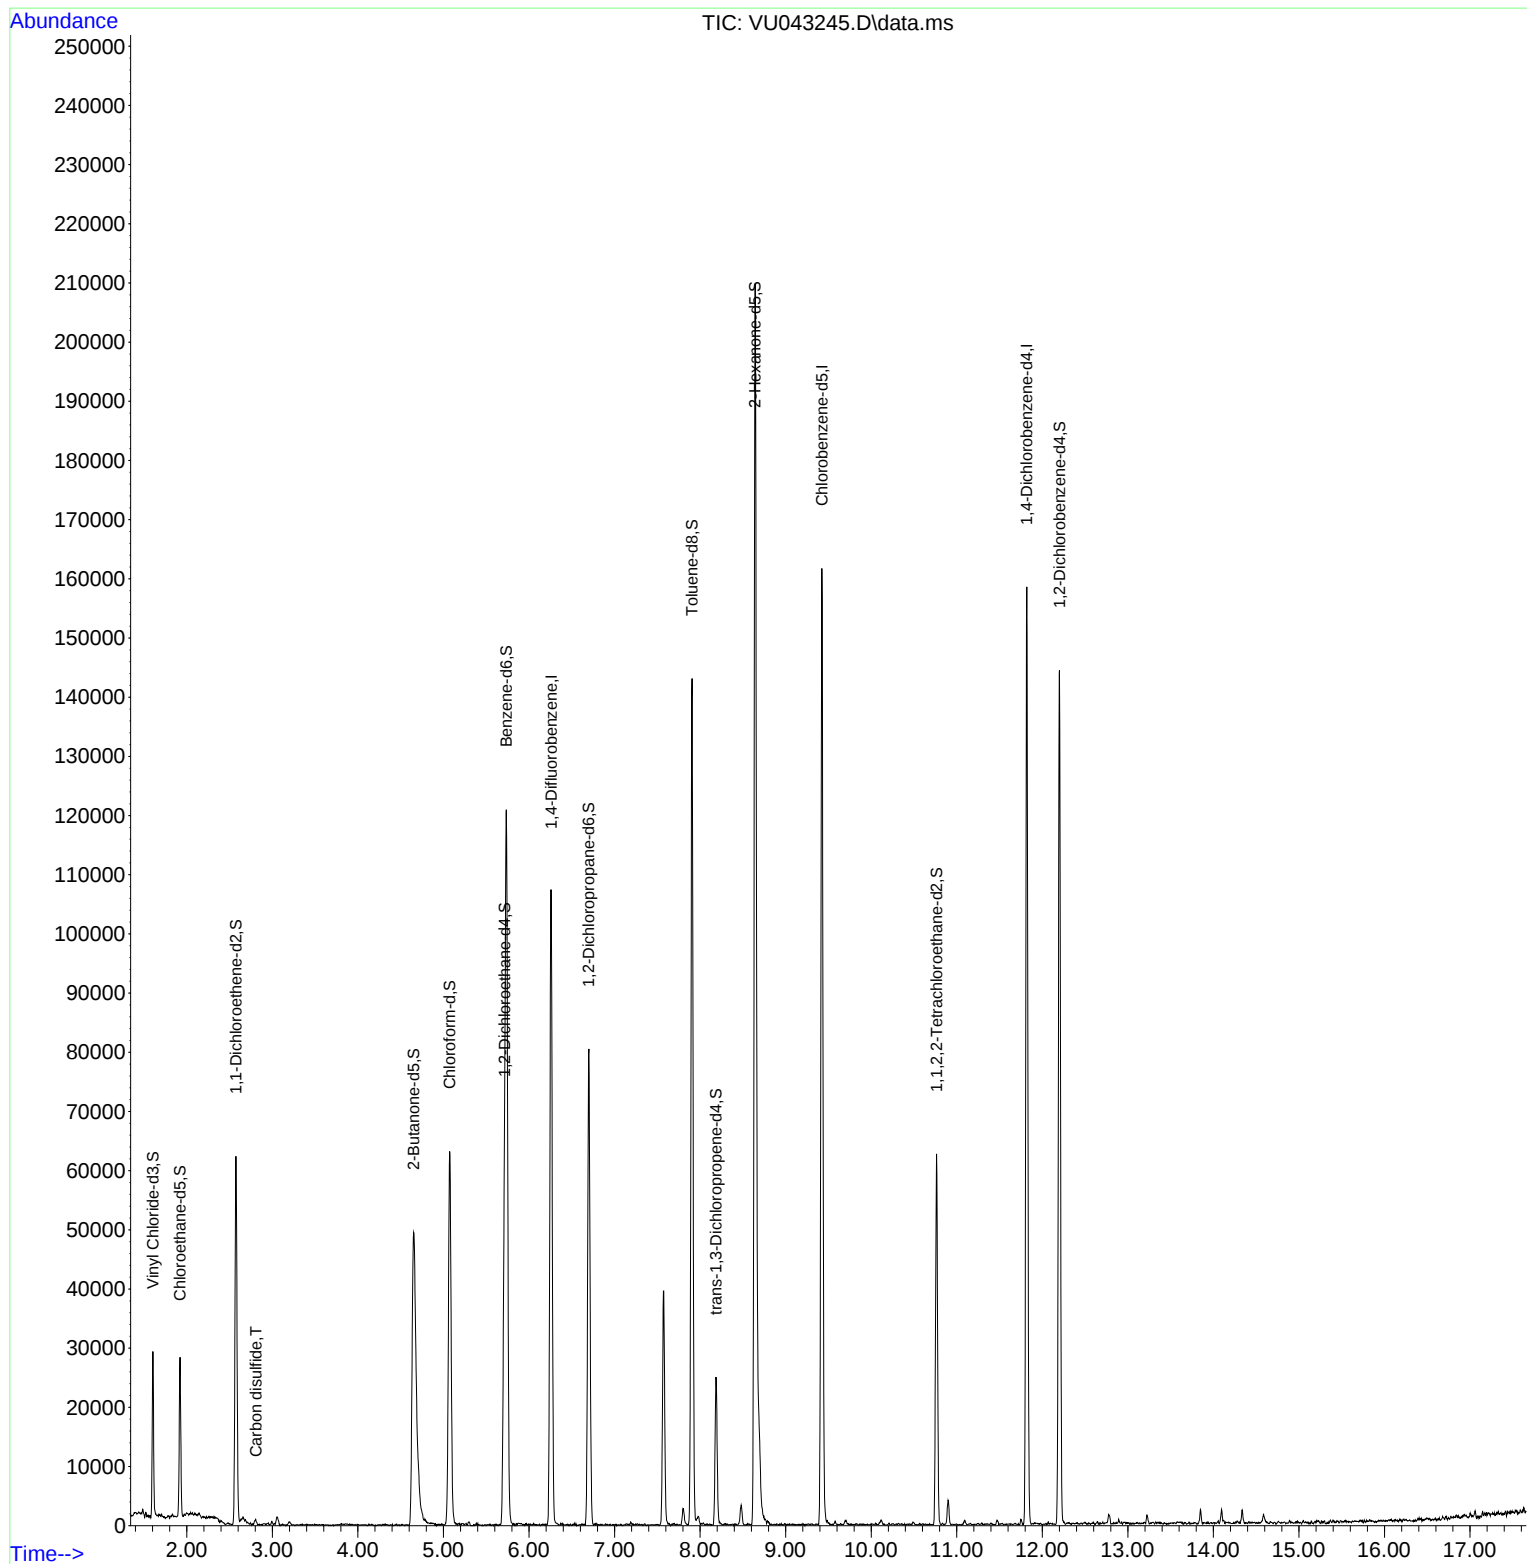

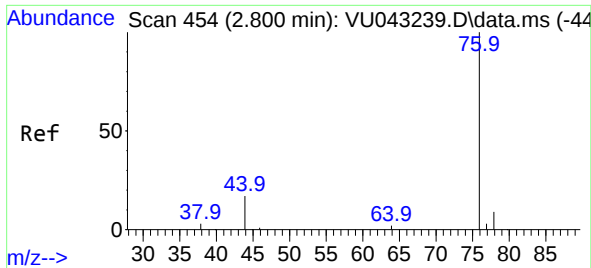

#14
Carbon disulfide
Concen: 0.09 ug/L
RT: 2.806 min Scan# 456
Delta R.T. 0.006 min
Lab File: VU043245.D
Acq: 21 Apr 2021 13:05

Instrument :
MSVOA_U
ClientSampleId :
H4540

Tgt Ion: 76 Resp: 1008
Ion Ratio Lower Upper
76 100
78 15.9 7.5 11.3#

