

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043254.D
 Acq On : 21 Apr 2021 16:44
 Operator : SY/MD
 Sample : M2088-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4490

Quant Time: Apr 22 04:43:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 22 04:40:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	80850	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	80871	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	38321	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	16276	3.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.20%
7) Chloroethane-d5	1.919	69	16876	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.575	65	10185	4.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.60%
20) 2-Butanone-d5	4.649	46	98259	54.49	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.98%
24) Chloroform-d	5.073	84	49950	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.713	65	32611	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
32) Benzene-d6	5.735	84	86337	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	6.700	67	30843	4.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.80%
41) Toluene-d8	7.906	98	76516	3.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.20%
43) trans-1,3-Dichloroprop...	8.185	79	11551	4.19	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.80%
46) 2-Hexanone-d5	8.645	63	61648	44.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.64%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	26475	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
66) 1,2-Dichlorobenzene-d4	12.201	152	31496	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%
Target Compounds						
13) Acetone	2.658	43	2521	1.90	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043254.D
Acq On : 21 Apr 2021 16:44
Operator : SY/MD
Sample : M2088-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4490

Quant Time: Apr 22 04:43:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 22 04:40:57 2021
Response via : Initial Calibration

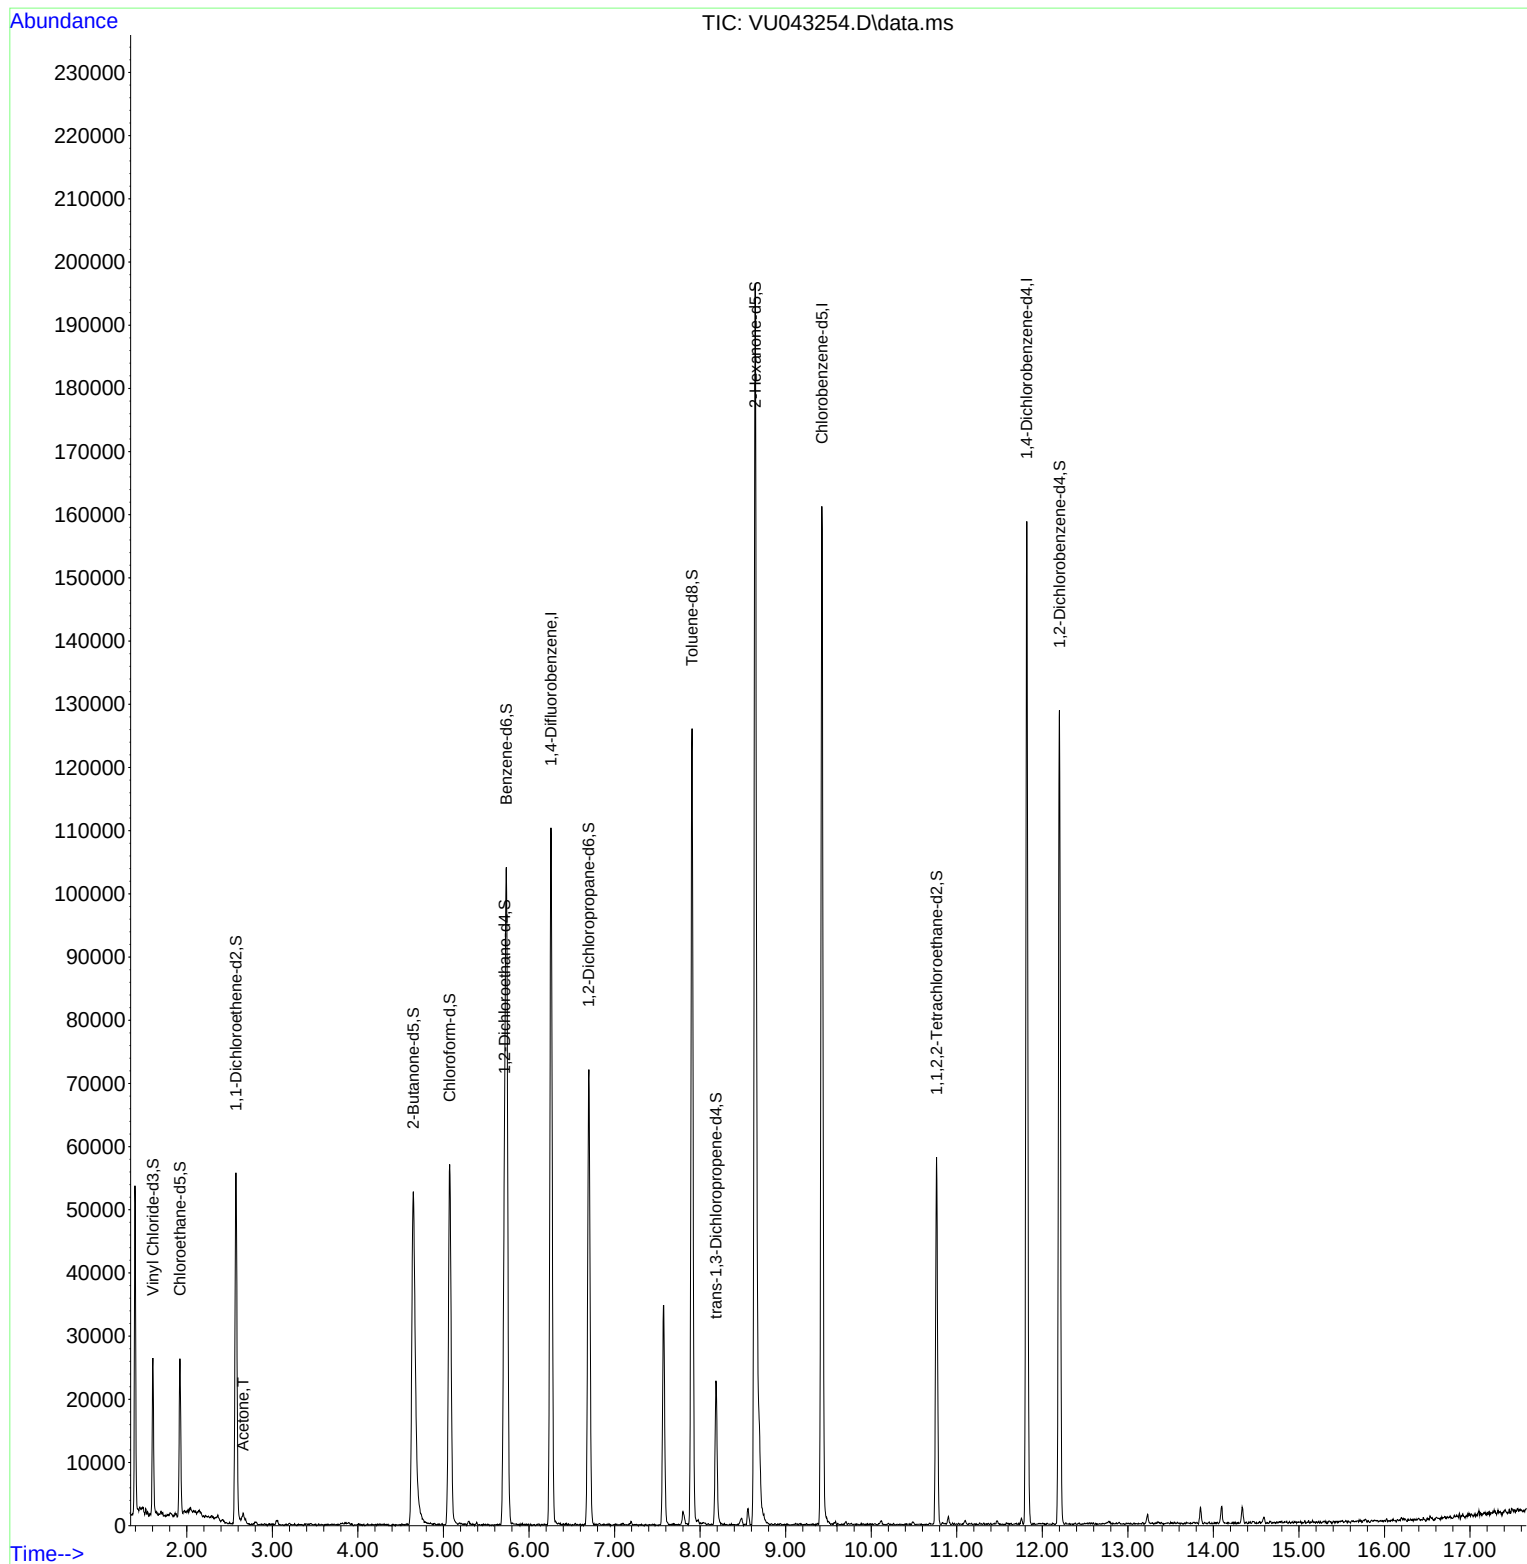

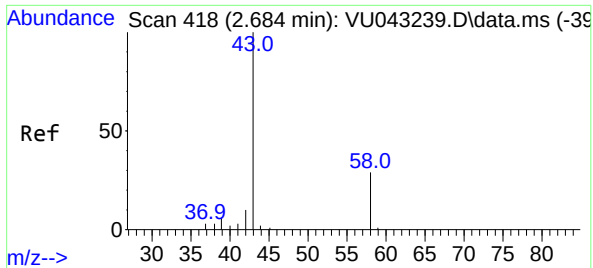

#13
 Acetone
 Concen: 1.90 ug/L
 RT: 2.658 min Scan# 410
 Delta R.T. -0.026 min
 Lab File: VU043254.D
 Acq: 21 Apr 2021 16:44

Instrument :
 MSVOA_U
 ClientSampleId :
 H4490

Tgt Ion: 43 Resp: 2521

Ion	Ratio	Lower	Upper
43	100		
58	16.3	0.0	25.0

