

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043262.D
 Acq On : 21 Apr 2021 19:55
 Operator : SY/MD
 Sample : M2088-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4501

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	10	17	26	rBV	75543	78678	19.18%	2.901%
2	1.604	74	82	93	rBV	26238	30783	7.50%	1.135%
3	1.919	171	180	192	rVB	24745	32926	8.03%	1.214%
4	2.575	372	384	398	rBV	59240	94974	23.15%	3.502%
5	4.662	1015	1033	1078	rBV2	36632	163140	39.76%	6.016%
6	5.073	1146	1161	1182	rBV	59192	131860	32.14%	4.862%
7	5.735	1347	1367	1387	rBV2	112301	293664	71.58%	10.829%
8	6.256	1515	1529	1546	rBV	100763	190634	46.47%	7.030%
9	6.700	1654	1667	1685	rVB	74049	142255	34.67%	5.246%
10	7.571	1927	1938	1953	rBV	35202	61802	15.06%	2.279%
11	7.906	2029	2042	2060	rBV	127967	216395	52.74%	7.980%
12	8.189	2120	2130	2143	rBV2	22407	38224	9.32%	1.410%
13	8.562	2236	2246	2257	rVB2	21135	34649	8.45%	1.278%
14	8.645	2257	2272	2304	rBV	196064	410267	100.00%	15.129%
15	9.423	2502	2514	2536	rBV	153561	252236	61.48%	9.301%
16	10.764	2915	2931	2945	rBV	60779	96616	23.55%	3.563%
17	11.819	3248	3259	3275	rBV	146805	229841	56.02%	8.475%
18	12.201	3365	3378	3393	rBV	132349	212921	51.90%	7.851%




Sum of corrected areas: 2711865

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043262.D
Acq On : 21 Apr 2021 19:55
Operator : SY/MD
Sample : M2088-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4501

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

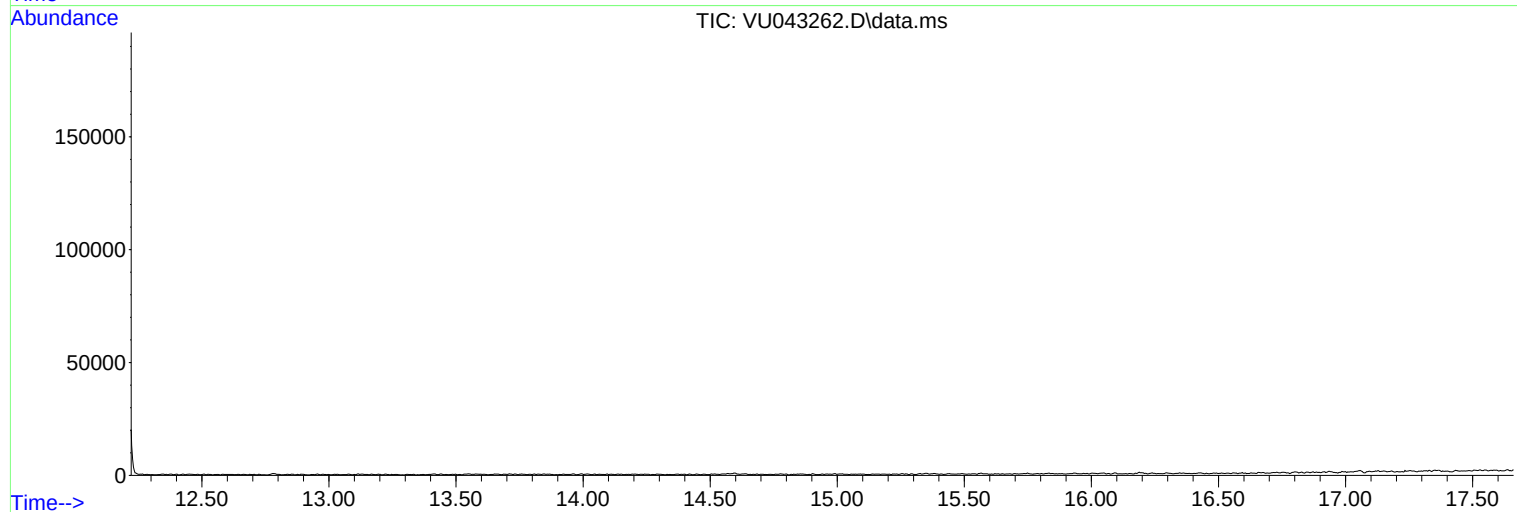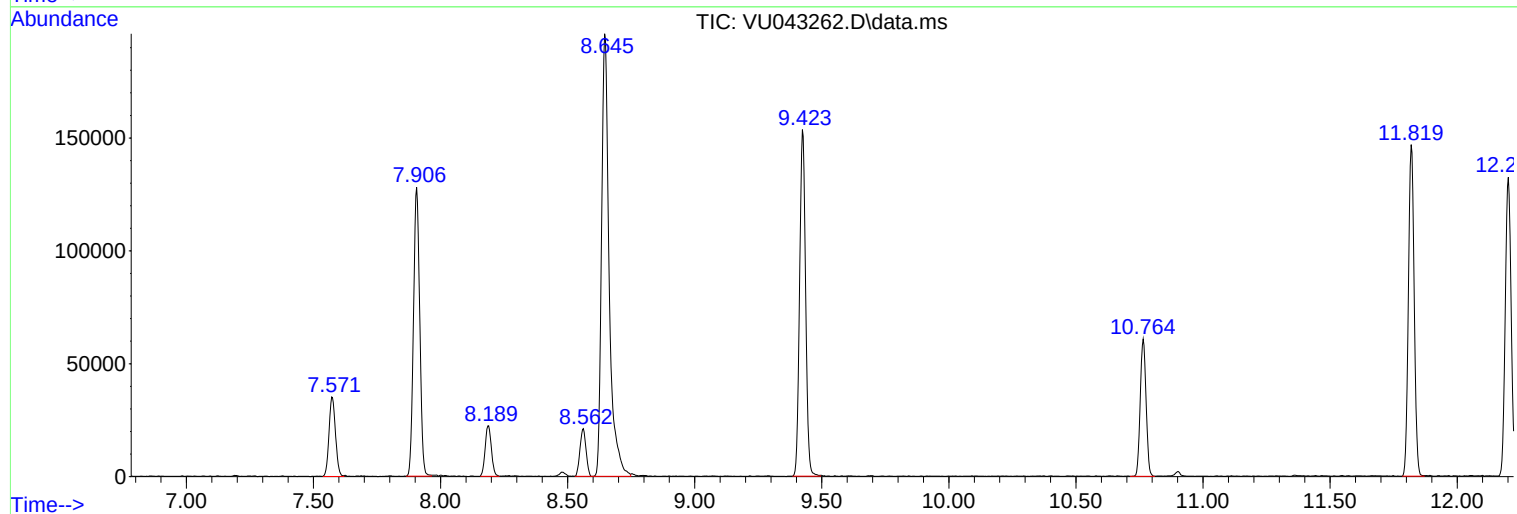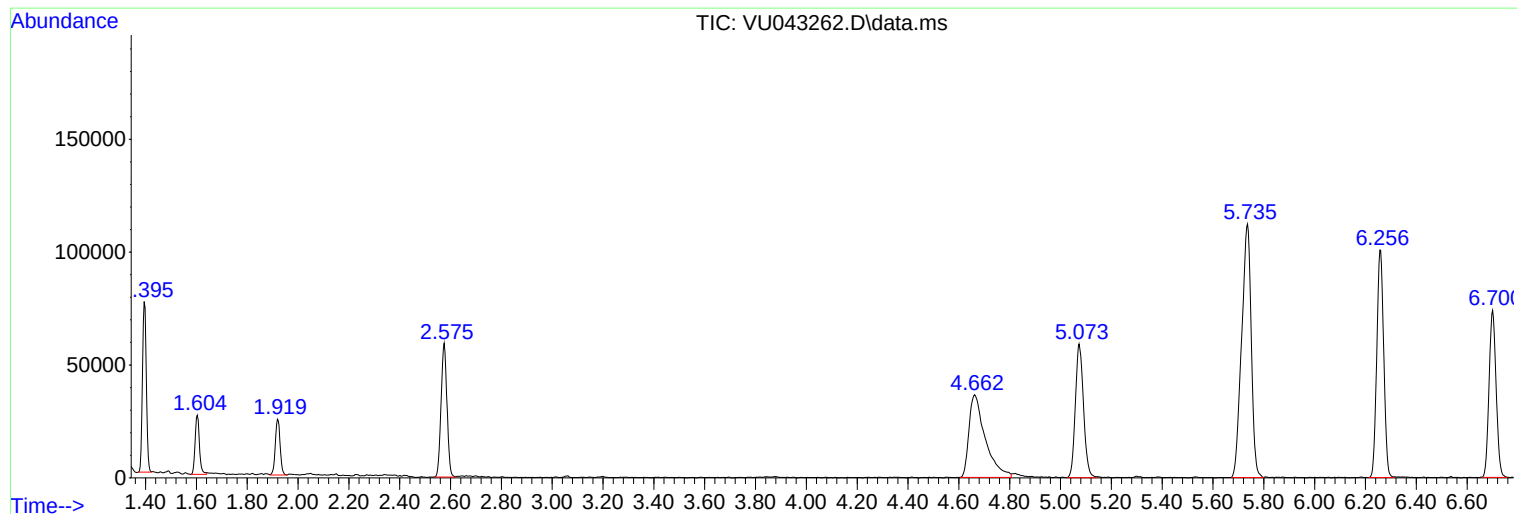

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043262.D
Acq On : 21 Apr 2021 19:55
Operator : SY/MD
Sample : M2088-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4501










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Difluorochloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.395	2.06 ug/L	78678	1,4-Difluorobenzene	6.260

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Difluorochloromethane	86	CHClF2	000075-45-6	91
2			Difluorochloromethane	86	CHClF2	000075-45-6	90
3			Propiolonitrile	51	C3HN	001070-71-9	4
4			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	4
5			2-p-Nitrobenzoyl-1,3,5-tribenzyl...	569	C33H31NO8	1000129-85-6	2

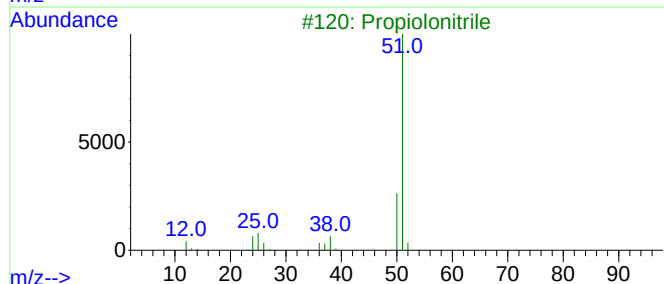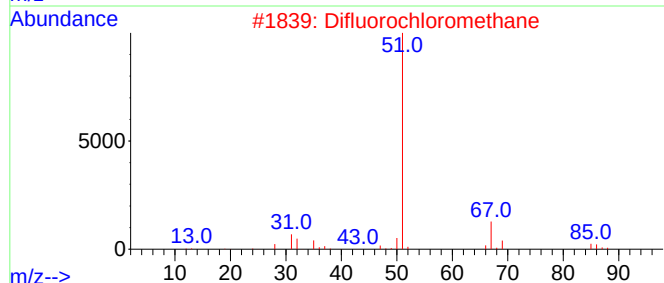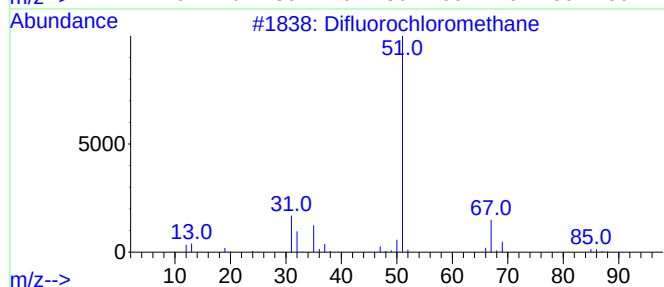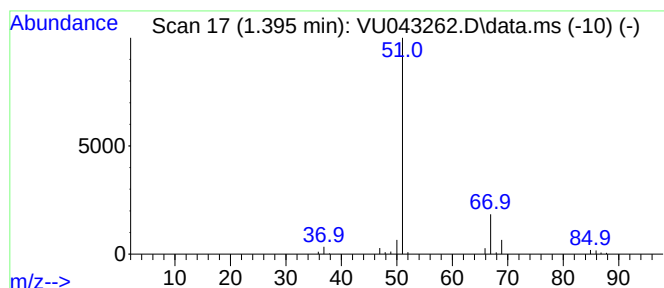

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043262.D
Acq On : 21 Apr 2021 19:55
Operator : SY/MD
Sample : M2088-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4501

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Difluorochlorom...	1.395	2.1	ug/L	78678	1	6.260	190634	5.0