

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043263.D
 Acq On : 21 Apr 2021 20:19
 Operator : SY/MD
 Sample : M2088-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4502

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	10	17	28	rVB	76351	80070	18.55%	2.894%
2	1.604	74	82	91	rBV	26599	29822	6.91%	1.078%
3	1.919	172	180	190	rBV	25665	32408	7.51%	1.171%
4	2.575	372	384	400	rBV2	60634	99154	22.97%	3.584%
5	4.662	1014	1033	1075	rBV2	40173	172729	40.02%	6.243%
6	5.073	1145	1161	1181	rBV	60640	136222	31.56%	4.924%
7	5.736	1345	1367	1387	rBV2	118293	306690	71.06%	11.085%
8	6.256	1515	1529	1548	rBV	97398	183122	42.43%	6.619%
9	6.700	1654	1667	1683	rVB	76485	148699	34.45%	5.375%
10	7.575	1927	1939	1956	rVB2	35858	64057	14.84%	2.315%
11	7.906	2027	2042	2058	rBV	131581	225206	52.18%	8.140%
12	8.186	2119	2129	2143	rBV2	23741	39992	9.27%	1.446%
13	8.559	2234	2245	2257	rVB3	20874	34692	8.04%	1.254%
14	8.645	2259	2272	2312	rBV	209000	431610	100.00%	15.601%
15	9.424	2502	2514	2537	rBV	144062	241379	55.93%	8.725%
16	10.764	2919	2931	2943	rBV	63744	100373	23.26%	3.628%
17	11.819	3248	3259	3272	rBV	138689	218086	50.53%	7.883%
18	12.202	3363	3378	3393	rBV	138884	222308	51.51%	8.035%




Sum of corrected areas: 2766619

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043263.D
Acq On : 21 Apr 2021 20:19
Operator : SY/MD
Sample : M2088-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4502

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

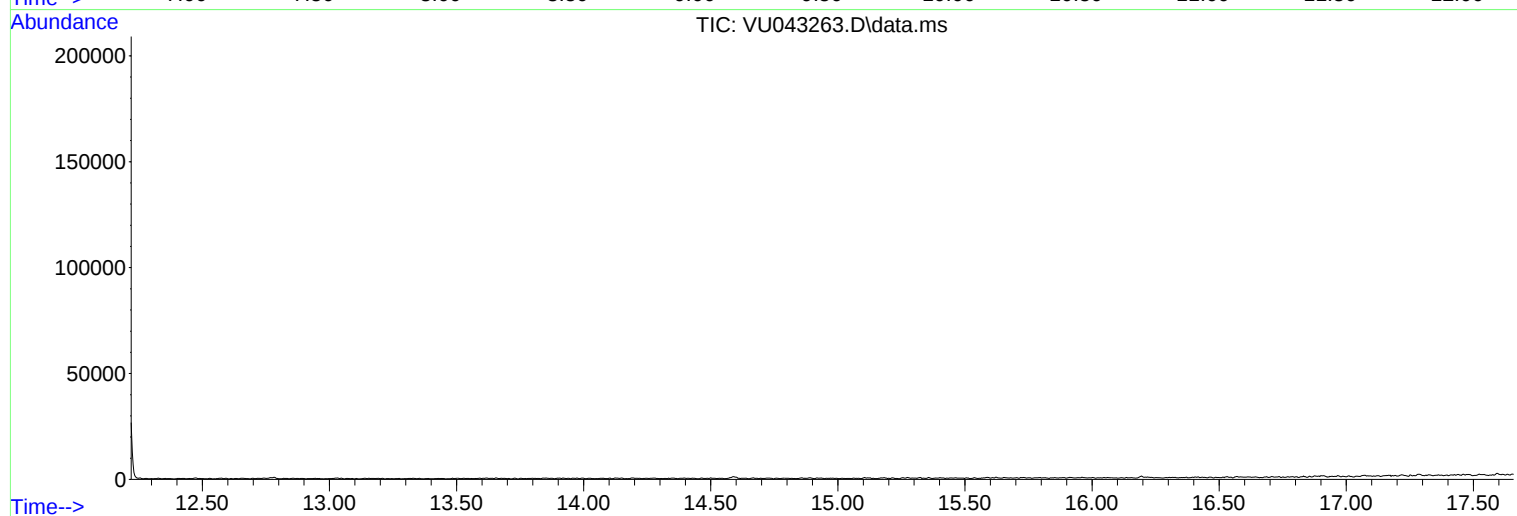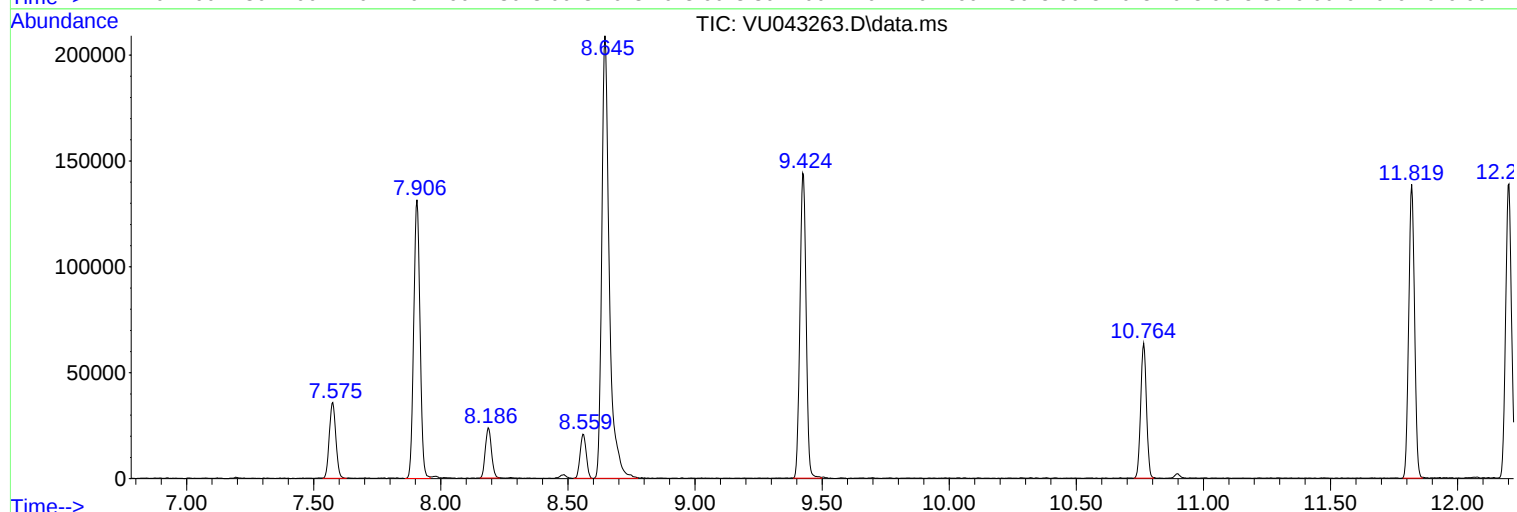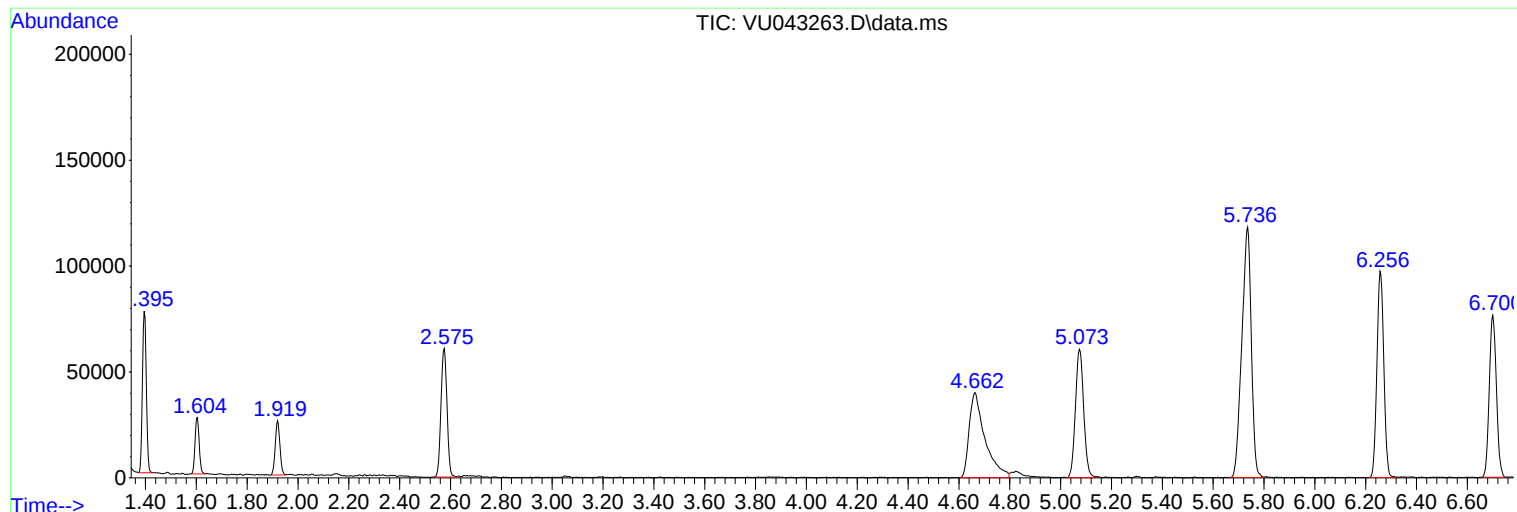

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043263.D
Acq On : 21 Apr 2021 20:19
Operator : SY/MD
Sample : M2088-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4502










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Difluorochloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.395	2.19 ug/L	80070	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Difluorochloromethane	86	CHClF2	000075-45-6	91
2			Difluorochloromethane	86	CHClF2	000075-45-6	74
3			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	7
4			Propiolonitrile	51	C3HN	001070-71-9	4
5			2-p-Nitrobenzoyl-1,3,5-tribenzyl...	569	C33H31NO8	1000129-85-6	2

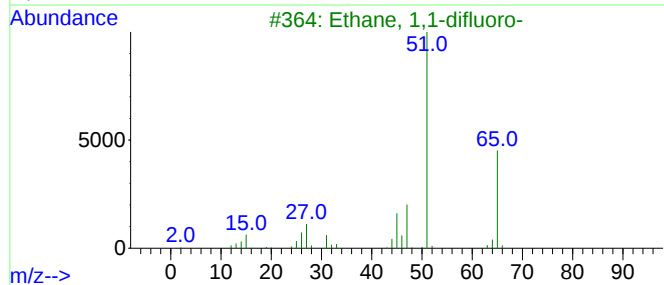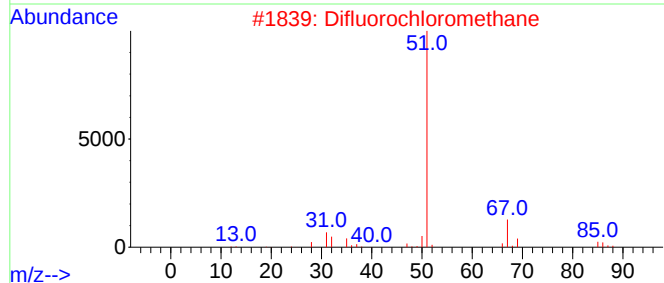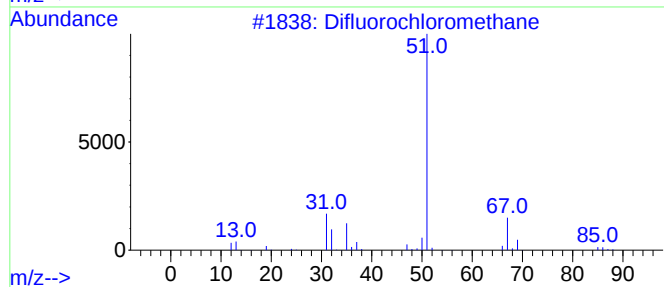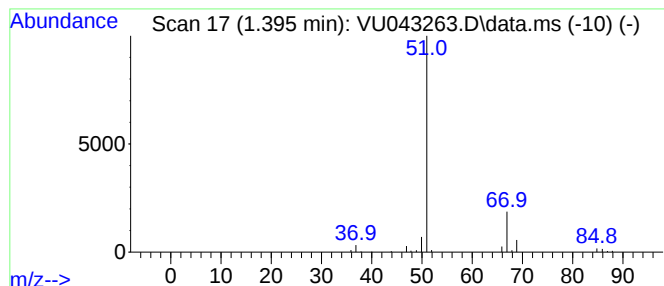

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
Data File : VU043263.D
Acq On : 21 Apr 2021 20:19
Operator : SY/MD
Sample : M2088-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4502

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Difluorochlorom...	1.395	2.2	ug/L	80070	1	6.256	183122	5.0