


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042121\
 Data File : VU043238.D
 Acq On : 21 Apr 2021 09:28
 Operator : SY/MD
 Sample : BFB33
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB133

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Apr 22 23:39:31 2021

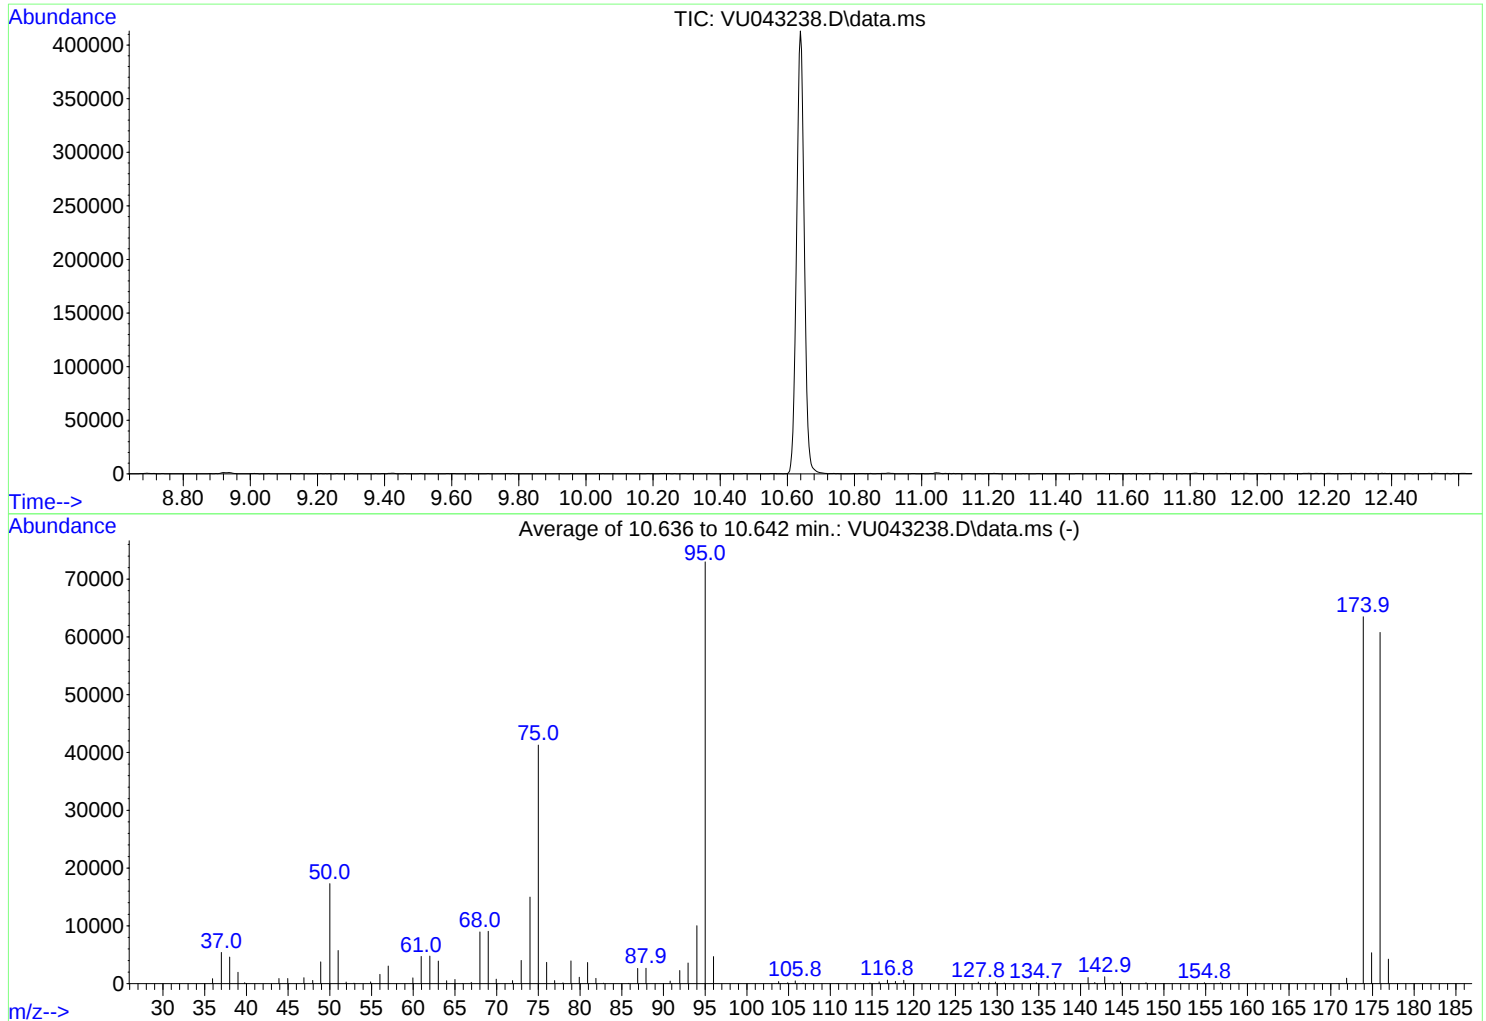

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	17307	PASS
75	95	30	80	56.6	41288	PASS
95	95	100	100	100.0	72995	PASS
96	95	5	9	6.4	4679	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.0	63488	PASS
175	174	5	9	8.4	5348	PASS
176	174	95	101	95.8	60792	PASS
177	176	5	9	7.0	4250	PASS

m/z	Abundance
43.80	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
36.00	885.0
37.00	5280.0
38.00	4775.0
39.00	1967.0
39.80	168.0
44.00	1096.0
44.90	920.0
46.90	1062.0
48.00	612.0
48.90	3621.0
50.00	17424.0
51.00	5739.0
52.00	300.0
52.90	114.0
54.90	318.0
56.00	1594.0
57.00	3007.0
59.90	908.0
60.90	4537.0
62.00	4709.0
63.00	3868.0
64.00	523.0
65.00	727.0
67.00	238.0
68.00	8767.0
69.00	8937.0
70.00	862.0
71.90	524.0
73.00	4085.0
74.00	15105.0
75.00	40528.0
76.00	3624.0
77.00	599.0
78.90	3898.0
79.90	1100.0
80.90	3724.0
81.90	893.0
82.80	112.0
86.90	2612.0
87.90	2755.0
90.80	368.0
91.90	2353.0
93.00	3476.0
94.00	9638.0
95.00	71704.0
96.00	4753.0
103.80	361.0
104.90	166.0
105.80	468.0
110.80	108.0
114.80	126.0
115.80	319.0
116.90	621.0
117.80	374.0
118.80	555.0
127.80	285.0
129.10	129.0
129.80	244.0
130.90	115.0
134.70	111.0
136.90	134.0
140.90	1058.0
141.70	197.0
142.90	1165.0
144.80	263.0
147.90	169.0
154.80	198.0
156.80	120.0
170.90	102.0
171.90	976.0
173.90	60728.0
174.90	5238.0
175.90	58464.0
176.90	4215.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
36.00	868.0
37.00	5536.0
38.00	4777.0
39.00	2002.0
39.80	182.0
43.90	1053.0
44.90	909.0
46.90	1098.0
48.00	539.0
48.90	3853.0
50.00	17776.0
51.00	5959.0
52.00	283.0
52.90	113.0
54.90	335.0
56.00	1686.0
57.00	3173.0
59.90	1054.0
61.00	4804.0
62.00	4893.0
63.00	4016.0
64.00	538.0
65.00	748.0
65.90	113.0
67.00	231.0
68.00	9285.0
69.00	9324.0
70.00	817.0
71.90	534.0
72.90	4141.0
74.00	15449.0
75.00	42576.0
76.00	3840.0
76.90	554.0
78.00	207.0
78.90	4062.0
79.90	1123.0
80.90	3697.0
81.90	940.0
82.80	120.0
85.80	103.0
86.90	2714.0
87.90	2785.0
90.80	474.0
91.90	2344.0
92.90	3622.0
94.00	10412.0
95.00	75632.0
96.00	4869.0
103.80	379.0
104.90	195.0
105.80	476.0
106.70	112.0
114.70	115.0
115.90	309.0
116.90	635.0
117.80	378.0
118.80	624.0
127.80	286.0
129.10	123.0
129.80	276.0
130.80	123.0
134.70	175.0
136.90	176.0
140.90	1063.0
141.70	206.0
142.90	1220.0
143.80	112.0
144.80	320.0
147.90	178.0
154.80	173.0
156.80	141.0
158.90	119.0
161.00	107.0
171.90	976.0
173.90	65368.0
174.90	5467.0
175.90	62664.0
176.90	4432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
35.90	856.0
37.00	5348.0
38.00	4199.0
39.00	1951.0
39.80	178.0
43.90	963.0
45.00	823.0
46.90	941.0
47.90	482.0
48.90	3819.0
50.00	16720.0
51.00	5519.0
51.90	288.0
54.90	267.0
56.00	1590.0
57.00	2927.0
60.00	1039.0
61.00	4751.0
62.00	4691.0
63.00	3797.0
64.00	456.0
65.00	683.0
66.90	228.0
68.00	8765.0
69.00	8928.0
69.90	664.0
71.90	510.0
72.90	3842.0
74.00	14413.0
75.00	40760.0
76.00	3551.0
76.90	444.0
77.90	204.0
78.90	3806.0
79.90	1077.0
80.90	3578.0
81.90	895.0
85.80	102.0
86.90	2556.0
87.90	2469.0
90.80	478.0
92.00	2157.0
92.90	3582.0
94.00	9992.0
95.00	71648.0
96.00	4415.0
103.80	380.0
104.90	183.0
105.80	440.0
106.80	107.0
114.70	104.0
115.90	285.0
116.80	614.0
117.80	384.0
118.80	615.0
127.70	285.0
128.90	145.0
129.80	291.0
130.80	134.0
134.70	219.0
136.80	165.0
140.90	1021.0
141.70	179.0
142.90	1211.0
143.80	113.0
144.80	298.0
147.80	187.0
150.00	116.0
154.90	157.0
156.80	166.0
158.90	134.0
161.00	123.0
171.90	891.0
173.90	64368.0
174.90	5340.0
175.90	61248.0
176.90	4103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133