




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048168.D
 Acq On : 21 Apr 2022 13:25
 Operator : SY/MD
 Sample : N2486-11 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J44

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 01:49:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 01:48:00 2022
 Response via : Initial Calibration

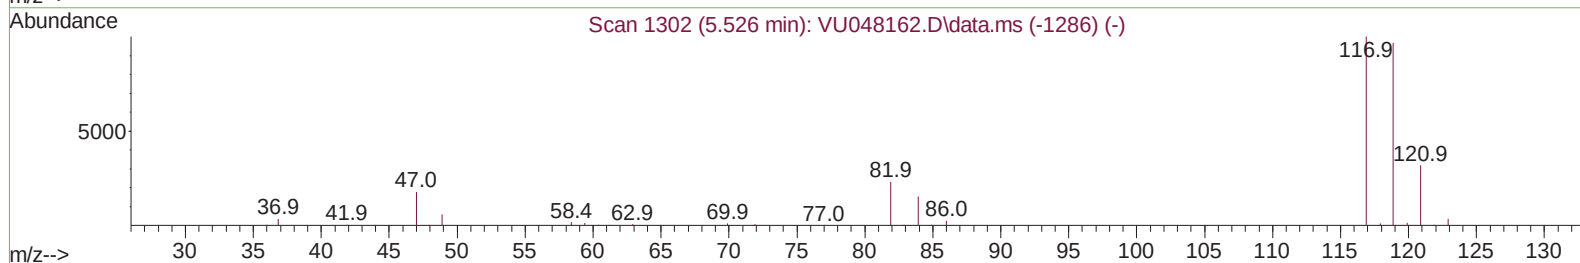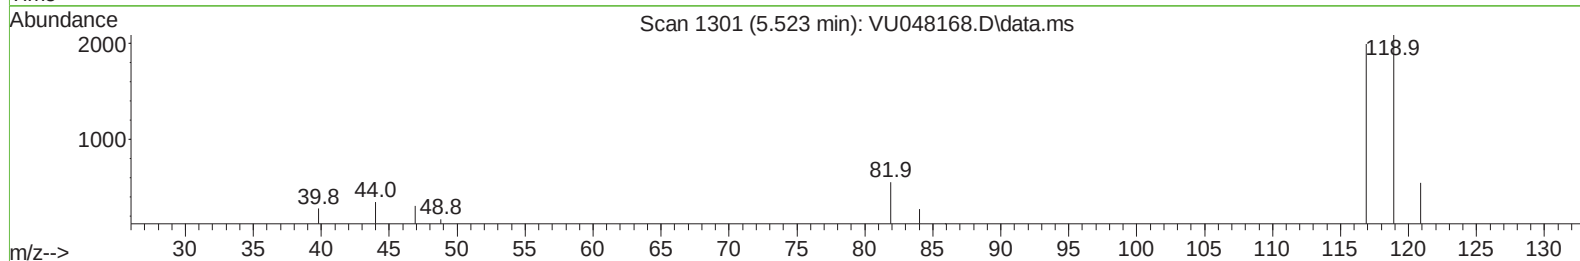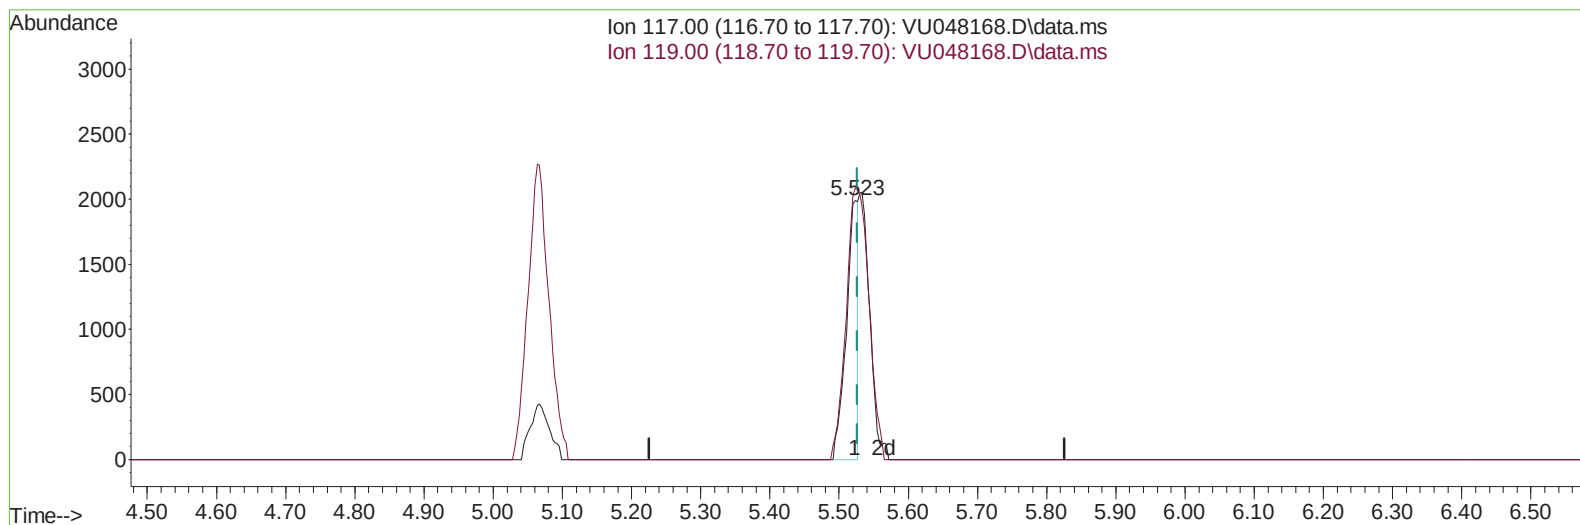

TIC: VU048168.D\data.ms

(31) Carbon tetrachloride (T)

5.523min (-0.003) 0.65 ug/L

response 2314

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	96.50	206.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048168.D
 Acq On : 21 Apr 2022 13:25
 Operator : SY/MD
 Sample : N2486-11 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J44

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 01:49:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 01:48:00 2022
 Response via : Initial Calibration

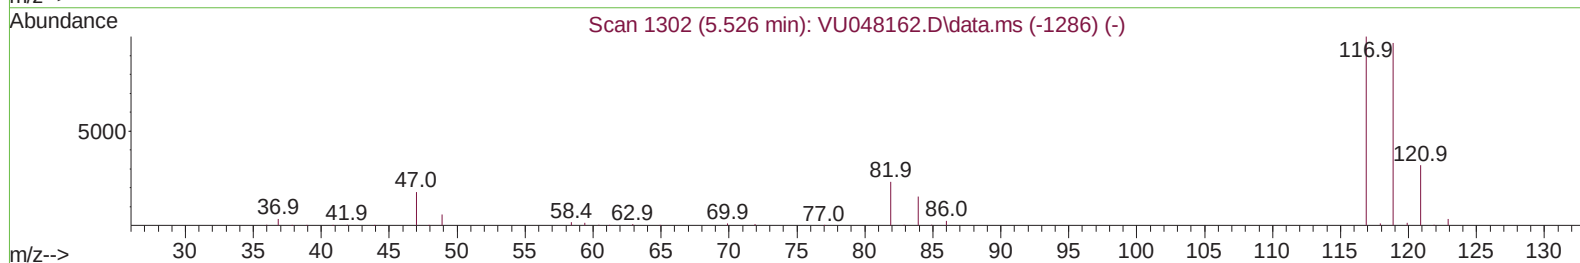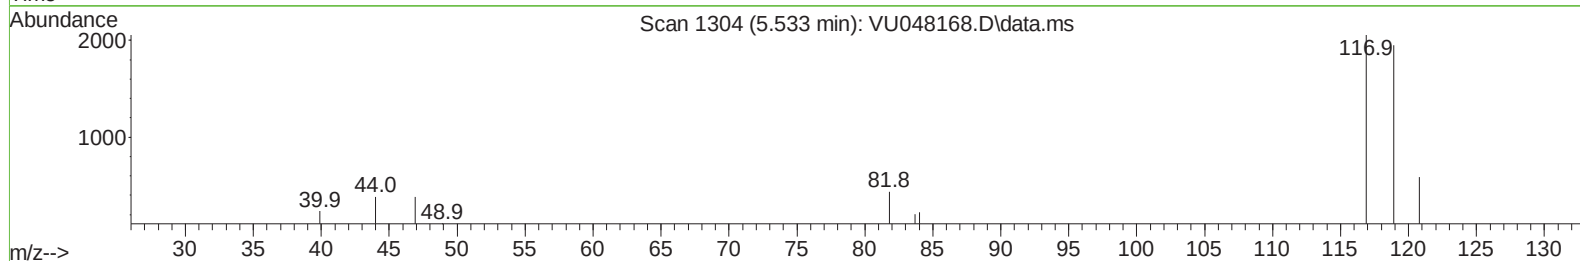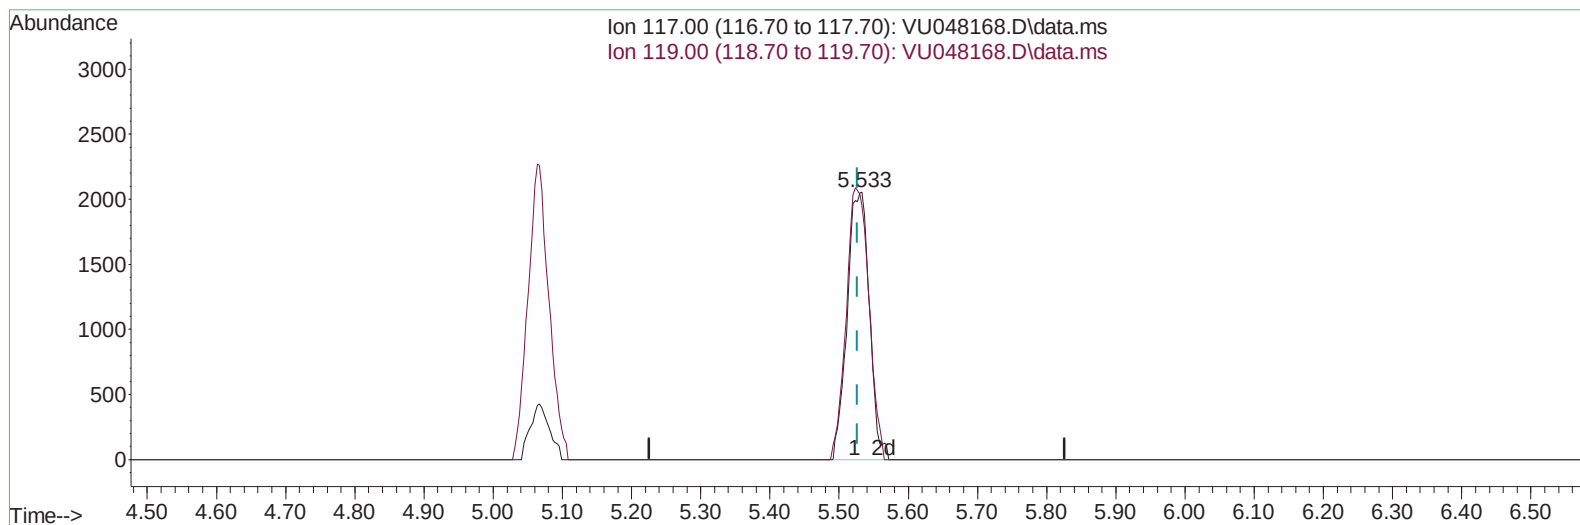

TIC: VU048168.D\data.ms

(31) Carbon tetrachloride (T)

5.533min (+ 0.007) 1.29 ug/L m

response 4573

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	96.50	104.26
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048168.D
 Acq On : 21 Apr 2022 13:25
 Operator : SY/MD
 Sample : N2486-11 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J44

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:49:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 01:48:00 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	345355	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	347040	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	177057	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	106773	42.634	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	85.260%	
7) Chloroethane-d5	1.916	69	90960	46.062	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	92.120%	
11) 1,1-Dichloroethene-d2	2.568	63	139950	30.543	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	61.080%	
21) 2-Butanone-d5	4.629	46	196775	91.541	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.540%	
24) Chloroform-d	5.067	84	203903	44.497	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.000%	
26) 1,2-Dichloroethane-d4	5.703	65	127030	45.199	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.400%	
32) Benzene-d6	5.729	84	410799	47.043	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.080%	
36) 1,2-Dichloropropane-d6	6.690	67	135617	50.569	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	101.140%	
41) Toluene-d8	7.899	98	352680	41.453	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.900%	
43) trans-1,3-Dichloroprop...	8.179	79	51913	38.209	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	76.420%	
47) 2-Hexanone-d5	8.636	63	133041	84.742	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	84.740%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	206223	44.807	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	89.620%	
66) 1,2-Dichlorobenzene-d4	12.192	152	160000	50.793	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	101.580%	
Target Compounds						
					Qvalue	
31) Carbon tetrachloride	5.533	117	4573m	1.287	ug/L	
33) Benzene	5.777	78	7946616	791.089	ug/L	100
51) Chlorobenzene	9.449	112	4840714	646.827	ug/L	97
64) 1,3-Dichlorobenzene	11.745	146	46546	8.751	ug/L	99
65) 1,4-Dichlorobenzene	11.835	146	1024230	185.918	ug/L	99
67) 1,2-Dichlorobenzene	12.211	146	738986	138.859	ug/L	100
70) 1,2,4-trichlorobenzene	13.841	180	53493	14.139	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048168.D
Acq On : 21 Apr 2022 13:25
Operator : SY/MD
Sample : N2486-11 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J44

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 01:49:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 22 01:48:00 2022
Response via : Initial Calibration

