




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048207.D
 Acq On : 22 Apr 2022 06:22
 Operator : SY/MD
 Sample : N2488-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1

Manual IntegrationsAPPROVED

Quant Time: Apr 22 07:43:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

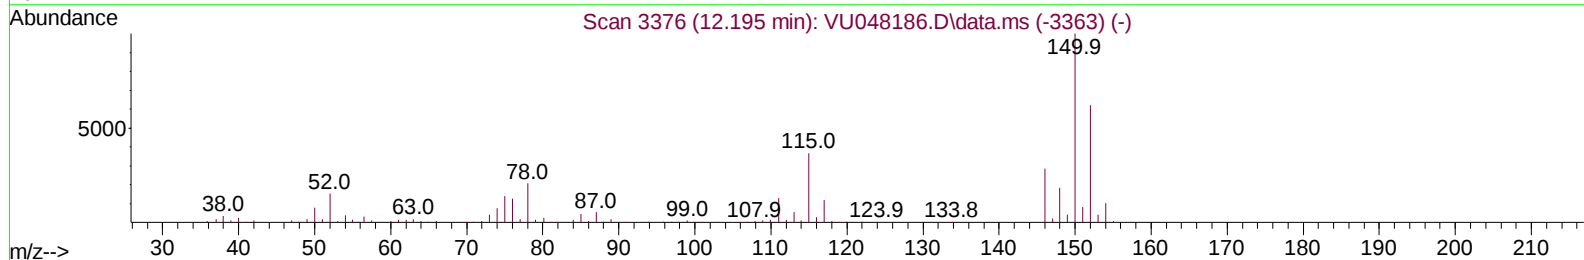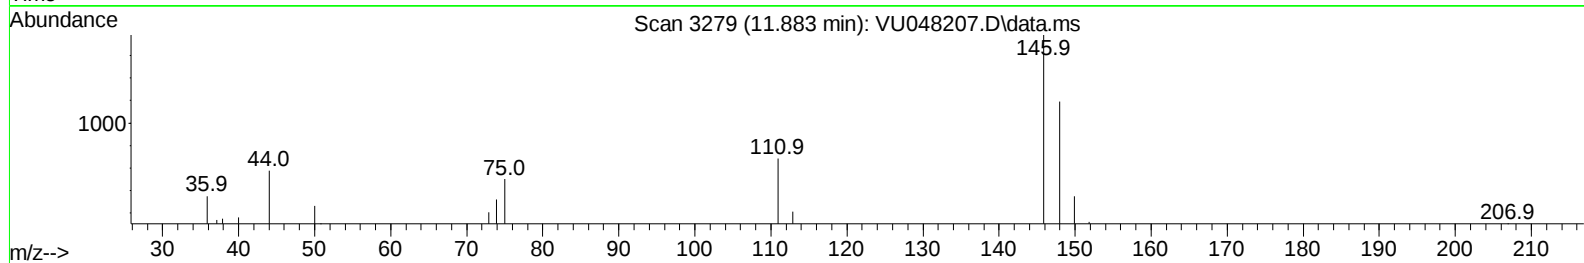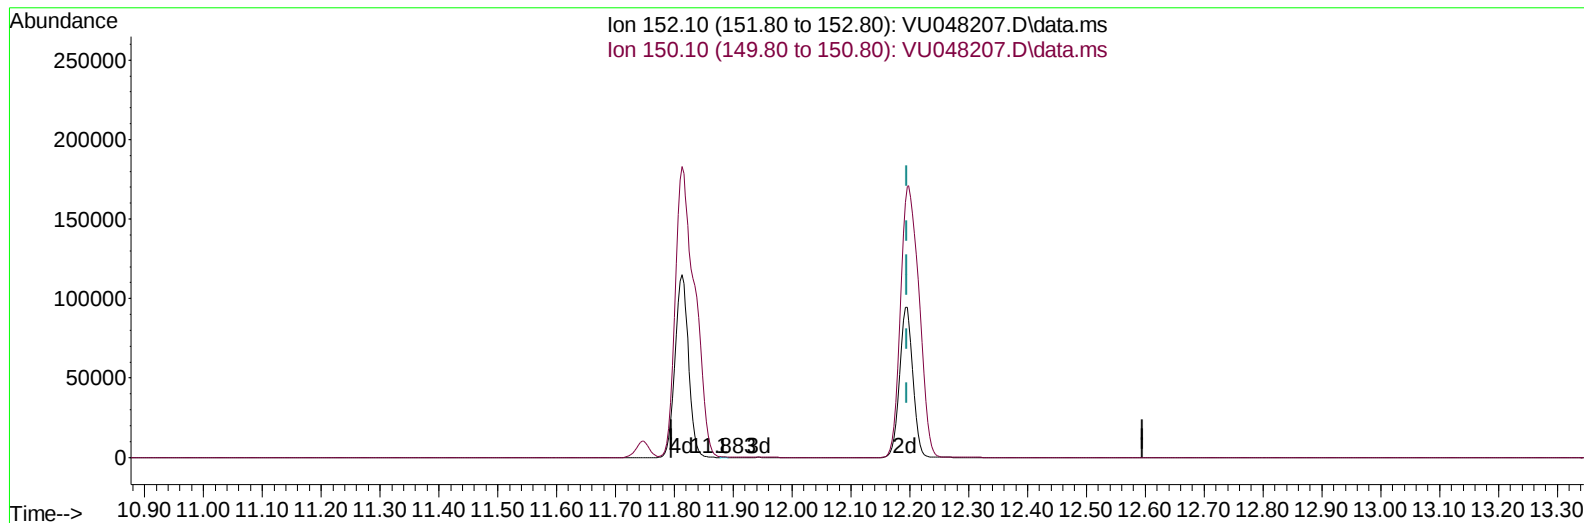

TIC: VU048207.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.883min (-0.312) 0.02 ug/L

response 65

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	171.40	183.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048207.D
 Acq On : 22 Apr 2022 06:22
 Operator : SY/MD
 Sample : N2488-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1

Manual IntegrationsAPPROVED

Quant Time: Apr 22 07:43:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

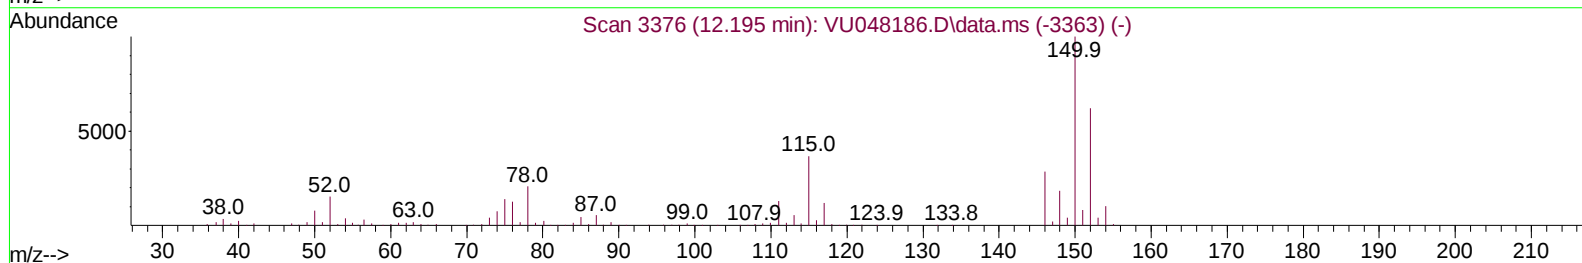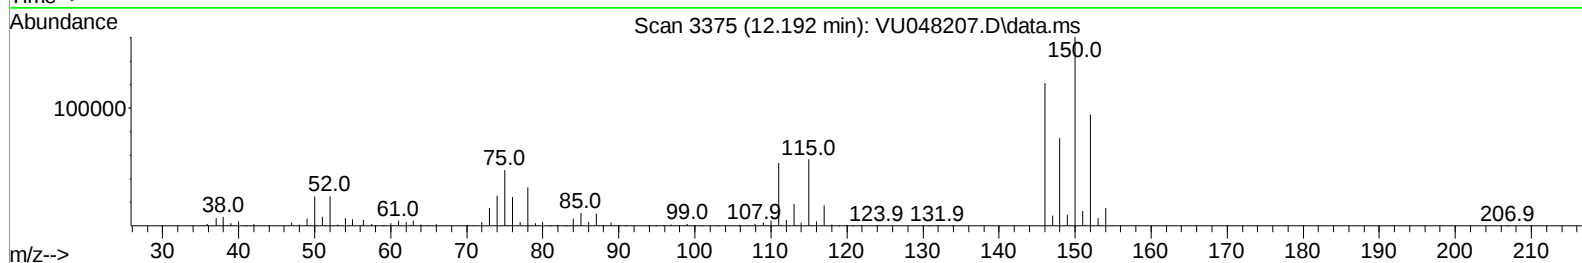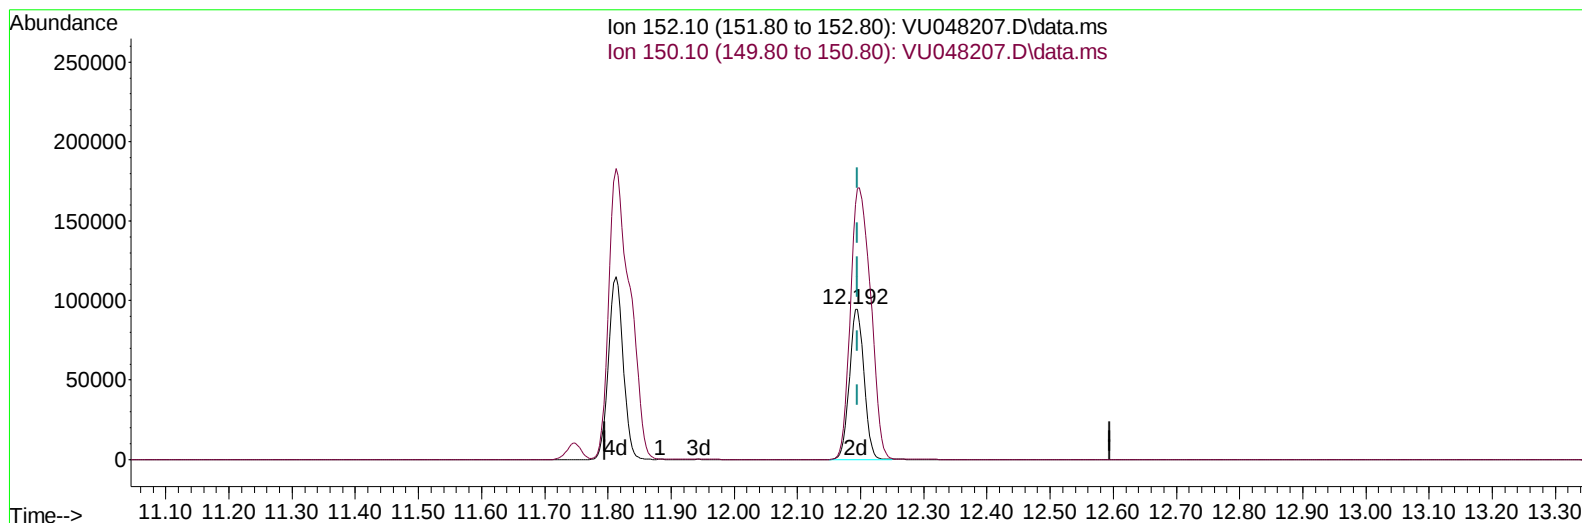

TIC: VU048207.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

12.192min (-0.003) 45.97 ug/L m

response 151757

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	171.40	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048207.D
 Acq On : 22 Apr 2022 06:22
 Operator : SY/MD
 Sample : N2488-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 07:43:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	335741	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	344705	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	185565	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	88161	36.211	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	72.420%	
7) Chloroethane-d5	1.916	69	76210	39.698	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	79.400%	
11) 1,1-Dichloroethene-d2	2.569	63	122020	27.393	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	54.780%#	
21) 2-Butanone-d5	4.620	46	186468	89.230	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	89.230%	
24) Chloroform-d	5.067	84	187605	42.113	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.220%	
26) 1,2-Dichloroethane-d4	5.703	65	117895	43.150	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.300%	
32) Benzene-d6	5.729	84	378952	43.690	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.380%	
36) 1,2-Dichloropropane-d6	6.691	67	126703	47.565	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	95.140%	
41) Toluene-d8	7.899	98	320594	37.937	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	75.880%#	
43) trans-1,3-Dichloroprop...	8.179	79	48124	35.660	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.320%	
47) 2-Hexanone-d5	8.633	63	119592	76.692	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	76.690%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	198165	43.348	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	86.700%	
66) 1,2-Dichlorobenzene-d4	12.192	152	151757m	45.968	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	91.940%	
Target Compounds						
					Qvalue	
31) Carbon tetrachloride	5.527	117	4299	1.218	ug/L	100
33) Benzene	5.777	78	982240	98.445	ug/L	100
51) Chlorobenzene	9.449	112	3166097	425.927	ug/L	99
64) 1,3-Dichlorobenzene	11.745	146	158228	28.386	ug/L	99
65) 1,4-Dichlorobenzene	11.838	146	1376345	238.379	ug/L	99
67) 1,2-Dichlorobenzene	12.211	146	1383249	248.003	ug/L	99
70) 1,2,4-trichlorobenzene	13.841	180	265262	66.896	ug/L	99
72) 1,2,3-Trichlorobenzene	14.330	180	71553	18.000	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048207.D
Acq On : 22 Apr 2022 06:22
Operator : SY/MD
Sample : N2488-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 07:43:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 22 02:51:38 2022
Response via : Initial Calibration

