




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048208.D
 Acq On : 22 Apr 2022 06:46
 Operator : SY/MD
 Sample : N2488-10 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 07:43:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

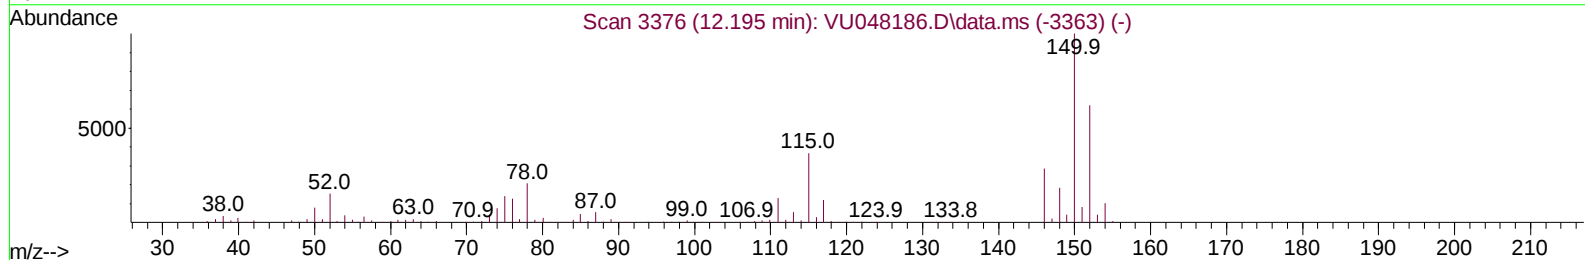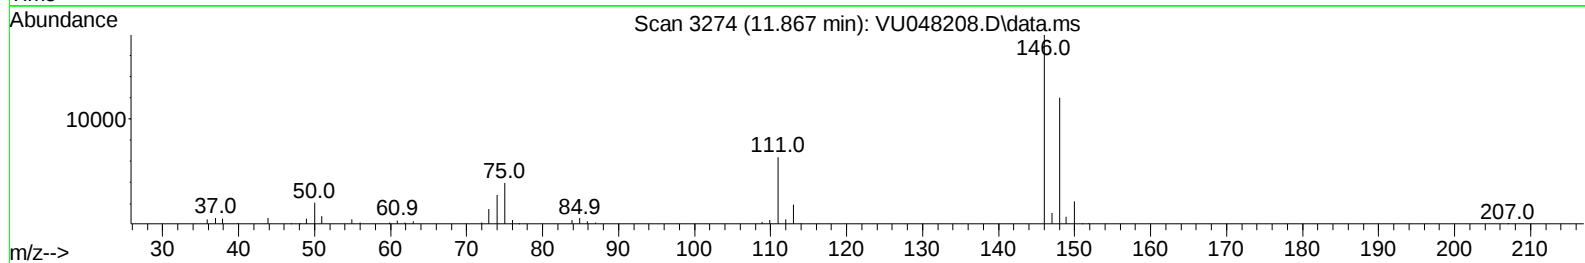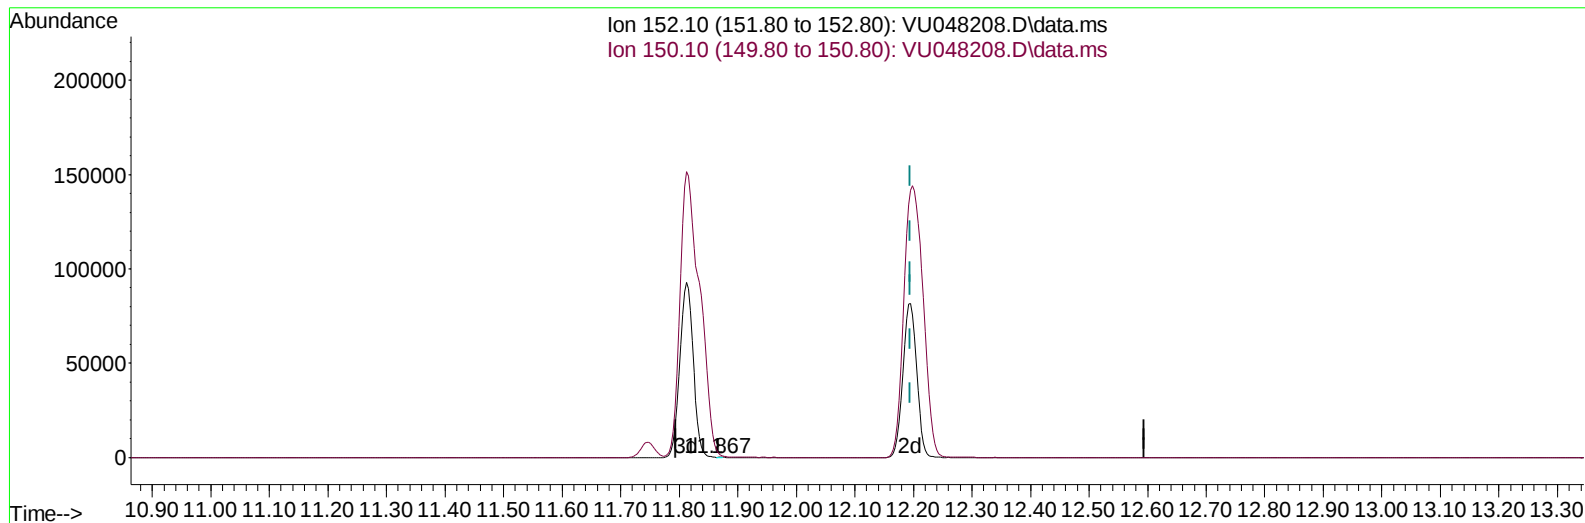

TIC: VU048208.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.867min (-0.328) 0.03 ug/L

response 71

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	171.40	154.93
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048208.D
 Acq On : 22 Apr 2022 06:46
 Operator : SY/MD
 Sample : N2488-10 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 07:43:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

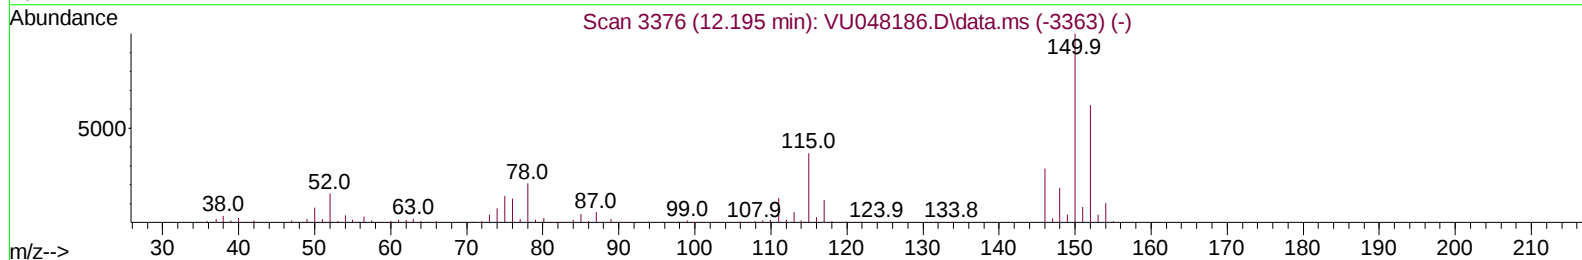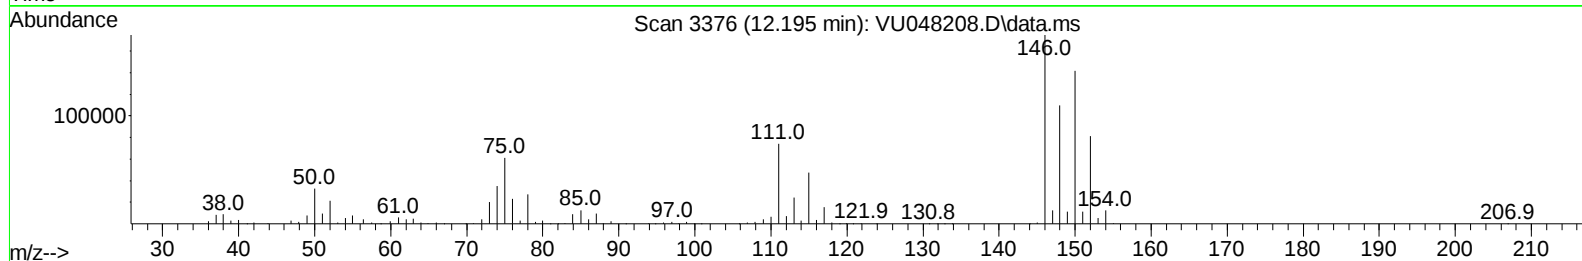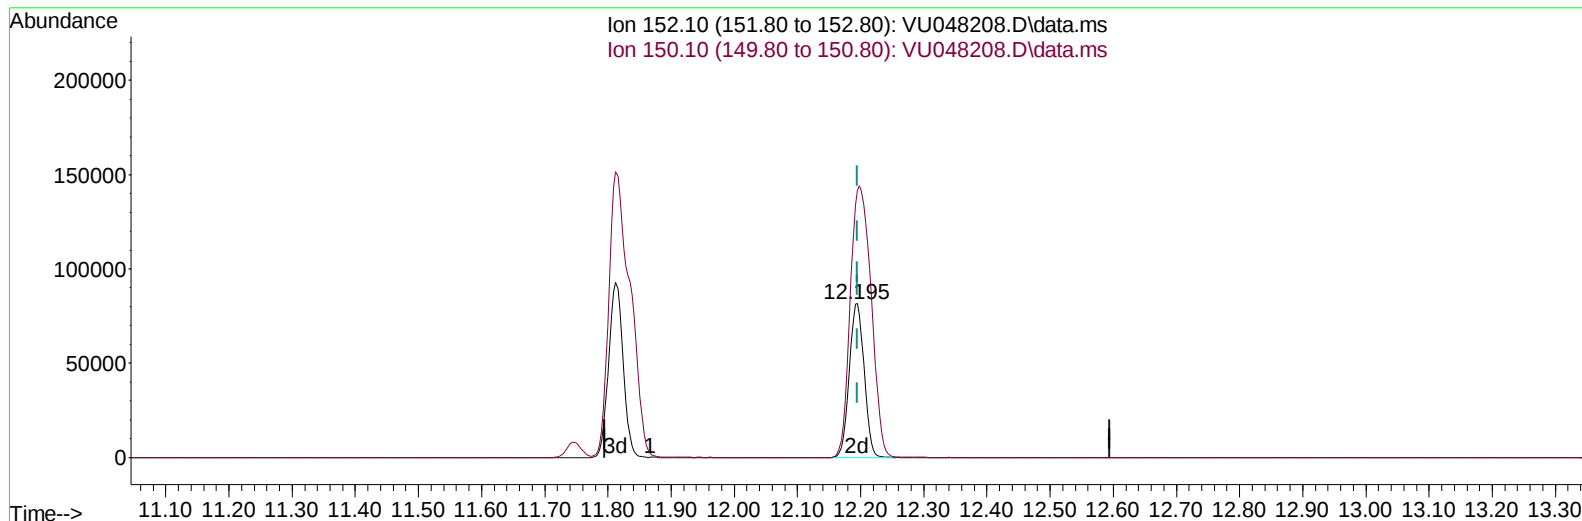

TIC: VU048208.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

12.195min (-0.000) 50.46 ug/L m

response 132887

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	171.40	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048208.D
 Acq On : 22 Apr 2022 06:46
 Operator : SY/MD
 Sample : N2488-10 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
 Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 07:43:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	295310	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	296849	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	148023	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	81835	38.214	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	76.420%	
7) Chloroethane-d5	1.915	69	73181	43.339	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	86.680%	
11) 1,1-Dichloroethene-d2	2.568	63	106248	27.118	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	54.240%#	
21) 2-Butanone-d5	4.620	46	190066	103.404	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	103.400%	
24) Chloroform-d	5.066	84	179711	45.864	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.720%	
26) 1,2-Dichloroethane-d4	5.703	65	115469	48.048	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.100%	
32) Benzene-d6	5.729	84	348269	46.625	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.260%	
36) 1,2-Dichloropropane-d6	6.693	67	122418	53.365	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.740%	
41) Toluene-d8	7.899	98	276908	38.050	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	76.100%#	
43) trans-1,3-Dichloroprop...	8.179	79	45970	39.555	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.120%	
47) 2-Hexanone-d5	8.632	63	122459	91.191	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	91.190%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	195140	49.568	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	99.140%	
66) 1,2-Dichlorobenzene-d4	12.195	152	132887m	50.461	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.920%	
Target Compounds					Qvalue	
31) Carbon tetrachloride	5.533	117	3516	1.157	ug/L	97
33) Benzene	5.777	78	936889	109.037	ug/L	100
51) Chlorobenzene	9.449	112	2849069	445.067	ug/L	98
64) 1,3-Dichlorobenzene	11.745	146	128801	28.967	ug/L	98
65) 1,4-Dichlorobenzene	11.838	146	1167286	253.445	ug/L	99
67) 1,2-Dichlorobenzene	12.214	146	1226614	275.696	ug/L	100
70) 1,2,4-trichlorobenzene	13.841	180	237189	74.987	ug/L	99
72) 1,2,3-Trichlorobenzene	14.330	180	65983	20.809	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048208.D
Acq On : 22 Apr 2022 06:46
Operator : SY/MD
Sample : N2488-10 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2022
Supervised By :Mahesh Dadoda 04/25/2022

Quant Time: Apr 22 07:43:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 22 02:51:38 2022
Response via : Initial Calibration

