

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048193.D
 Acq On : 21 Apr 2022 23:42
 Operator : SY/MD
 Sample : N2485-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J25

Quant Time: Apr 22 06:36:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 22 02:51:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	319224	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	340589	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	161921	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	92534	39.973	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.940%
7) Chloroethane-d5	1.916	69	82019	44.935	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.860%
11) 1,1-Dichloroethene-d2	2.568	63	126682	29.911	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.820%#
21) 2-Butanone-d5	4.620	46	174656	87.902	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.900%
24) Chloroform-d	5.067	84	194194	45.847	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.700%
26) 1,2-Dichloroethane-d4	5.703	65	121614	46.814	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.620%
32) Benzene-d6	5.729	84	383466	44.744	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.480%
36) 1,2-Dichloropropane-d6	6.694	67	130601	49.621	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.240%
41) Toluene-d8	7.899	98	324288	38.837	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.680%#
43) trans-1,3-Dichloroprop...	8.179	79	51008	38.254	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.500%
47) 2-Hexanone-d5	8.632	63	118490	76.904	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.900%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	202488	44.829	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.660%
66) 1,2-Dichlorobenzene-d4	12.195	152	142094	49.326	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.660%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	24986	13.513	ug/L	98
51) Chlorobenzene	9.446	112	11956	1.628	ug/L	94
64) 1,3-Dichlorobenzene	11.745	146	6298	1.295	ug/L	95
65) 1,4-Dichlorobenzene	11.838	146	27740	5.506	ug/L	96
67) 1,2-Dichlorobenzene	12.214	146	22727	4.670	ug/L	97
70) 1,2,4-trichlorobenzene	13.841	180	30794	8.900	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048193.D
Acq On : 21 Apr 2022 23:42
Operator : SY/MD
Sample : N2485-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J25

Quant Time: Apr 22 06:36:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 22 02:51:38 2022
Response via : Initial Calibration




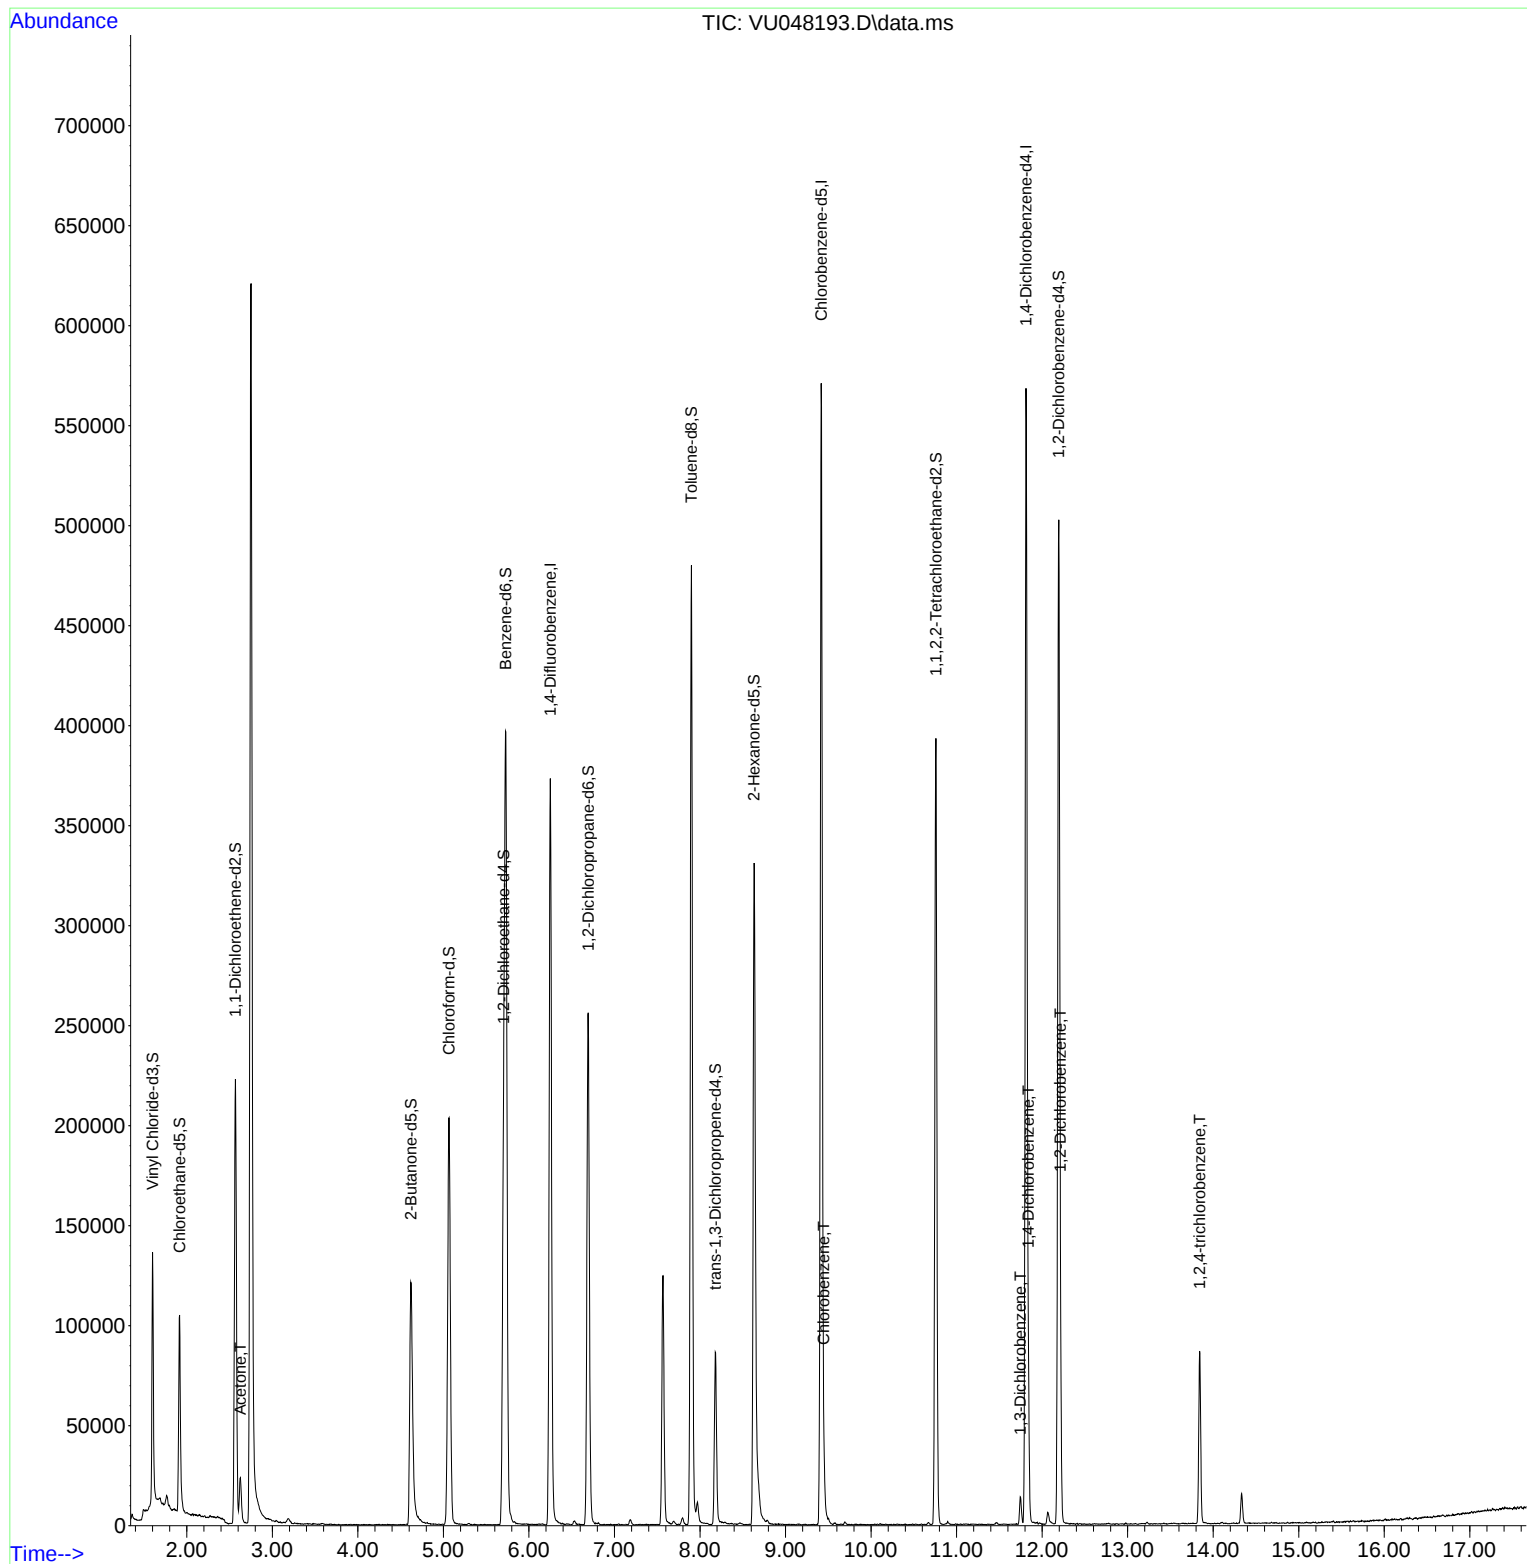


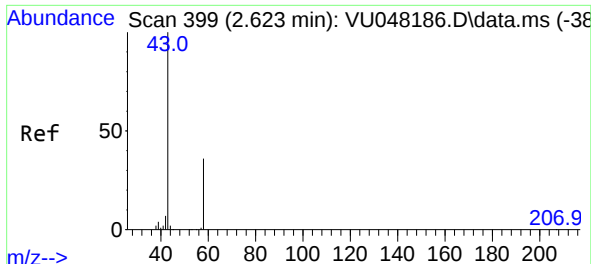

#13
Acetone
Concen: 13.513 ug/L
RT: 2.626 min Scan# 400
Delta R.T. 0.003 min
Lab File: VU048193.D
Acq: 21 Apr 2022 23:42




Instrument :
MSVOA_U
ClientSampleId :
C0J25


Tgt Ion: 43 Resp: 24986
Ion Ratio Lower Upper
43 100
58 36.1 0.0 70.0

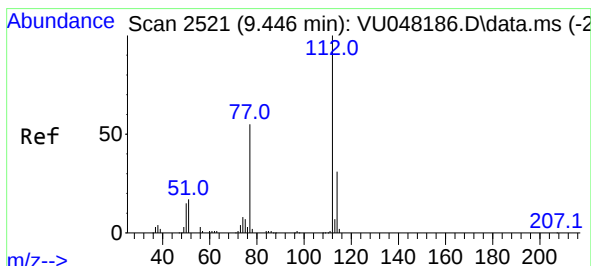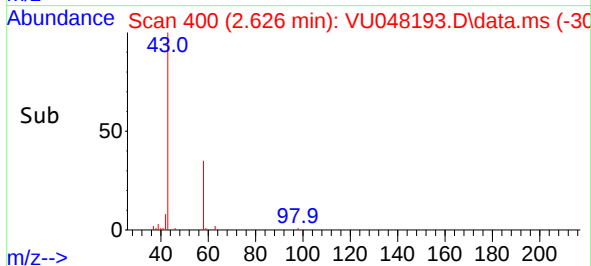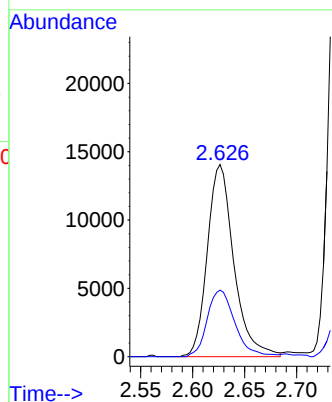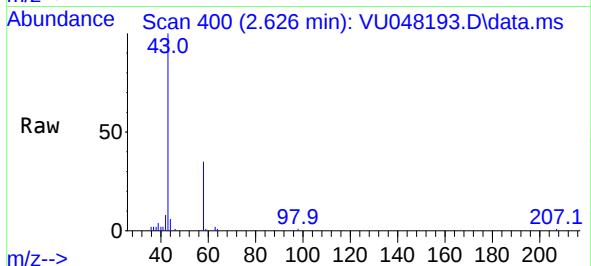

#51
Chlorobenzene
Concen: 1.628 ug/L
RT: 9.446 min Scan# 2521
Delta R.T. 0.000 min
Lab File: VU048193.D
Acq: 21 Apr 2022 23:42

Tgt Ion: 112 Resp: 11956
Ion Ratio Lower Upper
112 100
114 32.7 22.1 41.1
77 60.1 43.4 65.0


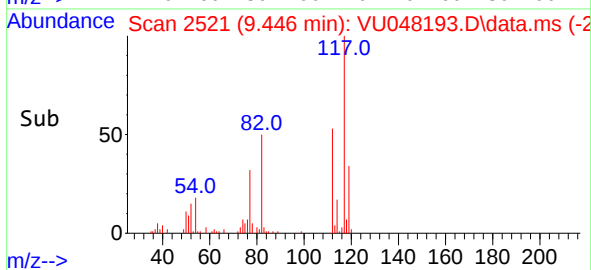
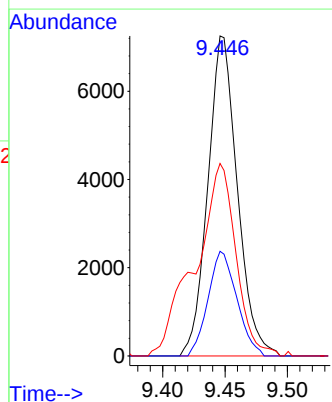
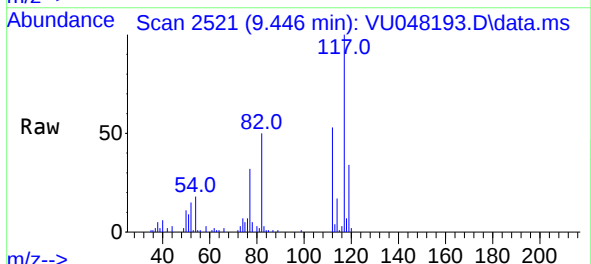


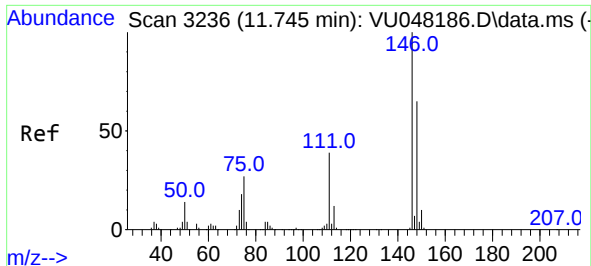

#64
1,3-Dichlorobenzene
Concen: 1.295 ug/L
RT: 11.745 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU048193.D
Acq: 21 Apr 2022 23:42




Instrument :
MSVOA_U
ClientSampleId :
C0J25


Tgt Ion:146 Resp: 6298
Ion Ratio Lower Upper
146 100
111 38.5 26.7 49.7
148 69.7 44.4 82.5

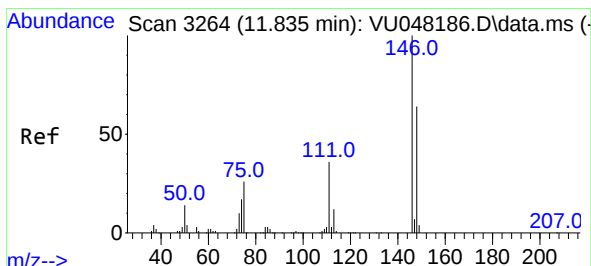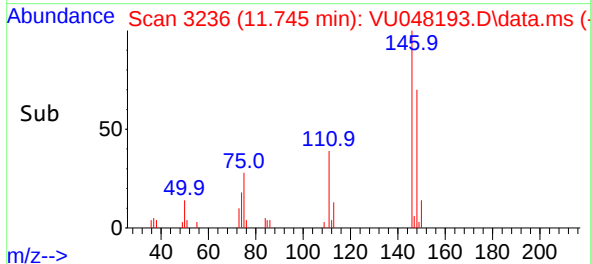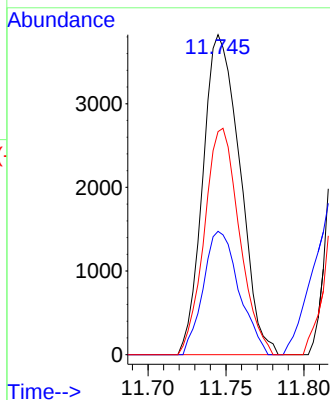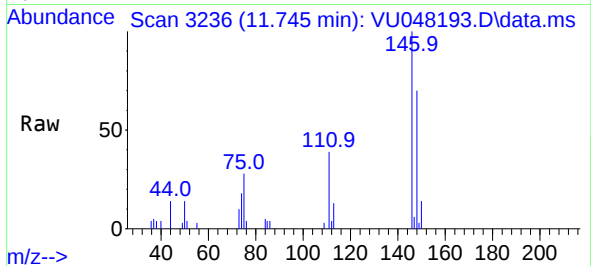

#65
1,4-Dichlorobenzene
Concen: 5.506 ug/L
RT: 11.838 min Scan# 3265
Delta R.T. 0.003 min
Lab File: VU048193.D
Acq: 21 Apr 2022 23:42

Tgt Ion:146 Resp: 27740
Ion Ratio Lower Upper
146 100
111 38.3 25.3 47.1
148 67.4 44.5 82.7

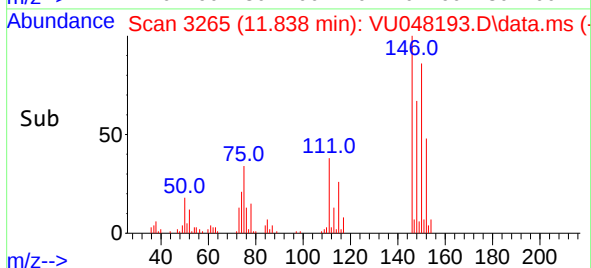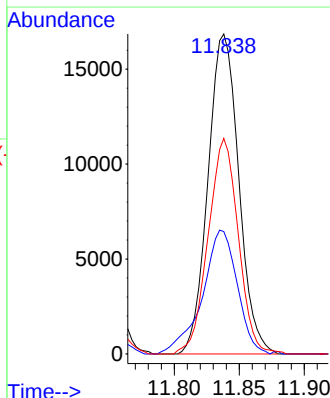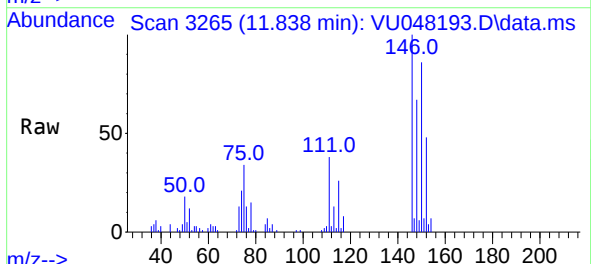

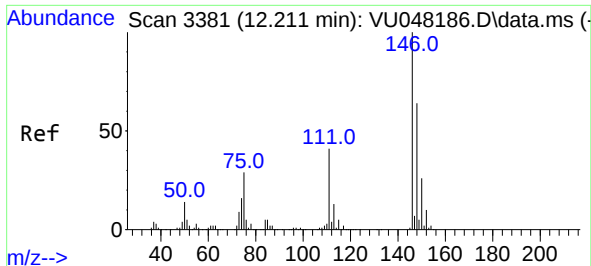

#67

1,2-Dichlorobenzene

Concen: 4.670 ug/L

RT: 12.214 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU048193.D

Acq: 21 Apr 2022 23:42

Instrument :

MSVOA_U

ClientSampleId :

C0J25





Tgt Ion:146 Resp: 22727

Ion Ratio Lower Upper

146 100

111 42.5 31.7 47.5

148 65.5 51.4 77.2

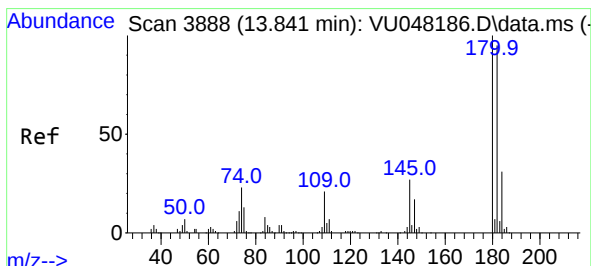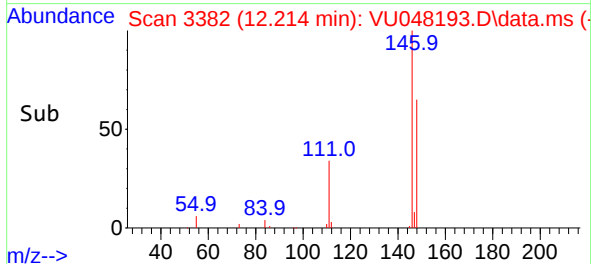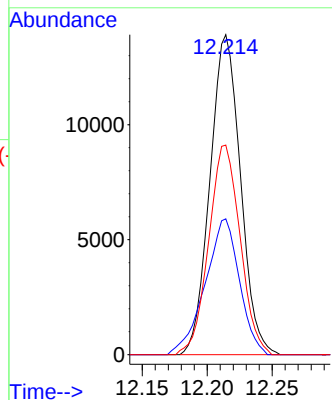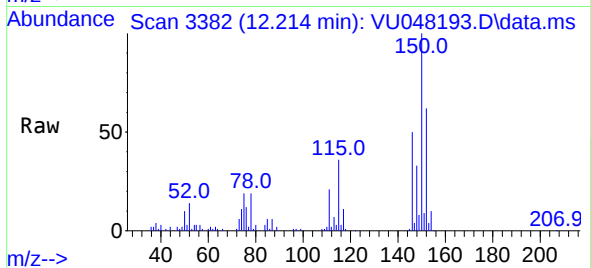

#70

1,2,4-trichlorobenzene

Concen: 8.900 ug/L

RT: 13.841 min Scan# 3888

Delta R.T. 0.000 min

Lab File: VU048193.D

Acq: 21 Apr 2022 23:42

Tgt Ion:180 Resp: 30794

Ion Ratio Lower Upper

180 100

182 91.7 76.2 114.2

145 26.7 21.8 32.8

