

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048164.D
 Acq On : 21 Apr 2022 11:29
 Operator : SY/MD
 Sample : VU0421WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	144596	169048	14.48%	1.804%
2	1.916	170	179	200	rVB	114227	162374	13.91%	1.733%
3	2.572	370	383	399	rBV	241006	396881	34.00%	4.236%
4	2.710	421	426	430	rVB3	434	498	0.04%	0.005%
5	2.729	430	432	436	rBV	372	293	0.03%	0.003%
6	2.768	441	444	448	rVV	549	524	0.04%	0.006%
7	2.790	448	451	457	rVB4	565	660	0.06%	0.007%
8	2.864	470	474	479	rVB2	341	313	0.03%	0.003%
9	2.954	498	502	503	rBV2	302	219	0.02%	0.002%
10	3.051	524	532	542	rVB4	1756	2991	0.26%	0.032%
11	3.192	562	576	593	rVB	4613	11196	0.96%	0.120%
12	3.330	617	619	627	rVB2	183	175	0.01%	0.002%
13	3.520	674	678	681	rBV2	234	200	0.02%	0.002%
14	3.719	738	740	747	rVB2	261	209	0.02%	0.002%
15	4.073	844	850	852	rBV2	190	213	0.02%	0.002%
16	4.105	857	860	869	rVB2	181	218	0.02%	0.002%
17	4.144	869	872	876	rBV2	239	211	0.02%	0.002%
18	4.282	912	915	920	rBV2	179	193	0.02%	0.002%
19	4.346	932	935	940	rVB2	215	186	0.02%	0.002%
20	4.414	951	956	962	rVB2	166	189	0.02%	0.002%
21	4.626	1005	1022	1053	rBV	139387	355352	30.44%	3.793%
22	5.067	1142	1159	1193	rBV	217576	472219	40.45%	5.041%
23	5.295	1224	1230	1239	rVB4	699	962	0.08%	0.010%
24	5.642	1332	1338	1341	rBV2	214	229	0.02%	0.002%
25	5.729	1343	1365	1391	rBV2	428461	1167443	100.00%	12.462%
26	5.864	1405	1407	1411	rVB2	489	286	0.02%	0.003%
27	5.887	1411	1414	1417	rVB2	349	198	0.02%	0.002%
28	6.073	1468	1472	1475	rVB2	376	231	0.02%	0.002%
29	6.099	1475	1480	1481	rBV	386	301	0.03%	0.003%
30	6.115	1481	1485	1489	rBV2	312	319	0.03%	0.003%
31	6.160	1495	1499	1509	rVB2	223	276	0.02%	0.003%
32	6.250	1509	1527	1552	rBV	352314	677144	58.00%	7.228%
33	6.488	1595	1601	1604	rVB2	306	354	0.03%	0.004%
34	6.533	1604	1615	1622	rBV6	1924	3574	0.31%	0.038%
35	6.694	1650	1665	1688	rBV	272020	531729	45.55%	5.676%
36	6.806	1697	1700	1707	rVB3	921	1083	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048164.D
 Acq On : 21 Apr 2022 11:29
 Operator : SY/MD
 Sample : VU0421WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.845	1707	1712	1714	rBV3	245	193	0.02%	0.002%
38	6.870	1717	1720	1723	rVB2	358	176	0.02%	0.002%
39	6.935	1738	1740	1748	rVB2	287	240	0.02%	0.003%
40	6.980	1748	1754	1759	rBV2	275	236	0.02%	0.003%
41	7.057	1771	1778	1783	rVB3	390	559	0.05%	0.006%
42	7.179	1810	1816	1817	rBV3	2324	1780	0.15%	0.019%
43	7.266	1839	1843	1846	rBV	225	184	0.02%	0.002%
44	7.478	1896	1909	1914	rBV	299	550	0.05%	0.006%
45	7.568	1924	1937	1967	rBV	123366	221811	19.00%	2.368%
46	7.687	1967	1974	1984	rVB5	1362	2638	0.23%	0.028%
47	7.739	1987	1990	1996	rVB2	328	285	0.02%	0.003%
48	7.793	2001	2007	2017	rVB3	1481	1685	0.14%	0.018%
49	7.899	2023	2040	2057	rBV	495031	874245	74.89%	9.332%
50	8.112	2102	2106	2113	rVB3	483	538	0.05%	0.006%
51	8.182	2113	2128	2143	rBV	89321	154017	13.19%	1.644%
52	8.349	2178	2180	2185	rVB2	369	215	0.02%	0.002%
53	8.555	2240	2244	2249	rBV3	503	508	0.04%	0.005%
54	8.636	2255	2269	2302	rBV	388959	720549	61.72%	7.691%
55	8.915	2351	2356	2362	rVB4	791	749	0.06%	0.008%
56	8.996	2379	2381	2386	rVB2	303	261	0.02%	0.003%
57	9.173	2434	2436	2443	rVB2	268	260	0.02%	0.003%
58	9.253	2456	2461	2466	rBV2	263	231	0.02%	0.002%
59	9.346	2485	2490	2493	rBV2	255	242	0.02%	0.003%
60	9.420	2499	2513	2553	rBV	542863	947708	81.18%	10.116%
61	9.565	2555	2558	2565	rVB4	659	626	0.05%	0.007%
62	9.697	2592	2599	2607	rVB4	719	1162	0.10%	0.012%
63	9.742	2607	2613	2617	rBV2	190	238	0.02%	0.003%
64	9.874	2650	2654	2659	rVB2	228	175	0.01%	0.002%
65	10.108	2722	2727	2728	rBV2	346	333	0.03%	0.004%
66	10.439	2828	2830	2836	rVB2	296	191	0.02%	0.002%
67	10.481	2836	2843	2847	rBV2	465	394	0.03%	0.004%
68	10.652	2889	2896	2897	rBV	333	324	0.03%	0.003%
69	10.671	2897	2902	2903	rBV2	798	580	0.05%	0.006%
70	10.758	2916	2929	2950	rVB	414260	677081	58.00%	7.227%
71	10.883	2965	2968	2974	rVB2	324	332	0.03%	0.004%
72	11.099	3033	3035	3041	rVB3	279	197	0.02%	0.002%
73	11.259	3082	3085	3088	rVB2	321	193	0.02%	0.002%
74	11.465	3145	3149	3160	rVB5	1034	1483	0.13%	0.016%
75	11.539	3167	3172	3175	rBV2	268	229	0.02%	0.002%
76	11.565	3178	3180	3183	rVB2	273	180	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048164.D
 Acq On : 21 Apr 2022 11:29
 Operator : SY/MD
 Sample : VU0421WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.664	3207	3211	3214	rVB2	266	201	0.02%	0.002%
78	11.684	3214	3217	3218	rBV	396	212	0.02%	0.002%
79	11.748	3231	3237	3245	rBV3	2260	2951	0.25%	0.032%
80	11.812	3245	3257	3277	rBV	539621	895943	76.74%	9.564%
81	11.938	3294	3296	3297	rBV	474	200	0.02%	0.002%
82	11.967	3303	3305	3309	rVB2	499	268	0.02%	0.003%
83	12.195	3360	3376	3396	rBV	523107	872533	74.74%	9.314%
84	12.340	3418	3421	3422	rBV	367	243	0.02%	0.003%
85	12.507	3471	3473	3475	rBV	360	198	0.02%	0.002%
86	12.603	3499	3503	3508	rVV3	284	315	0.03%	0.003%
87	12.719	3536	3539	3541	rBV	318	239	0.02%	0.003%
88	12.790	3559	3561	3566	rVB2	400	281	0.02%	0.003%
89	12.816	3566	3569	3571	rBV2	280	179	0.02%	0.002%
90	12.886	3587	3591	3592	rBV	326	222	0.02%	0.002%
91	13.044	3636	3640	3645	rBV2	359	369	0.03%	0.004%
92	13.086	3649	3653	3656	rVB2	439	364	0.03%	0.004%
93	13.140	3665	3670	3672	rBV3	309	338	0.03%	0.004%
94	13.179	3677	3682	3685	rBV2	364	388	0.03%	0.004%
95	13.224	3691	3696	3701	rBV3	863	1088	0.09%	0.012%
96	13.844	3882	3889	3900	rVB3	5120	7436	0.64%	0.079%
97	14.095	3959	3967	3980	rVB	4658	6898	0.59%	0.074%
98	14.333	4033	4041	4050	rBV4	3020	4208	0.36%	0.045%
99	15.327	4347	4350	4352	rBV	556	380	0.03%	0.004%
100	15.442	4384	4386	4393	rVB2	849	716	0.06%	0.008%




Sum of corrected areas: 9368239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048164.D
Acq On : 21 Apr 2022 11:29
Operator : SY/MD
Sample : VU0421WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK105

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

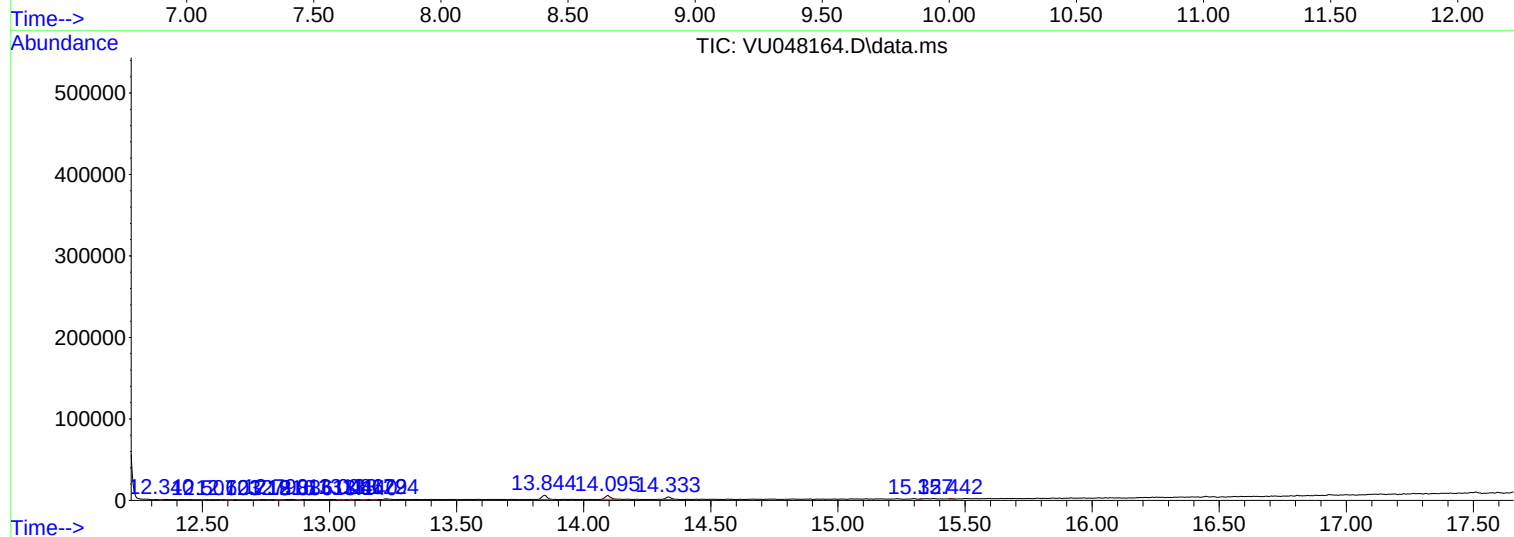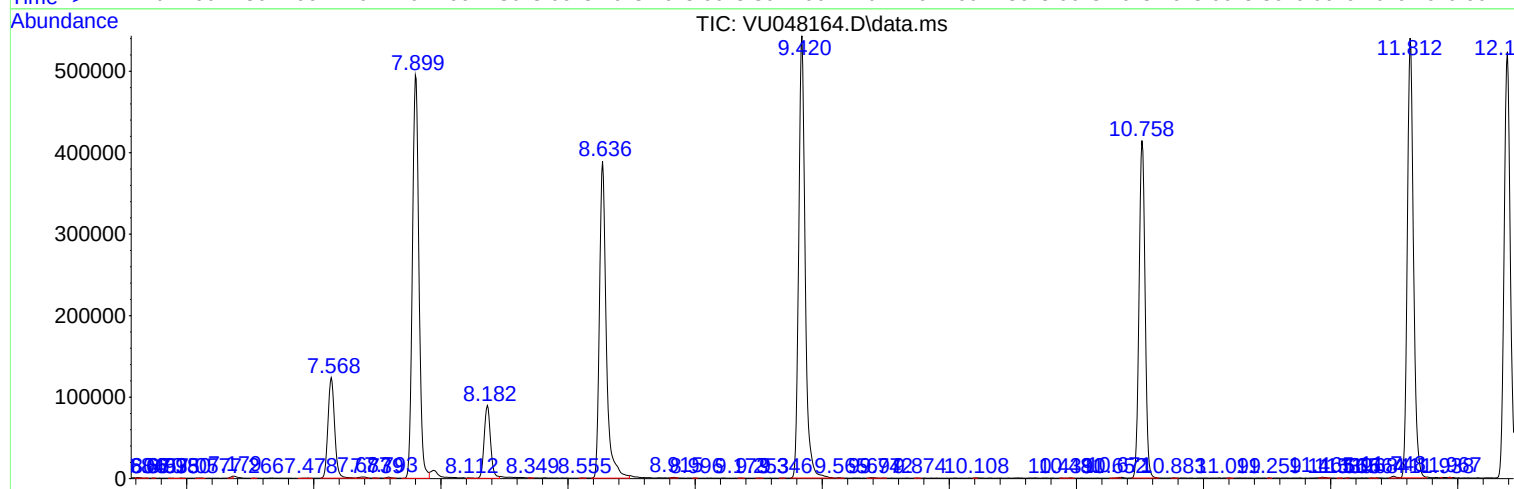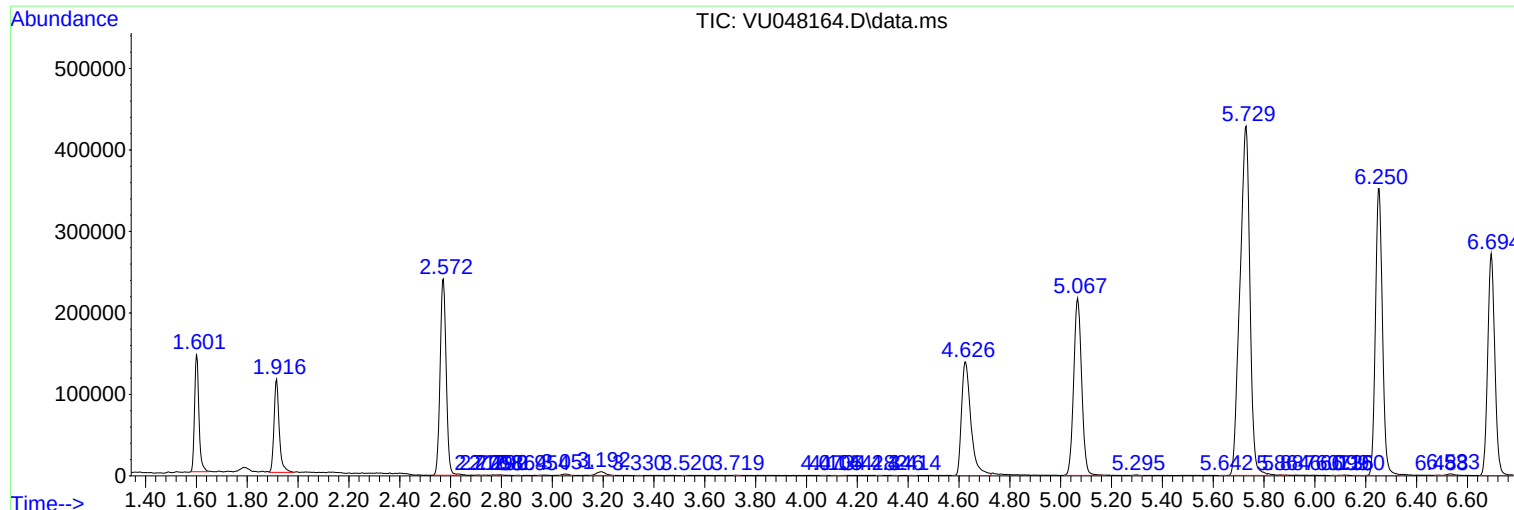

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048164.D
Acq On : 21 Apr 2022 11:29
Operator : SY/MD
Sample : VU0421WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK105

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048164.D
Acq On : 21 Apr 2022 11:29
Operator : SY/MD
Sample : VU0421WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK105

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------