

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048165.D
 Acq On : 21 Apr 2022 12:15
 Operator : SY/MD
 Sample : N2486-08DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rBV	139483	162998	11.09%	1.544%
2	1.915	171	179	194	rBV	106940	148901	10.13%	1.410%
3	2.571	370	383	397	rBV	242878	395758	26.93%	3.748%
4	2.758	426	441	450	rBV2	2833	5422	0.37%	0.051%
5	2.825	459	462	463	rBV	198	89	0.01%	0.001%
6	3.050	524	532	541	rVB3	1999	3224	0.22%	0.031%
7	3.112	548	551	554	rBV	179	130	0.01%	0.001%
8	3.189	561	575	592	rBV2	29626	66762	4.54%	0.632%
9	3.301	603	610	614	rBV2	267	316	0.02%	0.003%
10	3.378	631	634	637	rVB2	209	132	0.01%	0.001%
11	3.401	637	641	645	rBV	237	246	0.02%	0.002%
12	3.481	664	666	669	rVB2	72	37	0.00%	0.000%
13	3.513	673	676	677	rBV	202	96	0.01%	0.001%
14	3.607	703	705	707	rVB	110	46	0.00%	0.000%
15	3.623	707	710	713	rVB2	184	111	0.01%	0.001%
16	3.642	713	716	717	rBV	125	74	0.01%	0.001%
17	3.687	726	730	737	rVB2	206	248	0.02%	0.002%
18	3.726	737	742	745	rBV2	132	107	0.01%	0.001%
19	3.768	751	755	759	rBV2	144	132	0.01%	0.001%
20	3.813	766	769	771	rBV2	146	104	0.01%	0.001%
21	3.973	811	819	822	rBV	212	193	0.01%	0.002%
22	3.999	822	827	830	rVB2	185	149	0.01%	0.001%
23	4.041	830	840	846	rBV2	302	416	0.03%	0.004%
24	4.150	870	874	875	rBV	135	100	0.01%	0.001%
25	4.214	890	894	897	rBV2	272	180	0.01%	0.002%
26	4.269	906	911	917	rBV2	184	226	0.02%	0.002%
27	4.356	935	938	940	rBV	69	41	0.00%	0.000%
28	4.417	953	957	961	rVB	148	111	0.01%	0.001%
29	4.456	961	969	974	rBV2	200	290	0.02%	0.003%
30	4.507	982	985	991	rVB	239	171	0.01%	0.002%
31	4.546	994	997	999	rBV	219	142	0.01%	0.001%
32	4.623	1008	1021	1054	rBV	129933	321772	21.90%	3.047%
33	5.066	1143	1159	1185	rBV	209797	458689	31.22%	4.344%
34	5.221	1204	1207	1211	rBV3	300	220	0.01%	0.002%
35	5.263	1216	1220	1223	rBV3	227	168	0.01%	0.002%
36	5.292	1223	1229	1233	rBV3	745	888	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048165.D
 Acq On : 21 Apr 2022 12:15
 Operator : SY/MD
 Sample : N2486-08DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.333	1239	1242	1244	rBV2	231	94	0.01%	0.001%
38	5.346	1244	1246	1247	rVV	245	76	0.01%	0.001%
39	5.359	1247	1250	1254	rVB2	118	86	0.01%	0.001%
40	5.382	1254	1257	1261	rVB2	159	105	0.01%	0.001%
41	5.401	1261	1263	1265	rBV	74	34	0.00%	0.000%
42	5.414	1265	1267	1269	rVB	84	35	0.00%	0.000%
43	5.494	1288	1292	1295	rBV2	192	177	0.01%	0.002%
44	5.552	1308	1310	1312	rBV	80	36	0.00%	0.000%
45	5.600	1322	1325	1328	rBV	91	65	0.00%	0.001%
46	5.616	1328	1330	1332	rBV2	109	50	0.00%	0.000%
47	5.648	1337	1340	1343	rBV2	118	97	0.01%	0.001%
48	5.729	1343	1365	1401	rBV2	416832	1147438	78.09%	10.867%
49	6.009	1448	1452	1458	rBV3	267	386	0.03%	0.004%
50	6.121	1482	1487	1495	rBV2	578	632	0.04%	0.006%
51	6.163	1496	1500	1503	rVB2	262	186	0.01%	0.002%
52	6.253	1513	1528	1552	rBV	363859	705431	48.01%	6.681%
53	6.529	1607	1614	1625	rBV8	1742	3303	0.22%	0.031%
54	6.629	1642	1645	1648	rVB	300	136	0.01%	0.001%
55	6.693	1649	1665	1689	rBV	263582	517087	35.19%	4.897%
56	6.899	1722	1729	1733	rBV2	215	257	0.02%	0.002%
57	6.925	1734	1737	1738	rBV	174	85	0.01%	0.001%
58	6.957	1744	1747	1749	rBV2	124	82	0.01%	0.001%
59	7.012	1761	1764	1765	rBV	121	74	0.01%	0.001%
60	7.099	1787	1791	1794	rBV	182	138	0.01%	0.001%
61	7.118	1794	1797	1802	rBV2	131	114	0.01%	0.001%
62	7.185	1807	1818	1827	rBV7	2262	4043	0.28%	0.038%
63	7.353	1867	1870	1876	rBV	178	224	0.02%	0.002%
64	7.391	1880	1882	1885	rVV2	230	135	0.01%	0.001%
65	7.423	1885	1892	1895	rVV2	210	231	0.02%	0.002%
66	7.455	1899	1902	1906	rVB	154	90	0.01%	0.001%
67	7.494	1911	1914	1917	rVB2	124	73	0.00%	0.001%
68	7.568	1920	1937	1957	rBV2	122547	216555	14.74%	2.051%
69	7.690	1967	1975	1988	rVB2	1876	3161	0.22%	0.030%
70	7.761	1995	1997	2000	rBV	224	78	0.01%	0.001%
71	7.793	2000	2007	2008	rBV2	986	959	0.07%	0.009%
72	7.899	2026	2040	2056	rBV	490449	859356	58.48%	8.139%
73	8.182	2113	2128	2143	rBV	86799	148040	10.08%	1.402%
74	8.635	2253	2269	2305	rBV	341563	653774	44.49%	6.192%
75	8.925	2357	2359	2361	rBV2	193	113	0.01%	0.001%
76	8.938	2361	2363	2366	rVB2	334	168	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048165.D
 Acq On : 21 Apr 2022 12:15
 Operator : SY/MD
 Sample : N2486-08DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.134	2418	2424	2426	rBV	217	208	0.01%	0.002%
78	9.317	2478	2481	2484	rBV2	282	232	0.02%	0.002%
79	9.420	2499	2513	2553	rBV2	561469	1290251	87.81%	12.220%
80	9.642	2579	2582	2589	rVB2	472	380	0.03%	0.004%
81	9.684	2591	2595	2597	rBV2	338	312	0.02%	0.003%
82	9.738	2609	2612	2613	rBV2	205	118	0.01%	0.001%
83	9.825	2634	2639	2643	rVB2	264	280	0.02%	0.003%
84	9.996	2689	2692	2702	rVB	331	422	0.03%	0.004%
85	10.047	2702	2708	2713	rBV2	173	197	0.01%	0.002%
86	10.089	2718	2721	2723	rBV	218	158	0.01%	0.001%
87	10.163	2741	2744	2745	rBV	184	88	0.01%	0.001%
88	10.221	2759	2762	2765	rBV	229	148	0.01%	0.001%
89	10.417	2822	2823	2826	rBV	163	85	0.01%	0.001%
90	10.758	2916	2929	2955	rBV	396324	651259	44.32%	6.168%
91	10.922	2977	2980	2986	rBV3	252	202	0.01%	0.002%
92	11.272	3085	3089	3092	rBV2	227	204	0.01%	0.002%
93	11.468	3142	3150	3157	rVB5	1079	1841	0.13%	0.017%
94	11.690	3216	3219	3223	rBV2	446	241	0.02%	0.002%
95	11.748	3227	3237	3246	rBV	16929	25929	1.76%	0.246%
96	11.815	3246	3258	3284	rVB2	559288	1047462	71.29%	9.920%
97	12.201	3363	3378	3406	rBV2	624084	1469362	100.00%	13.916%
98	12.979	3615	3620	3622	rBV3	815	819	0.06%	0.008%
99	13.841	3878	3888	3913	rBV	126219	198469	13.51%	1.880%
100	14.333	4032	4041	4053	rVB2	23862	38355	2.61%	0.363%




Sum of corrected areas: 10558915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048165.D
Acq On : 21 Apr 2022 12:15
Operator : SY/MD
Sample : N2486-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

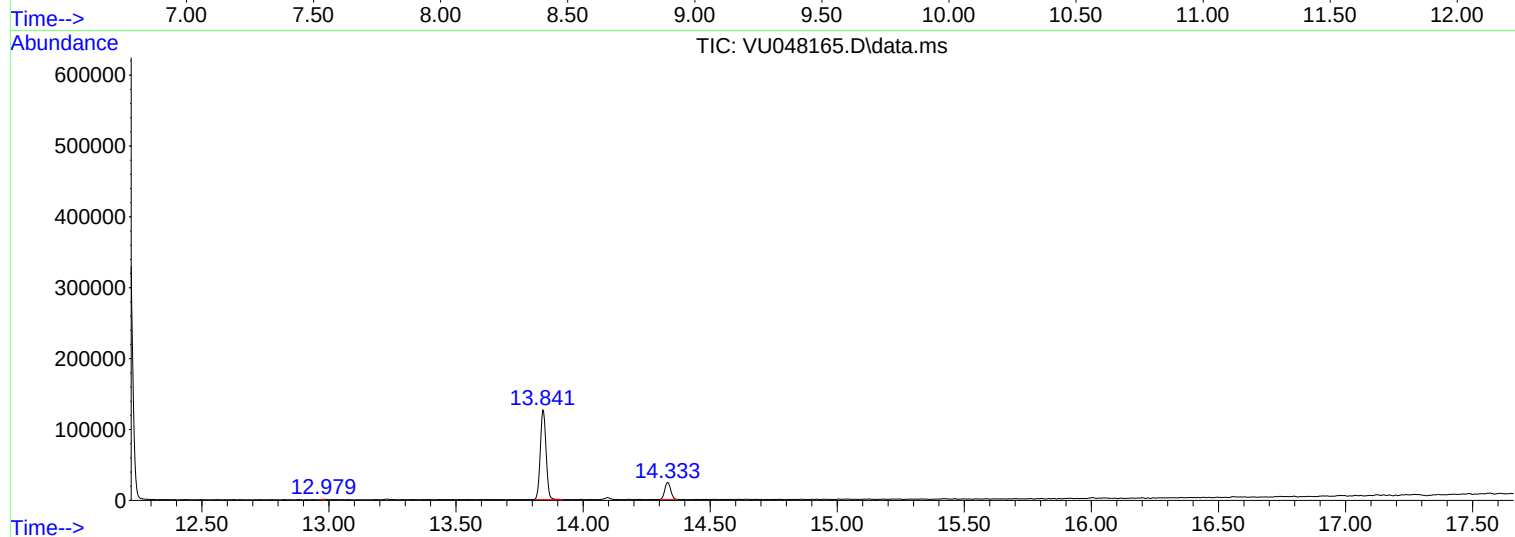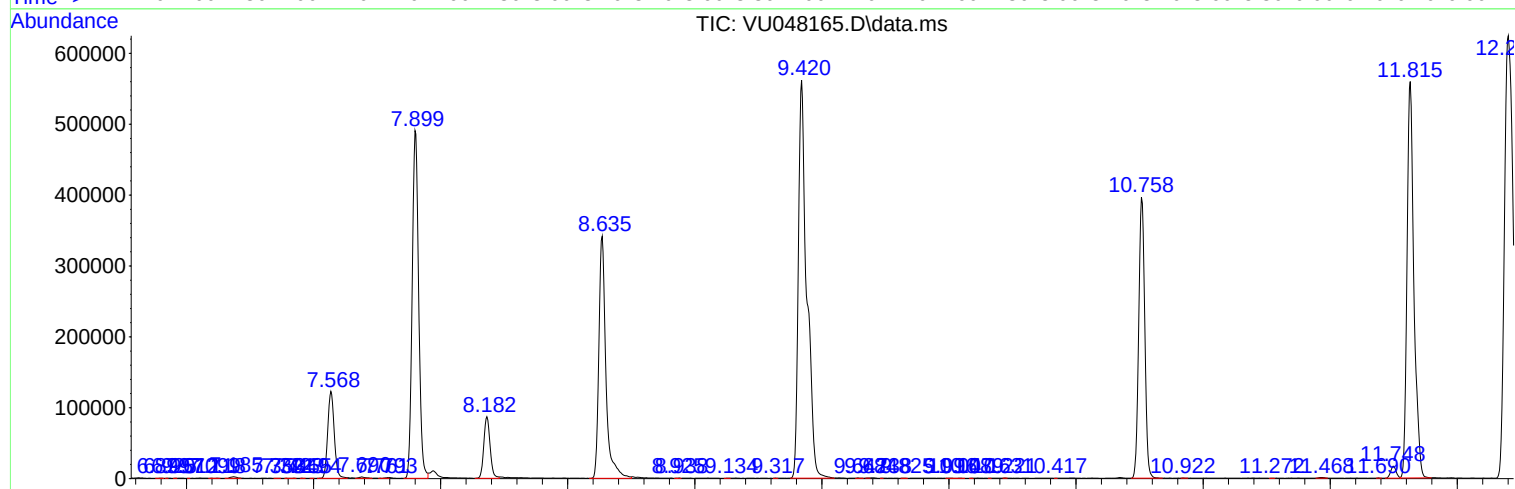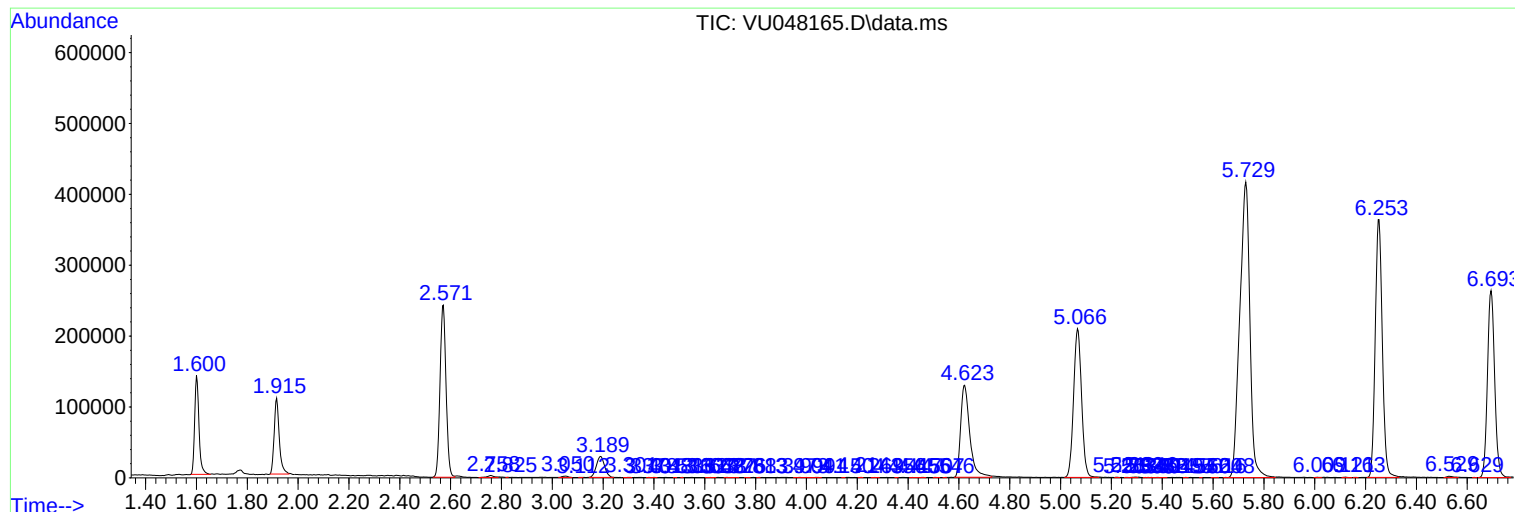

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048165.D
Acq On : 21 Apr 2022 12:15
Operator : SY/MD
Sample : N2486-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048165.D
Acq On : 21 Apr 2022 12:15
Operator : SY/MD
Sample : N2486-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------