

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048166.D
 Acq On : 21 Apr 2022 12:38
 Operator : SY/MD
 Sample : N2486-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	100	rBV	141974	165873	14.39%	1.755%
2	1.913	170	178	197	rVB	104062	153464	13.31%	1.624%
3	2.569	370	382	402	rBV	243432	401475	34.82%	4.249%
4	2.742	432	436	437	rBV4	512	367	0.03%	0.004%
5	2.826	457	462	465	rVB3	368	309	0.03%	0.003%
6	2.932	491	495	498	rBV3	311	257	0.02%	0.003%
7	2.954	499	502	506	rVB2	338	276	0.02%	0.003%
8	3.048	524	531	543	rVB3	2341	4185	0.36%	0.044%
9	3.096	543	546	548	rBV	212	165	0.01%	0.002%
10	3.109	548	550	556	rVB	363	219	0.02%	0.002%
11	3.189	557	575	595	rVB2	31031	72352	6.28%	0.766%
12	3.469	659	662	666	rBV2	225	185	0.02%	0.002%
13	3.491	666	669	673	rVV3	285	214	0.02%	0.002%
14	3.559	686	690	692	rBV2	302	218	0.02%	0.002%
15	3.575	692	695	699	rVB2	209	164	0.01%	0.002%
16	3.749	744	749	759	rVB3	338	439	0.04%	0.005%
17	3.835	766	776	779	rBV2	178	251	0.02%	0.003%
18	4.022	828	834	835	rBV2	187	177	0.02%	0.002%
19	4.093	853	856	861	rBV2	176	183	0.02%	0.002%
20	4.234	895	900	901	rBV2	224	174	0.02%	0.002%
21	4.620	1006	1020	1055	rBV	132200	322158	27.94%	3.409%
22	5.067	1142	1159	1177	rBV	209943	461156	40.00%	4.880%
23	5.221	1203	1207	1209	rVB2	347	251	0.02%	0.003%
24	5.289	1223	1228	1229	rBV2	373	311	0.03%	0.003%
25	5.462	1279	1282	1287	rVB2	196	200	0.02%	0.002%
26	5.575	1314	1317	1322	rVB	199	155	0.01%	0.002%
27	5.636	1330	1336	1338	rBV2	210	199	0.02%	0.002%
28	5.726	1343	1364	1399	rVV2	421493	1153001	100.00%	12.201%
29	5.967	1436	1439	1445	rVB3	559	509	0.04%	0.005%
30	5.996	1445	1448	1453	rVB2	270	163	0.01%	0.002%
31	6.028	1456	1458	1462	rVB2	270	209	0.02%	0.002%
32	6.102	1478	1481	1485	rBV3	333	255	0.02%	0.003%
33	6.128	1486	1489	1491	rVB	345	204	0.02%	0.002%
34	6.147	1492	1495	1500	rVB2	352	262	0.02%	0.003%
35	6.250	1513	1527	1554	rBV	379012	729883	63.30%	7.724%
36	6.536	1607	1616	1622	rBV6	1807	2680	0.23%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048166.D
 Acq On : 21 Apr 2022 12:38
 Operator : SY/MD
 Sample : N2486-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.691	1650	1664	1685	rBV	267180	525346	45.56%	5.559%
38	7.031	1766	1770	1772	rBV2	215	170	0.01%	0.002%
39	7.099	1785	1791	1796	rVB	259	271	0.02%	0.003%
40	7.186	1809	1818	1830	rVB6	2464	4669	0.40%	0.049%
41	7.565	1924	1936	1958	rBV	122347	217739	18.88%	2.304%
42	7.691	1968	1975	1981	rBV5	1590	2428	0.21%	0.026%
43	7.768	1997	1999	2002	rBV2	313	167	0.01%	0.002%
44	7.787	2002	2005	2006	rBV2	322	237	0.02%	0.003%
45	7.900	2026	2040	2055	rBV	506012	869927	75.45%	9.206%
46	8.134	2109	2113	2115	rBV3	284	180	0.02%	0.002%
47	8.179	2115	2127	2143	rBV	88446	148501	12.88%	1.571%
48	8.440	2204	2208	2211	rBV4	280	258	0.02%	0.003%
49	8.485	2218	2222	2224	rVB2	269	186	0.02%	0.002%
50	8.562	2243	2246	2248	rBV2	280	155	0.01%	0.002%
51	8.633	2256	2268	2314	rBV	349796	673989	58.46%	7.132%
52	8.809	2321	2323	2325	rVB2	381	165	0.01%	0.002%
53	8.890	2344	2348	2351	rVV3	315	267	0.02%	0.003%
54	8.932	2358	2361	2366	rVB2	289	196	0.02%	0.002%
55	9.002	2379	2383	2387	rVB2	328	275	0.02%	0.003%
56	9.112	2413	2417	2420	rBV2	271	185	0.02%	0.002%
57	9.205	2442	2446	2449	rBV3	242	188	0.02%	0.002%
58	9.285	2467	2471	2475	rVB2	273	239	0.02%	0.003%
59	9.417	2497	2512	2546	rBV	581552	1028733	89.22%	10.886%
60	9.694	2592	2598	2609	rVB4	675	1083	0.09%	0.011%
61	10.022	2695	2700	2707	rVV2	194	275	0.02%	0.003%
62	10.099	2722	2724	2734	rVB3	405	364	0.03%	0.004%
63	10.141	2734	2737	2740	rVB	264	159	0.01%	0.002%
64	10.192	2748	2753	2755	rBV2	227	167	0.01%	0.002%
65	10.256	2768	2773	2776	rBV	183	203	0.02%	0.002%
66	10.369	2804	2808	2810	rBV2	219	173	0.02%	0.002%
67	10.568	2867	2870	2873	rVB	279	179	0.02%	0.002%
68	10.600	2873	2880	2884	rBV2	262	292	0.03%	0.003%
69	10.674	2896	2903	2911	rBV4	926	1108	0.10%	0.012%
70	10.758	2916	2929	2950	rBV	411449	660229	57.26%	6.987%
71	10.880	2963	2967	2972	rBV2	374	354	0.03%	0.004%
72	11.215	3066	3071	3074	rVB2	267	260	0.02%	0.003%
73	11.465	3140	3149	3159	rVV4	975	1809	0.16%	0.019%
74	11.507	3159	3162	3166	rVB	316	225	0.02%	0.002%
75	11.533	3168	3170	3174	rVV	240	186	0.02%	0.002%
76	11.568	3178	3181	3186	rVV2	203	230	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048166.D
 Acq On : 21 Apr 2022 12:38
 Operator : SY/MD
 Sample : N2486-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.600	3189	3191	3197	rVB3	220	190	0.02%	0.002%
78	11.645	3202	3205	3210	rVB2	333	308	0.03%	0.003%
79	11.697	3220	3221	3227	rVB2	431	208	0.02%	0.002%
80	11.748	3228	3237	3245	rBV3	2660	3566	0.31%	0.038%
81	11.813	3245	3257	3278	rBV	564701	941673	81.67%	9.965%
82	11.938	3294	3296	3299	rBV2	332	207	0.02%	0.002%
83	12.015	3315	3320	3324	rBV2	486	574	0.05%	0.006%
84	12.041	3325	3328	3331	rVV3	418	262	0.02%	0.003%
85	12.121	3351	3353	3360	rVB4	288	215	0.02%	0.002%
86	12.195	3362	3376	3394	rBV	505901	862159	74.78%	9.124%
87	12.594	3497	3500	3504	rVB2	310	218	0.02%	0.002%
88	12.706	3533	3535	3538	rVB2	418	235	0.02%	0.002%
89	12.726	3538	3541	3544	rBV2	451	341	0.03%	0.004%
90	12.861	3579	3583	3585	rBV	241	182	0.02%	0.002%
91	12.906	3595	3597	3601	rVB2	308	195	0.02%	0.002%
92	13.022	3630	3633	3636	rVB2	292	224	0.02%	0.002%
93	13.041	3636	3639	3640	rBV	406	250	0.02%	0.003%
94	13.121	3661	3664	3666	rBV	258	186	0.02%	0.002%
95	13.208	3687	3691	3694	rBV2	365	368	0.03%	0.004%
96	13.845	3880	3889	3901	rBV3	10527	16904	1.47%	0.179%
97	14.095	3963	3967	3972	rBV3	948	965	0.08%	0.010%
98	14.337	4035	4042	4052	rVB4	3291	4880	0.42%	0.052%
99	14.787	4180	4182	4184	rBV	554	280	0.02%	0.003%
100	15.218	4311	4316	4320	rBV4	705	851	0.07%	0.009%


Sum of corrected areas: 9449751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048166.D
Acq On : 21 Apr 2022 12:38
Operator : SY/MD
Sample : N2486-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

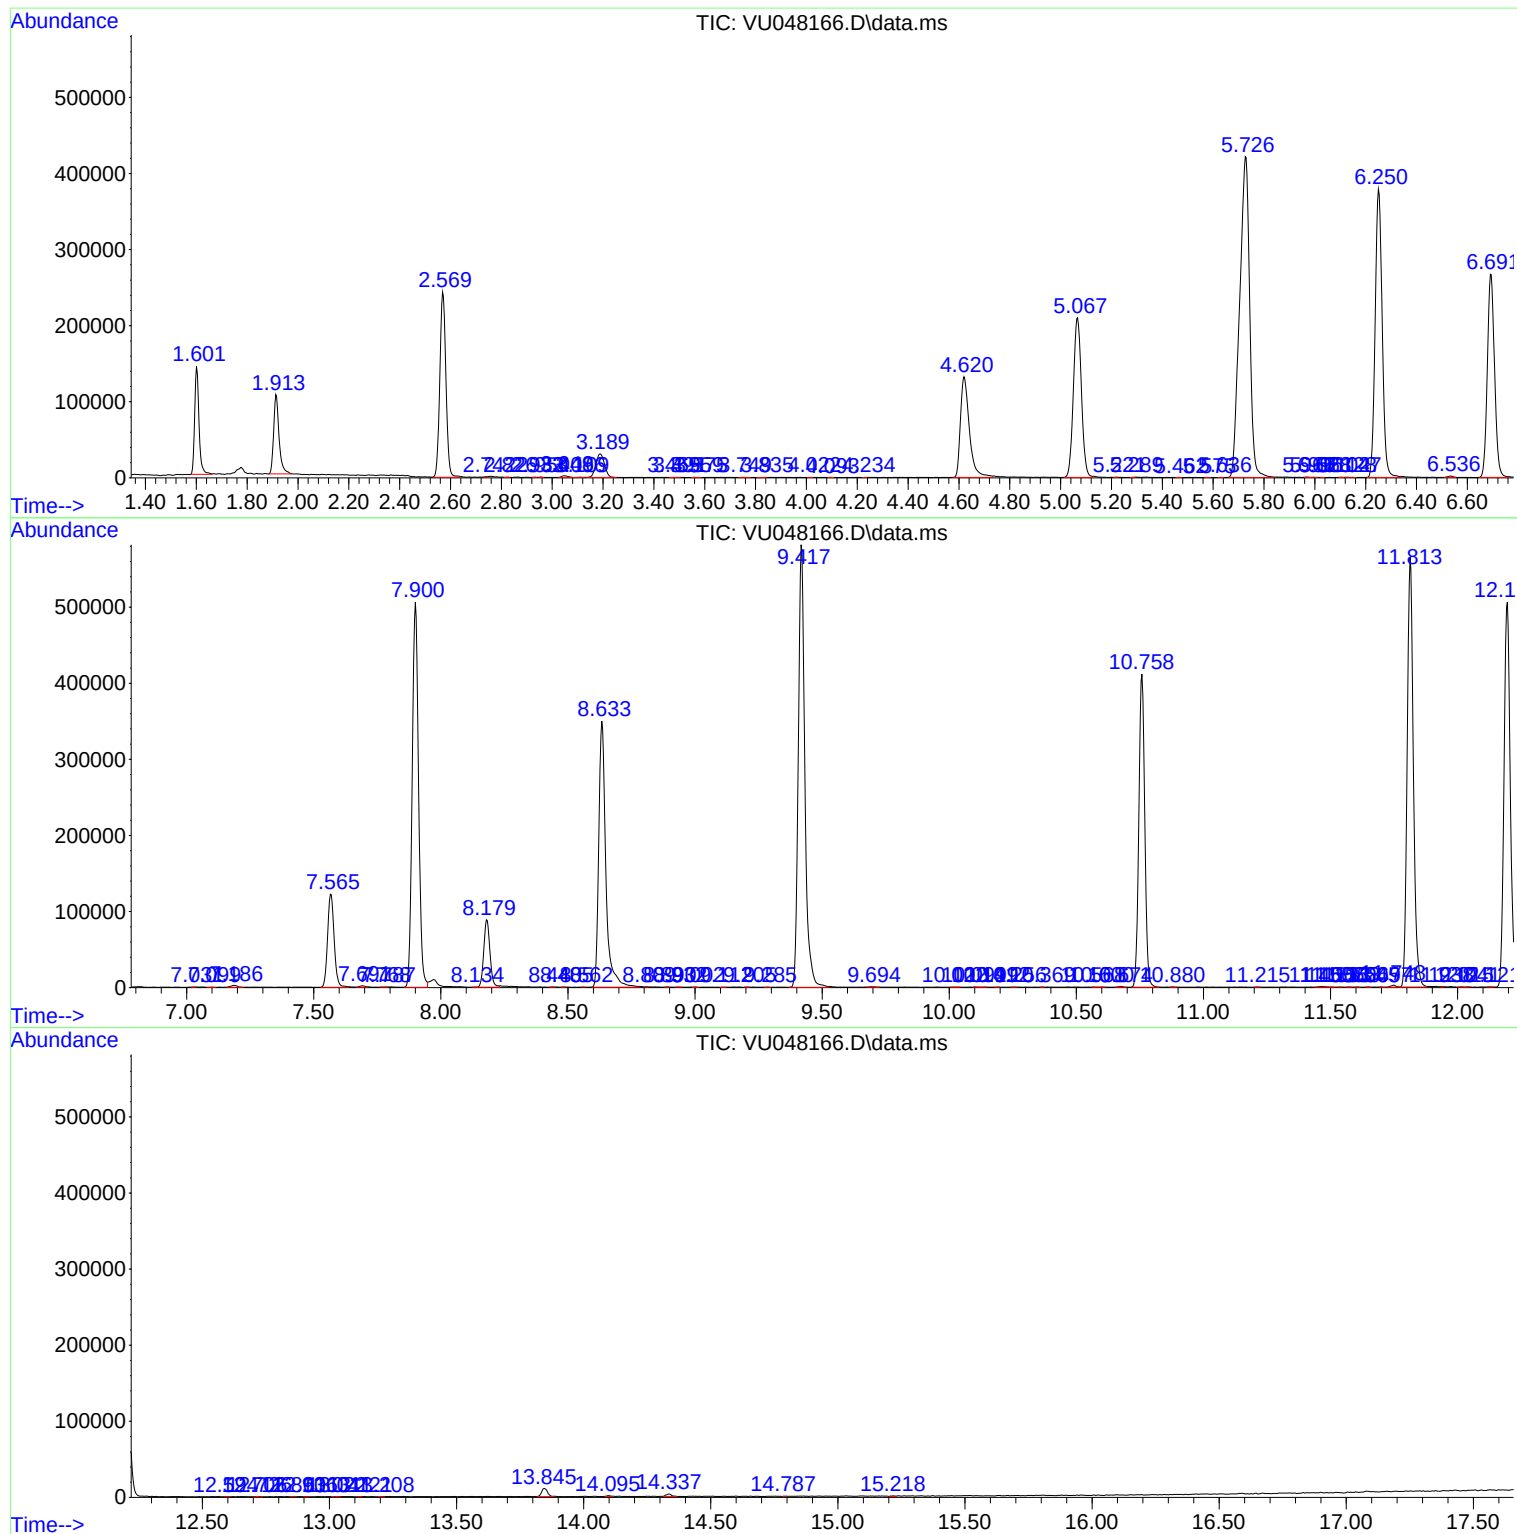

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048166.D
Acq On : 21 Apr 2022 12:38
Operator : SY/MD
Sample : N2486-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048166.D
Acq On : 21 Apr 2022 12:38
Operator : SY/MD
Sample : N2486-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------