

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048167.D
 Acq On : 21 Apr 2022 13:02
 Operator : SY/MD
 Sample : N2486-10 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rVB	134151	159480	14.27%	1.736%
2	1.912	171	178	197	rVB	103366	144853	12.96%	1.577%
3	2.568	370	382	399	rBV	236200	386940	34.62%	4.211%
4	3.051	524	532	544	rVB7	2117	3949	0.35%	0.043%
5	3.096	544	546	548	rBV	140	62	0.01%	0.001%
6	3.192	561	576	592	rVB2	11137	25573	2.29%	0.278%
7	3.295	604	608	610	rBV	231	186	0.02%	0.002%
8	3.330	616	619	621	rBV	346	178	0.02%	0.002%
9	3.427	647	649	652	rBV3	175	111	0.01%	0.001%
10	3.501	669	672	674	rBV	214	83	0.01%	0.001%
11	3.514	674	676	682	rVV2	166	129	0.01%	0.001%
12	3.639	713	715	717	rBV	163	87	0.01%	0.001%
13	3.726	739	742	745	rBV	189	157	0.01%	0.002%
14	3.809	766	768	770	rVB	127	51	0.00%	0.001%
15	3.883	789	791	794	rBV2	194	150	0.01%	0.002%
16	3.928	798	805	809	rBV2	171	174	0.02%	0.002%
17	3.954	809	813	819	rVB2	296	257	0.02%	0.003%
18	4.047	839	842	845	rBV2	193	143	0.01%	0.002%
19	4.157	873	876	878	rBV	262	144	0.01%	0.002%
20	4.205	888	891	893	rBV	167	111	0.01%	0.001%
21	4.266	907	910	915	rBV	181	193	0.02%	0.002%
22	4.353	934	937	943	rVB	259	273	0.02%	0.003%
23	4.420	955	958	961	rBV2	211	162	0.01%	0.002%
24	4.552	996	999	1001	rVB	217	96	0.01%	0.001%
25	4.626	1001	1022	1060	rBV2	140383	365672	32.72%	3.980%
26	5.067	1142	1159	1179	rBV	205425	451023	40.35%	4.909%
27	5.231	1206	1210	1213	rBB3	347	228	0.02%	0.002%
28	5.247	1213	1215	1218	rBV2	194	112	0.01%	0.001%
29	5.263	1218	1220	1224	rVB2	232	114	0.01%	0.001%
30	5.295	1224	1230	1237	rVB3	828	1262	0.11%	0.014%
31	5.337	1237	1243	1247	rBV2	299	277	0.02%	0.003%
32	5.366	1248	1252	1253	rBV	174	130	0.01%	0.001%
33	5.398	1259	1262	1265	rBV2	178	118	0.01%	0.001%
34	5.427	1268	1271	1273	rBV2	115	72	0.01%	0.001%
35	5.549	1307	1309	1311	rBV	109	55	0.00%	0.001%
36	5.587	1319	1321	1324	rVB	124	65	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048167.D
 Acq On : 21 Apr 2022 13:02
 Operator : SY/MD
 Sample : N2486-10 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.607	1324	1327	1329	rBV	129	70	0.01%	0.001%
38	5.626	1330	1333	1336	rBV	154	111	0.01%	0.001%
39	5.729	1343	1365	1391	rBV2	411369	1117731	100.00%	12.165%
40	6.189	1507	1508	1509	rBV	127	34	0.00%	0.000%
41	6.250	1512	1527	1556	rBV	366882	711700	63.67%	7.746%
42	6.530	1607	1614	1623	rBV4	1470	2412	0.22%	0.026%
43	6.694	1649	1665	1690	rBV	258266	506663	45.33%	5.514%
44	6.935	1737	1740	1742	rBV	208	93	0.01%	0.001%
45	7.018	1762	1766	1768	rBV	226	159	0.01%	0.002%
46	7.102	1790	1792	1794	rBV	162	70	0.01%	0.001%
47	7.182	1809	1817	1829	rBV7	2336	4354	0.39%	0.047%
48	7.324	1858	1861	1862	rBV	149	81	0.01%	0.001%
49	7.420	1887	1891	1894	rBV2	240	161	0.01%	0.002%
50	7.468	1904	1906	1909	rBV	227	147	0.01%	0.002%
51	7.568	1923	1937	1958	rBV	119795	212710	19.03%	2.315%
52	7.693	1969	1976	1984	rVB5	1548	2546	0.23%	0.028%
53	7.758	1994	1996	2001	rBV2	297	235	0.02%	0.003%
54	7.835	2016	2020	2023	rVB2	360	235	0.02%	0.003%
55	7.854	2023	2026	2027	rBV	201	118	0.01%	0.001%
56	7.899	2027	2040	2056	rBV	488419	842034	75.33%	9.165%
57	8.105	2102	2104	2107	rBV2	256	150	0.01%	0.002%
58	8.179	2116	2127	2140	rBV	84300	143279	12.82%	1.559%
59	8.510	2227	2230	2233	rBV2	246	196	0.02%	0.002%
60	8.571	2247	2249	2250	rBV2	145	79	0.01%	0.001%
61	8.636	2257	2269	2299	rBV	365007	682842	61.09%	7.432%
62	8.986	2374	2378	2380	rBV3	195	157	0.01%	0.002%
63	9.028	2388	2391	2392	rBV2	182	84	0.01%	0.001%
64	9.121	2418	2420	2423	rVB2	134	74	0.01%	0.001%
65	9.140	2424	2426	2429	rVV2	207	93	0.01%	0.001%
66	9.156	2429	2431	2435	rVV2	369	205	0.02%	0.002%
67	9.198	2441	2444	2446	rBV	175	105	0.01%	0.001%
68	9.230	2451	2454	2456	rVV	230	173	0.02%	0.002%
69	9.417	2499	2512	2549	rBV	556036	985148	88.14%	10.722%
70	9.693	2594	2598	2612	rVB4	831	1155	0.10%	0.013%
71	9.816	2632	2636	2638	rBV	159	128	0.01%	0.001%
72	10.279	2777	2780	2783	rVB2	258	171	0.02%	0.002%
73	10.330	2793	2796	2799	rBV	161	112	0.01%	0.001%
74	10.594	2875	2878	2879	rBV2	282	157	0.01%	0.002%
75	10.674	2891	2903	2909	rBV5	1340	1874	0.17%	0.020%
76	10.758	2916	2929	2949	rBV	402230	646518	57.84%	7.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048167.D
 Acq On : 21 Apr 2022 13:02
 Operator : SY/MD
 Sample : N2486-10 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.002	3004	3005	3006	rBV	116	31	0.00%	0.000%
78	11.012	3006	3008	3009	rBV	245	98	0.01%	0.001%
79	11.098	3032	3035	3041	rVB	301	217	0.02%	0.002%
80	11.198	3063	3066	3067	rBV	283	151	0.01%	0.002%
81	11.465	3143	3149	3150	rBV2	668	595	0.05%	0.006%
82	11.745	3230	3236	3244	rBV4	1843	2440	0.22%	0.027%
83	11.812	3244	3257	3280	rBV	565156	929651	83.17%	10.118%
84	11.963	3302	3304	3306	rBV2	503	212	0.02%	0.002%
85	12.192	3363	3375	3393	rBV	494278	838537	75.02%	9.127%
86	13.844	3883	3889	3902	rVB4	5842	8868	0.79%	0.097%


Sum of corrected areas: 9187834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048167.D
Acq On : 21 Apr 2022 13:02
Operator : SY/MD
Sample : N2486-10 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

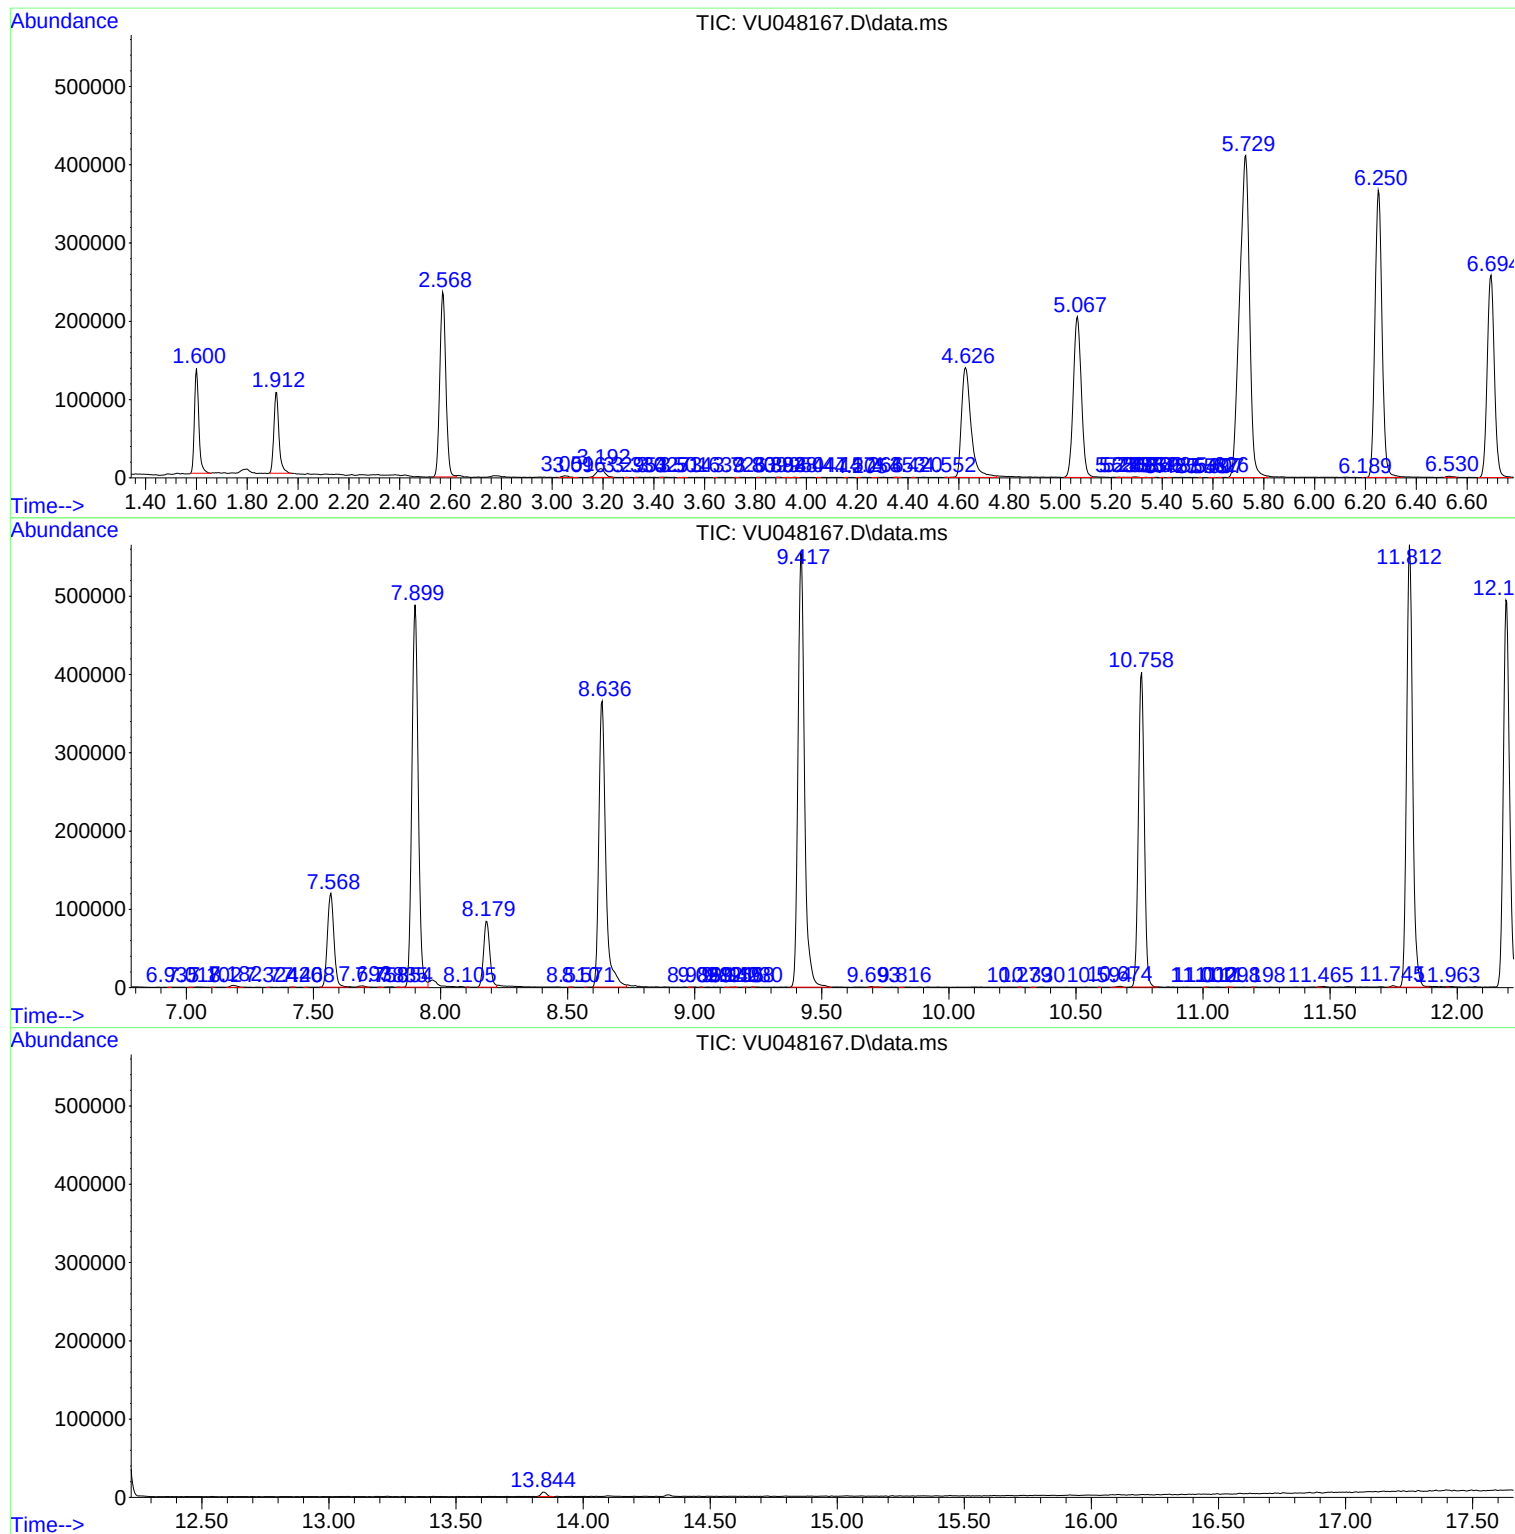

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048167.D
Acq On : 21 Apr 2022 13:02
Operator : SY/MD
Sample : N2486-10 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048167.D
Acq On : 21 Apr 2022 13:02
Operator : SY/MD
Sample : N2486-10 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------