

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048170.D
 Acq On : 21 Apr 2022 14:11
 Operator : SY/MD
 Sample : N2486-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rVB	133451	158409	4.11%	0.975%
2	1.912	170	178	200	rVB	106683	150942	3.92%	0.929%
3	2.568	370	382	397	rBV	234088	387464	10.05%	2.385%
4	2.687	416	419	424	rVB2	417	368	0.01%	0.002%
5	2.777	437	447	451	rBV4	2411	4489	0.12%	0.028%
6	2.883	474	480	483	rBV3	518	587	0.02%	0.004%
7	2.906	484	487	491	rVV	352	249	0.01%	0.002%
8	2.964	502	505	511	rVB	292	269	0.01%	0.002%
9	2.996	511	515	517	rVB2	396	257	0.01%	0.002%
10	3.051	522	532	542	rVB5	2232	4304	0.11%	0.026%
11	3.137	555	559	561	rBV2	316	205	0.01%	0.001%
12	3.186	561	574	594	rVB	9332	22421	0.58%	0.138%
13	3.269	598	600	608	rVB2	257	281	0.01%	0.002%
14	3.501	666	672	673	rBV2	240	235	0.01%	0.001%
15	3.633	710	713	718	rBV2	270	339	0.01%	0.002%
16	3.658	718	721	725	rVB2	323	259	0.01%	0.002%
17	3.700	731	734	740	rVB3	309	314	0.01%	0.002%
18	3.796	757	764	767	rBV2	260	242	0.01%	0.001%
19	4.096	852	857	858	rBV2	261	238	0.01%	0.001%
20	4.105	858	860	867	rVB2	217	217	0.01%	0.001%
21	4.327	923	929	931	rBV2	289	313	0.01%	0.002%
22	4.475	972	975	980	rVB2	218	206	0.01%	0.001%
23	4.504	980	984	988	rBV2	237	215	0.01%	0.001%
24	4.536	992	994	998	rVB	434	228	0.01%	0.001%
25	4.568	998	1004	1007	rBV	374	486	0.01%	0.003%
26	4.623	1007	1021	1058	rBV	133693	338819	8.79%	2.086%
27	4.845	1088	1090	1095	rVB2	550	358	0.01%	0.002%
28	5.063	1142	1158	1182	rBV2	204168	455131	11.81%	2.802%
29	5.282	1222	1226	1227	rBV2	517	307	0.01%	0.002%
30	5.385	1252	1258	1260	rBV2	239	207	0.01%	0.001%
31	5.530	1293	1303	1311	rVV4	1309	2603	0.07%	0.016%
32	5.726	1341	1364	1373	rBV2	411960	1123185	29.13%	6.915%
33	6.163	1498	1500	1504	rVB	271	192	0.00%	0.001%
34	6.192	1504	1509	1511	rBV2	251	217	0.01%	0.001%
35	6.250	1512	1527	1551	rBV	383379	729604	18.93%	4.492%
36	6.423	1577	1581	1585	rVB2	427	347	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048170.D
 Acq On : 21 Apr 2022 14:11
 Operator : SY/MD
 Sample : N2486-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.478	1593	1598	1603	rBV2	375	535	0.01%	0.003%
38	6.526	1607	1613	1624	rVV4	1677	3040	0.08%	0.019%
39	6.693	1647	1665	1685	rBV	262379	513158	13.31%	3.159%
40	6.874	1718	1721	1726	rBV3	222	249	0.01%	0.002%
41	7.044	1769	1774	1777	rBV2	329	316	0.01%	0.002%
42	7.185	1810	1818	1829	rBV4	2407	4337	0.11%	0.027%
43	7.243	1834	1836	1842	rVB	285	207	0.01%	0.001%
44	7.288	1846	1850	1853	rBV	234	203	0.01%	0.001%
45	7.446	1893	1899	1903	rBV2	313	419	0.01%	0.003%
46	7.497	1912	1915	1920	rVB2	267	286	0.01%	0.002%
47	7.568	1920	1937	1959	rBV	120644	214102	5.55%	1.318%
48	7.648	1959	1962	1963	rVV	474	317	0.01%	0.002%
49	7.658	1963	1965	1968	rVV3	526	422	0.01%	0.003%
50	7.687	1968	1974	1986	rVB3	1522	2851	0.07%	0.018%
51	7.800	2006	2009	2011	rVB2	388	214	0.01%	0.001%
52	7.899	2026	2040	2056	rBV	497529	859544	22.30%	5.292%
53	8.134	2110	2113	2115	rVB	323	208	0.01%	0.001%
54	8.179	2115	2127	2143	rBV	85929	147945	3.84%	0.911%
55	8.427	2201	2204	2208	rVV2	293	219	0.01%	0.001%
56	8.632	2254	2268	2298	rBV	365039	679052	17.61%	4.180%
57	8.857	2335	2338	2340	rBV2	326	255	0.01%	0.002%
58	8.960	2365	2370	2373	rBV3	288	317	0.01%	0.002%
59	9.166	2428	2434	2439	rVB3	422	532	0.01%	0.003%
60	9.446	2499	2521	2564	rBV2	1770881	3855189	100.00%	23.734%
61	9.635	2577	2580	2584	rBV3	515	342	0.01%	0.002%
62	9.690	2594	2597	2606	rVB2	1161	1466	0.04%	0.009%
63	9.767	2618	2621	2627	rVB4	441	407	0.01%	0.003%
64	10.279	2775	2780	2788	rBV3	394	545	0.01%	0.003%
65	10.417	2819	2823	2827	rBV	235	230	0.01%	0.001%
66	10.555	2863	2866	2872	rVB	300	236	0.01%	0.001%
67	10.671	2895	2902	2909	rBV3	1017	1413	0.04%	0.009%
68	10.758	2916	2929	2953	rVB	402321	650549	16.87%	4.005%
69	10.848	2953	2957	2960	rBV2	443	404	0.01%	0.002%
70	10.864	2960	2962	2966	rVB2	338	192	0.00%	0.001%
71	11.082	3026	3030	3037	rVB	437	481	0.01%	0.003%
72	11.115	3037	3040	3043	rBV	364	279	0.01%	0.002%
73	11.272	3086	3089	3096	rBV	176	244	0.01%	0.002%
74	11.307	3096	3100	3105	rVV	253	247	0.01%	0.002%
75	11.462	3143	3148	3150	rBV2	580	576	0.01%	0.004%
76	11.523	3164	3167	3170	rVB	334	220	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048170.D
 Acq On : 21 Apr 2022 14:11
 Operator : SY/MD
 Sample : N2486-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.668	3209	3212	3217	rBV3	498	539	0.01%	0.003%
78	11.693	3217	3220	3224	rVB2	521	345	0.01%	0.002%
79	11.745	3225	3236	3246	rBV	79484	127784	3.31%	0.787%
80	11.835	3246	3264	3281	rVB2	963605	2361915	61.27%	14.541%
81	11.931	3292	3294	3302	rVB5	1016	867	0.02%	0.005%
82	12.008	3315	3318	3323	rVB2	300	247	0.01%	0.002%
83	12.066	3331	3336	3338	rBV2	351	307	0.01%	0.002%
84	12.111	3347	3350	3356	rVB2	379	381	0.01%	0.002%
85	12.143	3356	3360	3362	rBV3	299	224	0.01%	0.001%
86	12.208	3362	3380	3397	rBV2	1055202	2341850	60.75%	14.417%
87	12.282	3401	3403	3406	rVB3	869	443	0.01%	0.003%
88	12.401	3438	3440	3444	rVB3	513	273	0.01%	0.002%
89	12.539	3481	3483	3486	rBV2	284	219	0.01%	0.001%
90	12.606	3500	3504	3506	rBV3	327	276	0.01%	0.002%
91	12.976	3611	3619	3627	rBV5	3918	6396	0.17%	0.039%
92	13.147	3668	3672	3673	rBV2	876	644	0.02%	0.004%
93	13.333	3722	3730	3736	rBV2	2339	2817	0.07%	0.017%
94	13.475	3771	3774	3779	rBV3	334	327	0.01%	0.002%
95	13.841	3875	3888	3909	rBV	528480	848296	22.00%	5.222%
96	14.221	4003	4006	4009	rBV	438	377	0.01%	0.002%
97	14.330	4029	4040	4056	rBV	128886	211372	5.48%	1.301%
98	15.204	4309	4312	4316	rVB4	603	466	0.01%	0.003%
99	15.243	4322	4324	4326	rBV2	494	273	0.01%	0.002%
100	16.002	4552	4560	4570	rBV3	6507	10597	0.27%	0.065%




Sum of corrected areas: 16243490

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048170.D
Acq On : 21 Apr 2022 14:11
Operator : SY/MD
Sample : N2486-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

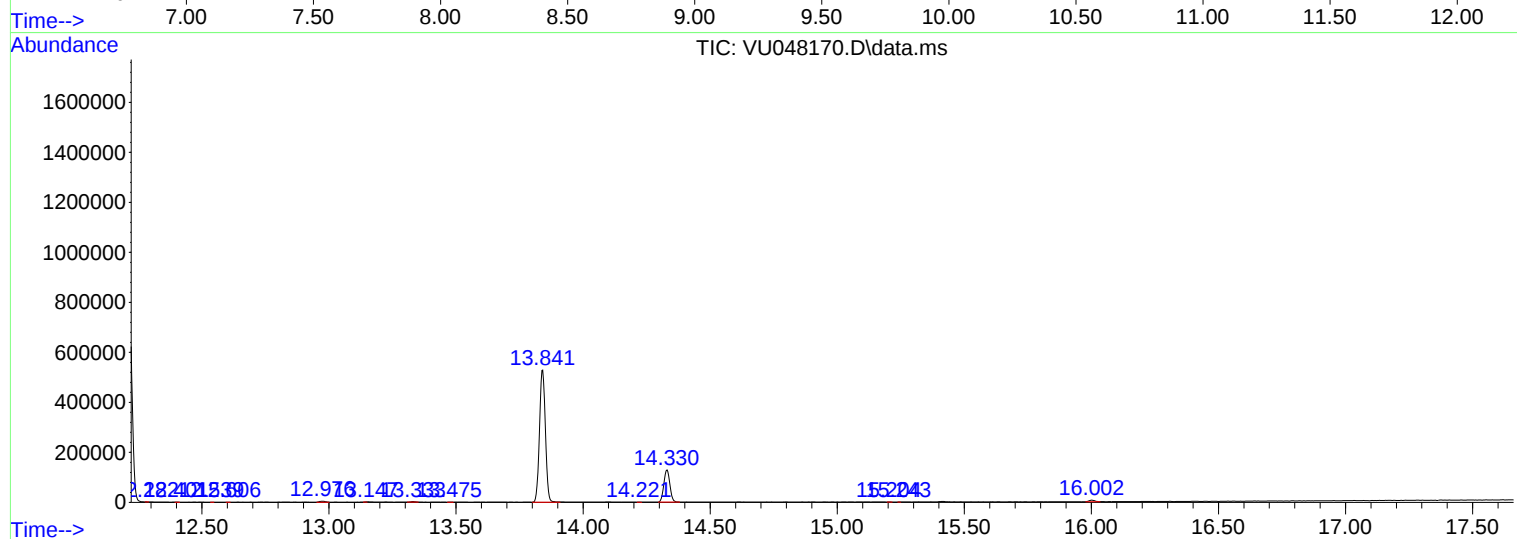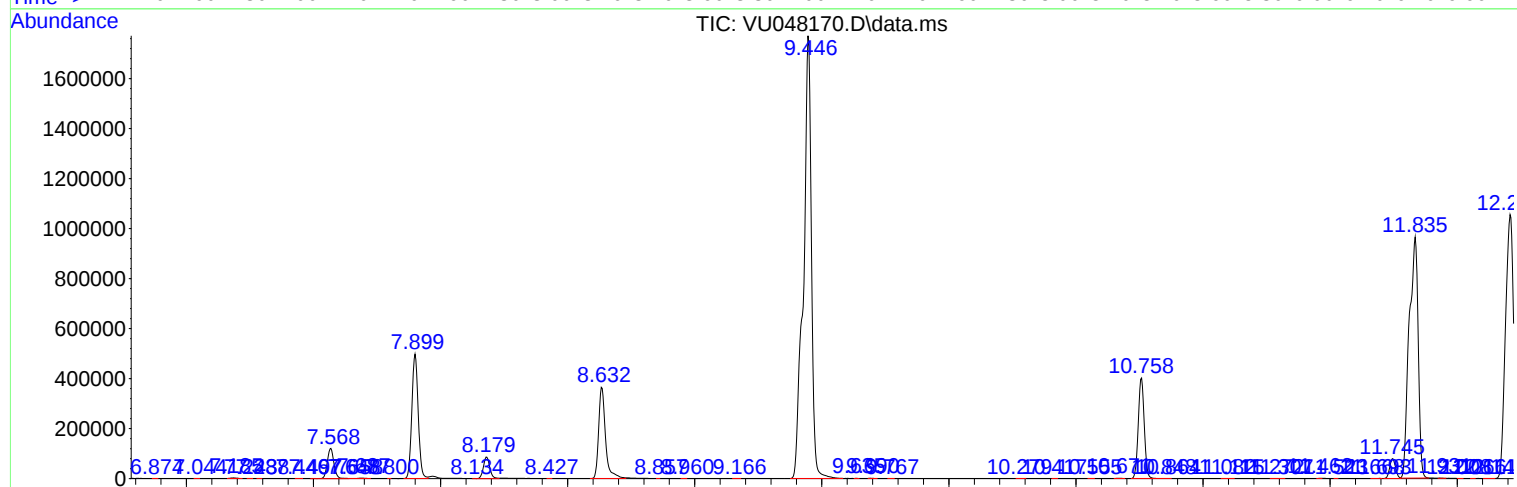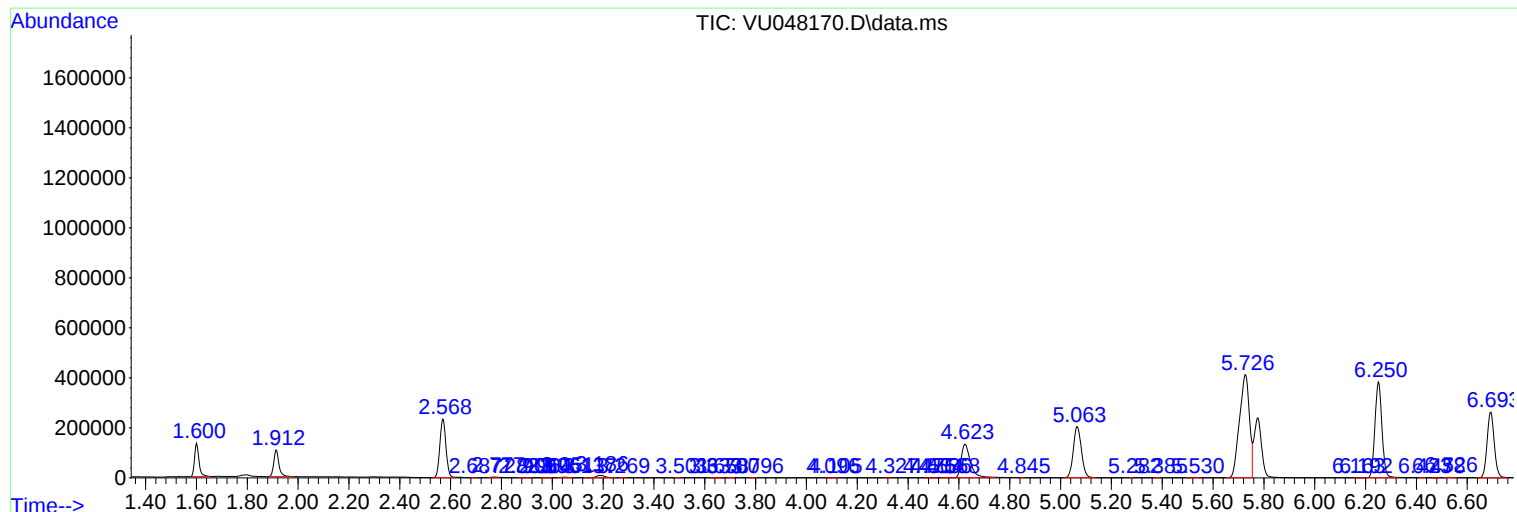

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048170.D
Acq On : 21 Apr 2022 14:11
Operator : SY/MD
Sample : N2486-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048170.D
Acq On : 21 Apr 2022 14:11
Operator : SY/MD
Sample : N2486-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------