

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048172.D
 Acq On : 21 Apr 2022 14:56
 Operator : SY/MD
 Sample : N2486-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rBV	135761	161974	2.56%	0.674%
2	1.912	170	178	204	rVB	107611	153715	2.43%	0.640%
3	2.568	369	382	397	rBV	236660	392298	6.20%	1.633%
4	2.710	424	426	428	rBV	307	188	0.00%	0.001%
5	2.729	428	432	435	rBV3	355	230	0.00%	0.001%
6	2.771	437	445	446	rBV4	2191	2266	0.04%	0.009%
7	2.867	471	475	477	rBV3	381	333	0.01%	0.001%
8	2.906	483	487	488	rBV2	419	266	0.00%	0.001%
9	2.954	498	502	505	rBV3	302	278	0.00%	0.001%
10	2.974	505	508	511	rVV3	323	273	0.00%	0.001%
11	3.044	525	530	531	rBB3	232	341	0.01%	0.001%
12	3.093	541	545	550	rVB	344	298	0.00%	0.001%
13	3.118	550	553	557	rBV2	300	304	0.00%	0.001%
14	3.189	561	575	594	rVV2	11746	27021	0.43%	0.112%
15	3.263	594	598	602	rVB3	362	343	0.01%	0.001%
16	3.353	622	626	632	rBV3	273	251	0.00%	0.001%
17	3.472	659	663	666	rBV2	286	271	0.00%	0.001%
18	3.568	689	693	698	rBV2	294	281	0.00%	0.001%
19	3.613	703	707	712	rBV	244	219	0.00%	0.001%
20	3.652	716	719	723	rVB2	290	240	0.00%	0.001%
21	3.681	723	728	729	rBV	450	315	0.00%	0.001%
22	3.829	769	774	780	rVB2	298	270	0.00%	0.001%
23	4.273	910	912	917	rVB2	268	197	0.00%	0.001%
24	4.321	919	927	929	rBV2	246	375	0.01%	0.002%
25	4.379	940	945	950	rVV2	282	373	0.01%	0.002%
26	4.514	984	987	989	rBV2	254	185	0.00%	0.001%
27	4.626	1006	1022	1048	rBV2	135473	346039	5.47%	1.441%
28	4.813	1077	1080	1083	rVB2	488	328	0.01%	0.001%
29	4.925	1112	1115	1120	rVB2	288	285	0.00%	0.001%
30	5.002	1135	1139	1142	rBV2	568	513	0.01%	0.002%
31	5.067	1142	1159	1186	rVV	207249	462749	7.31%	1.926%
32	5.192	1195	1198	1201	rVB3	562	362	0.01%	0.002%
33	5.292	1226	1229	1232	rBV3	255	234	0.00%	0.001%
34	5.346	1243	1246	1252	rVB2	262	229	0.00%	0.001%
35	5.469	1274	1284	1291	rBV	209	338	0.01%	0.001%
36	5.526	1291	1302	1313	rBV4	2553	5155	0.08%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048172.D
 Acq On : 21 Apr 2022 14:56
 Operator : SY/MD
 Sample : N2486-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.726	1343	1364	1372	rBV2	420343	1121815	17.72%	4.670%
38	6.041	1459	1462	1465	rVV3	358	265	0.00%	0.001%
39	6.063	1465	1469	1472	rVB3	402	304	0.00%	0.001%
40	6.134	1489	1491	1498	rVB2	508	355	0.01%	0.001%
41	6.250	1512	1527	1550	rBV	375911	713642	11.27%	2.971%
42	6.462	1591	1593	1596	rVB3	299	192	0.00%	0.001%
43	6.533	1607	1615	1623	rVV4	1587	2494	0.04%	0.010%
44	6.642	1646	1649	1650	rBV	286	192	0.00%	0.001%
45	6.694	1650	1665	1692	rBV	263124	514847	8.13%	2.143%
46	6.809	1697	1701	1707	rBV3	943	959	0.02%	0.004%
47	7.018	1760	1766	1770	rBV2	368	464	0.01%	0.002%
48	7.070	1780	1782	1791	rVB2	285	284	0.00%	0.001%
49	7.186	1810	1818	1830	rBV3	2283	3892	0.06%	0.016%
50	7.272	1842	1845	1851	rVB3	282	185	0.00%	0.001%
51	7.343	1863	1867	1872	rBV3	285	245	0.00%	0.001%
52	7.372	1872	1876	1879	rBV2	220	199	0.00%	0.001%
53	7.404	1883	1886	1892	rBV4	337	363	0.01%	0.002%
54	7.568	1924	1937	1953	rVV	122896	216267	3.42%	0.900%
55	7.645	1959	1961	1966	rVB2	484	297	0.00%	0.001%
56	7.687	1966	1974	1987	rVB4	1978	3587	0.06%	0.015%
57	7.825	2014	2017	2024	rVB2	269	194	0.00%	0.001%
58	7.899	2024	2040	2056	rBV	509174	869461	13.73%	3.620%
59	8.134	2110	2113	2116	rVB2	379	226	0.00%	0.001%
60	8.179	2116	2127	2141	rBV	86244	146994	2.32%	0.612%
61	8.369	2184	2186	2191	rVB2	340	278	0.00%	0.001%
62	8.488	2221	2223	2224	rBV	376	191	0.00%	0.001%
63	8.636	2256	2269	2303	rBV	373190	694189	10.97%	2.890%
64	8.967	2370	2372	2379	rVB3	351	335	0.01%	0.001%
65	9.166	2430	2434	2440	rVV3	522	533	0.01%	0.002%
66	9.446	2499	2521	2555	rBV2	1902508	4068685	64.27%	16.938%
67	9.636	2578	2580	2582	rBV2	374	209	0.00%	0.001%
68	9.690	2591	2597	2599	rBV4	985	822	0.01%	0.003%
69	9.771	2619	2622	2625	rVB2	335	187	0.00%	0.001%
70	9.812	2629	2635	2637	rBV3	299	263	0.00%	0.001%
71	9.877	2653	2655	2658	rBV	331	193	0.00%	0.001%
72	10.025	2698	2701	2706	rVB3	250	231	0.00%	0.001%
73	10.102	2722	2725	2729	rVB2	326	211	0.00%	0.001%
74	10.671	2894	2902	2908	rBV4	1417	1648	0.03%	0.007%
75	10.758	2916	2929	2949	rVB	399658	652543	10.31%	2.717%
76	10.899	2971	2973	2978	rVB2	392	261	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048172.D
 Acq On : 21 Apr 2022 14:56
 Operator : SY/MD
 Sample : N2486-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.989	2998	3001	3008	rVB2	498	584	0.01%	0.002%
78	11.063	3020	3024	3027	rBV2	374	291	0.00%	0.001%
79	11.208	3061	3069	3070	rBV2	385	395	0.01%	0.002%
80	11.465	3142	3149	3151	rBV3	582	709	0.01%	0.003%
81	11.684	3214	3217	3219	rBV2	583	378	0.01%	0.002%
82	11.700	3219	3222	3224	rVV2	354	199	0.00%	0.001%
83	11.745	3224	3236	3247	rVV	503480	803155	12.69%	3.344%
84	11.835	3247	3264	3286	rVB2	2675826	5089658	80.40%	21.188%
85	12.034	3322	3326	3329	rVB3	566	441	0.01%	0.002%
86	12.054	3329	3332	3335	rBV3	345	219	0.00%	0.001%
87	12.211	3362	3381	3401	rBV2	3487953	6330451	100.00%	26.354%
88	12.481	3462	3465	3467	rBV	296	229	0.00%	0.001%
89	12.568	3489	3492	3493	rBV2	371	231	0.00%	0.001%
90	12.861	3575	3583	3586	rBV3	394	549	0.01%	0.002%
91	12.973	3610	3618	3626	rVB4	3913	5899	0.09%	0.025%
92	13.050	3639	3642	3647	rBV3	344	311	0.00%	0.001%
93	13.111	3658	3661	3663	rBV3	303	191	0.00%	0.001%
94	13.140	3667	3670	3672	rBV	516	346	0.01%	0.001%
95	13.217	3686	3694	3703	rVB4	2151	3317	0.05%	0.014%
96	13.330	3721	3729	3737	rBV6	3035	4654	0.07%	0.019%
97	13.838	3875	3887	3913	rBV	552639	872974	13.79%	3.634%
98	14.330	4028	4040	4056	rBV	202004	321852	5.08%	1.340%
99	15.005	4248	4250	4253	rBV2	669	382	0.01%	0.002%
100	16.002	4554	4560	4567	rVB4	4392	5891	0.09%	0.025%



Sum of corrected areas: 24021145

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048172.D
Acq On : 21 Apr 2022 14:56
Operator : SY/MD
Sample : N2486-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

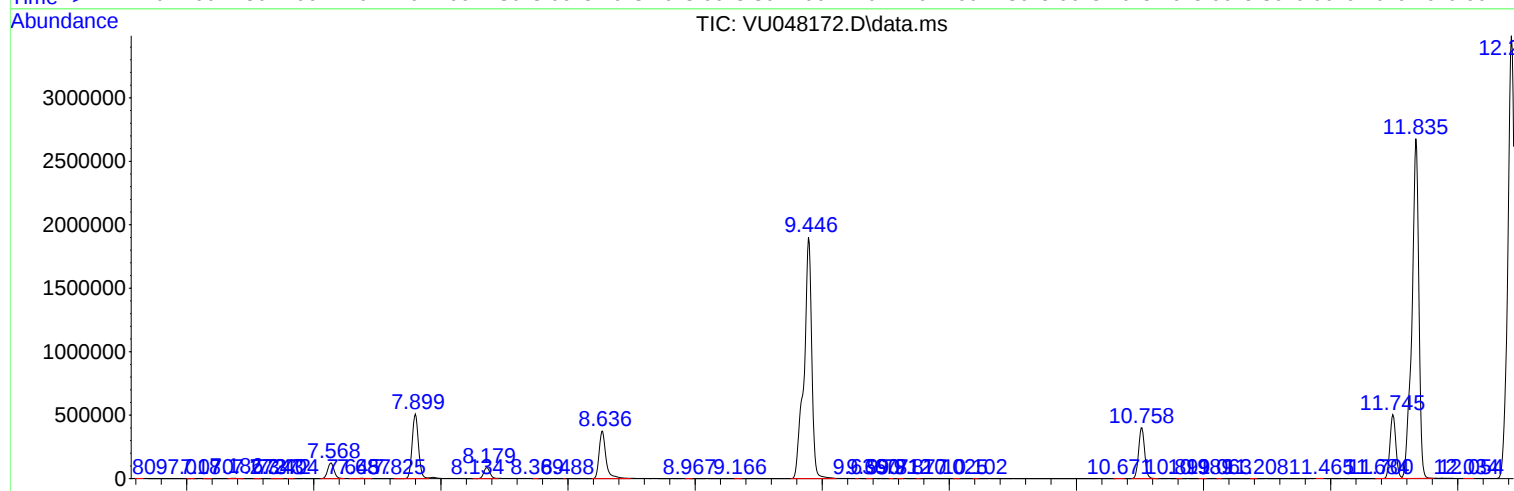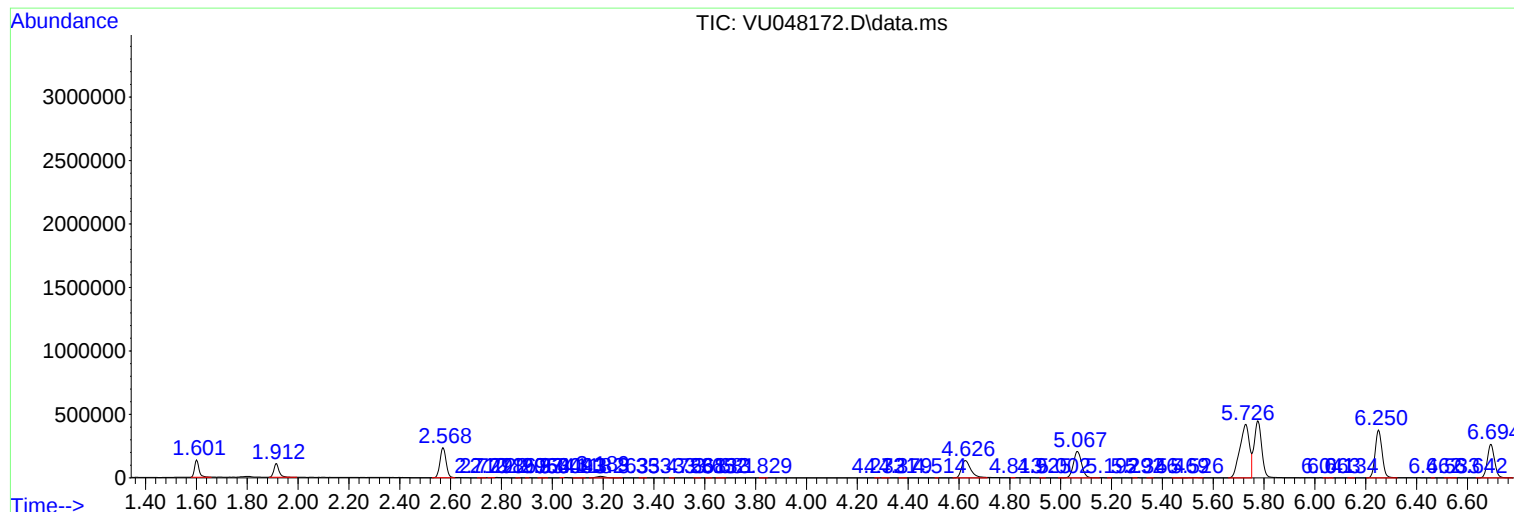

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048172.D
Acq On : 21 Apr 2022 14:56
Operator : SY/MD
Sample : N2486-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048172.D
Acq On : 21 Apr 2022 14:56
Operator : SY/MD
Sample : N2486-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------