

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048173.D
 Acq On : 21 Apr 2022 15:19
 Operator : SY/MD
 Sample : N2486-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	132261	159524	0.99%	0.357%
2	1.913	170	178	198	rVB	107649	153157	0.95%	0.343%
3	2.568	370	382	398	rBV	228464	379820	2.36%	0.850%
4	2.703	421	424	427	rVB2	365	215	0.00%	0.000%
5	2.726	427	431	432	rBV2	516	383	0.00%	0.001%
6	2.794	443	452	457	rBV3	2573	4292	0.03%	0.010%
7	3.022	520	523	524	rVV2	419	266	0.00%	0.001%
8	3.051	524	532	542	rVB5	2372	4328	0.03%	0.010%
9	3.125	552	555	556	rBV2	346	185	0.00%	0.000%
10	3.189	561	575	589	rVV	13289	30292	0.19%	0.068%
11	3.285	601	605	607	rVB3	483	296	0.00%	0.001%
12	3.359	626	628	635	rVB2	420	380	0.00%	0.001%
13	3.485	662	667	670	rVB2	198	198	0.00%	0.000%
14	3.511	670	675	680	rVB2	523	429	0.00%	0.001%
15	3.565	689	692	695	rBV2	241	191	0.00%	0.000%
16	3.594	698	701	709	rVB3	321	388	0.00%	0.001%
17	3.649	713	718	720	rBV3	409	419	0.00%	0.001%
18	3.761	748	753	756	rBV	229	229	0.00%	0.001%
19	3.797	761	764	766	rBV2	304	194	0.00%	0.000%
20	3.861	781	784	791	rVB3	328	290	0.00%	0.001%
21	4.134	866	869	873	rVB2	397	351	0.00%	0.001%
22	4.327	922	929	932	rBV2	246	292	0.00%	0.001%
23	4.375	941	944	950	rVB2	393	371	0.00%	0.001%
24	4.472	970	974	978	rBV	272	187	0.00%	0.000%
25	4.536	984	994	1001	rBV6	1306	2724	0.02%	0.006%
26	4.626	1006	1022	1055	rBV2	140833	375036	2.33%	0.840%
27	5.067	1142	1159	1183	rBV	207818	466265	2.89%	1.044%
28	5.163	1186	1189	1195	rVB3	477	449	0.00%	0.001%
29	5.189	1195	1197	1202	rVB3	318	262	0.00%	0.001%
30	5.285	1224	1227	1228	rBV2	769	434	0.00%	0.001%
31	5.350	1243	1247	1252	rBV2	296	391	0.00%	0.001%
32	5.388	1256	1259	1262	rVV3	283	196	0.00%	0.000%
33	5.530	1290	1303	1315	rVV3	6638	13121	0.08%	0.029%
34	5.588	1318	1321	1327	rVB2	202	206	0.00%	0.000%
35	5.629	1328	1334	1338	rBV	237	231	0.00%	0.001%
36	5.777	1368	1380	1427	rVB	7955499	16123583	100.00%	36.095%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048173.D
 Acq On : 21 Apr 2022 15:19
 Operator : SY/MD
 Sample : N2486-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1514	1527	1546	rVB	387598	724673	4.49%	1.622%
38	6.446	1585	1588	1595	rVB3	583	438	0.00%	0.001%
39	6.530	1607	1614	1615	rBV4	1255	1258	0.01%	0.003%
40	6.594	1629	1634	1636	rBV4	348	293	0.00%	0.001%
41	6.690	1650	1664	1687	rBV	258625	508922	3.16%	1.139%
42	6.803	1696	1699	1700	rBV3	368	202	0.00%	0.000%
43	7.038	1769	1772	1774	rBV2	310	197	0.00%	0.000%
44	7.189	1810	1819	1829	rBV2	2869	5047	0.03%	0.011%
45	7.343	1863	1867	1870	rBV2	240	186	0.00%	0.000%
46	7.359	1870	1872	1877	rVV3	280	222	0.00%	0.000%
47	7.404	1884	1886	1893	rVV3	252	228	0.00%	0.001%
48	7.565	1924	1936	1952	rVV	121028	214839	1.33%	0.481%
49	7.636	1956	1958	1959	rVV	725	351	0.00%	0.001%
50	7.649	1959	1962	1965	rVV2	842	646	0.00%	0.001%
51	7.690	1968	1975	1983	rVV4	1773	2967	0.02%	0.007%
52	7.803	2000	2010	2014	rBV3	728	983	0.01%	0.002%
53	7.851	2019	2025	2026	rBV	384	292	0.00%	0.001%
54	7.899	2026	2040	2055	rBV	492907	847424	5.26%	1.897%
55	8.179	2115	2127	2141	rBV	84788	145313	0.90%	0.325%
56	8.404	2193	2197	2202	rVB2	306	375	0.00%	0.001%
57	8.430	2202	2205	2207	rBV	366	315	0.00%	0.001%
58	8.462	2211	2215	2217	rBV	339	263	0.00%	0.001%
59	8.552	2240	2243	2250	rBV3	799	594	0.00%	0.001%
60	8.636	2256	2269	2301	rBV	385634	714839	4.43%	1.600%
61	8.845	2330	2334	2336	rBV2	309	213	0.00%	0.000%
62	8.903	2349	2352	2354	rBV	353	236	0.00%	0.001%
63	9.163	2430	2433	2440	rVB2	695	623	0.00%	0.001%
64	9.446	2499	2521	2565	rBV	8228158	14481293	89.81%	32.419%
65	9.639	2578	2581	2583	rBV2	389	244	0.00%	0.001%
66	9.684	2592	2595	2597	rBV3	681	477	0.00%	0.001%
67	9.700	2597	2600	2605	rVB3	1137	842	0.01%	0.002%
68	9.841	2642	2644	2648	rVB3	430	279	0.00%	0.001%
69	9.970	2679	2684	2687	rBV2	336	313	0.00%	0.001%
70	10.041	2704	2706	2713	rVB2	271	279	0.00%	0.001%
71	10.102	2721	2725	2728	rVB2	398	253	0.00%	0.001%
72	10.343	2795	2800	2803	rBV2	282	265	0.00%	0.001%
73	10.671	2899	2902	2909	rVV5	905	959	0.01%	0.002%
74	10.706	2909	2913	2916	rVB2	258	206	0.00%	0.000%
75	10.758	2916	2929	2948	rBV	404859	647343	4.01%	1.449%
76	10.867	2960	2963	2965	rBV	297	251	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048173.D
 Acq On : 21 Apr 2022 15:19
 Operator : SY/MD
 Sample : N2486-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.983	2995	2999	3000	rBV3	369	276	0.00%	0.001%
78	11.176	3056	3059	3061	rVB2	413	241	0.00%	0.001%
79	11.456	3140	3146	3147	rBV4	819	595	0.00%	0.001%
80	11.517	3163	3165	3170	rVB2	299	220	0.00%	0.000%
81	11.745	3225	3236	3246	rBV	112997	179210	1.11%	0.401%
82	11.835	3246	3264	3285	rVB2	2383756	4554196	28.25%	10.195%
83	12.031	3323	3325	3330	rBV3	302	258	0.00%	0.001%
84	12.211	3361	3381	3399	rBV2	1803408	3557215	22.06%	7.963%
85	12.382	3432	3434	3436	rBV2	490	277	0.00%	0.001%
86	12.462	3456	3459	3462	rBV2	509	438	0.00%	0.001%
87	12.632	3510	3512	3515	rVB2	554	333	0.00%	0.001%
88	12.652	3515	3518	3520	rBV2	353	251	0.00%	0.001%
89	12.816	3566	3569	3572	rBV3	486	369	0.00%	0.001%
90	12.838	3573	3576	3579	rBV3	271	196	0.00%	0.000%
91	12.944	3606	3609	3613	rBV3	287	263	0.00%	0.001%
92	13.044	3636	3640	3642	rBV2	345	252	0.00%	0.001%
93	13.218	3687	3694	3702	rVB5	1935	2950	0.02%	0.007%
94	13.800	3872	3875	3876	rBV	390	230	0.00%	0.001%
95	13.838	3876	3887	3911	rVB	185815	300660	1.86%	0.673%
96	13.925	3911	3914	3915	rBV2	475	255	0.00%	0.001%
97	14.330	4031	4040	4052	rVB2	28515	44930	0.28%	0.101%
98	14.517	4095	4098	4102	rVB4	521	427	0.00%	0.001%
99	14.722	4159	4162	4163	rBV2	453	207	0.00%	0.000%
100	15.057	4262	4266	4268	rBV2	711	529	0.00%	0.001%




Sum of corrected areas: 44669296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048173.D
Acq On : 21 Apr 2022 15:19
Operator : SY/MD
Sample : N2486-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

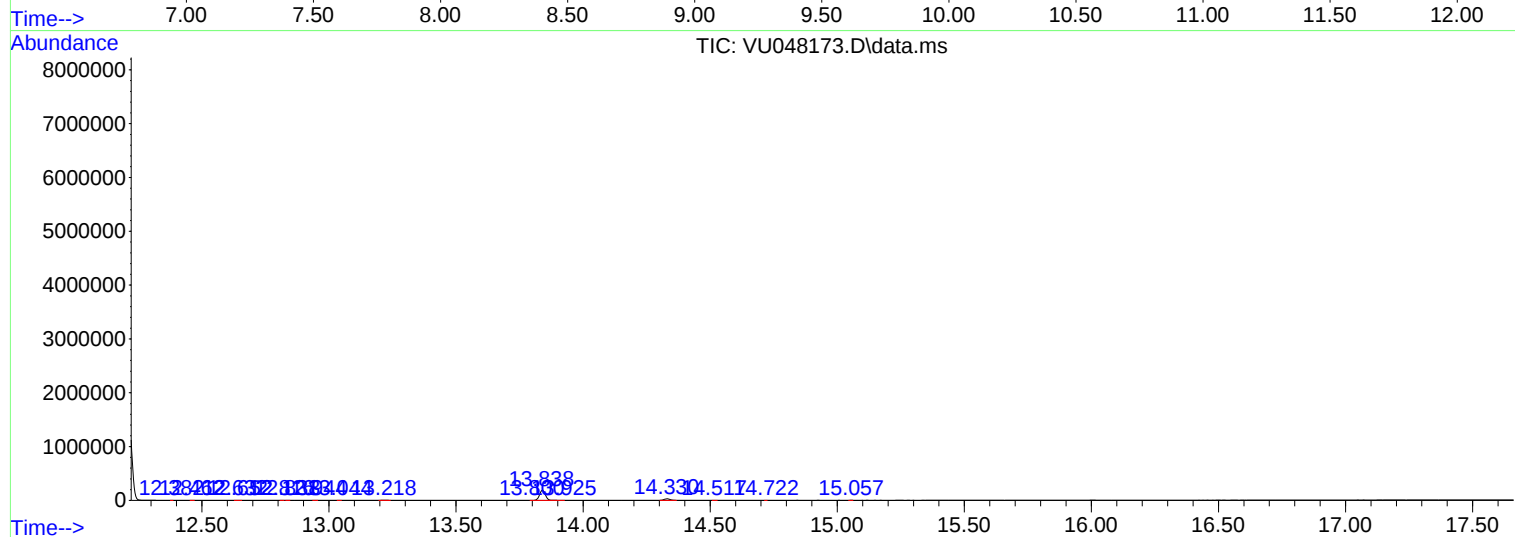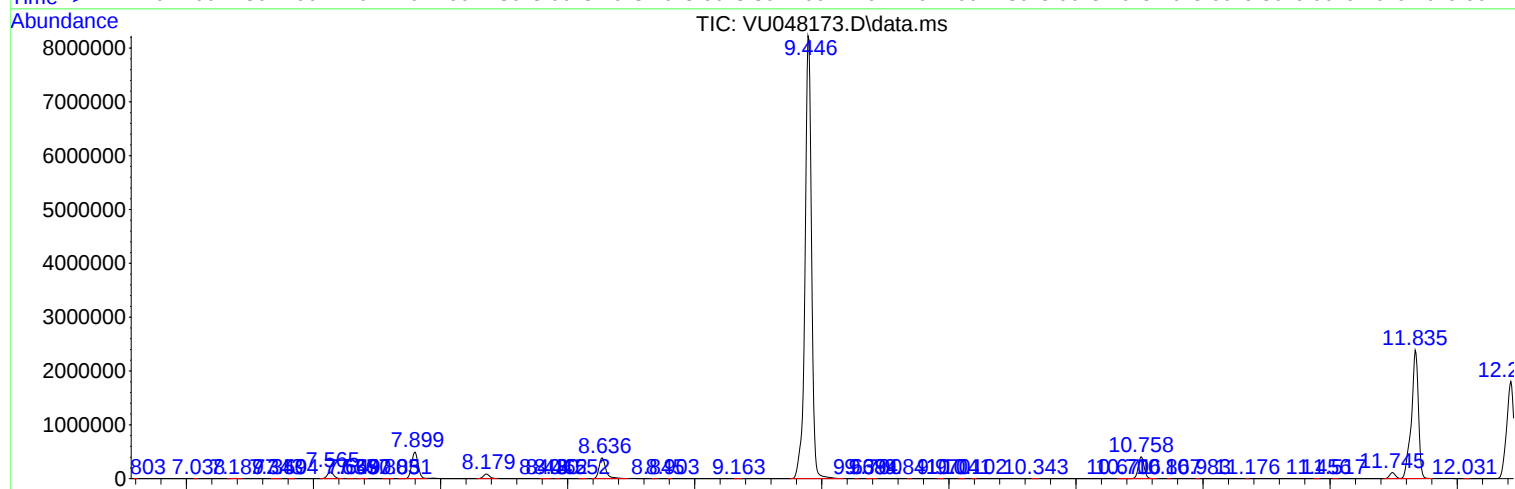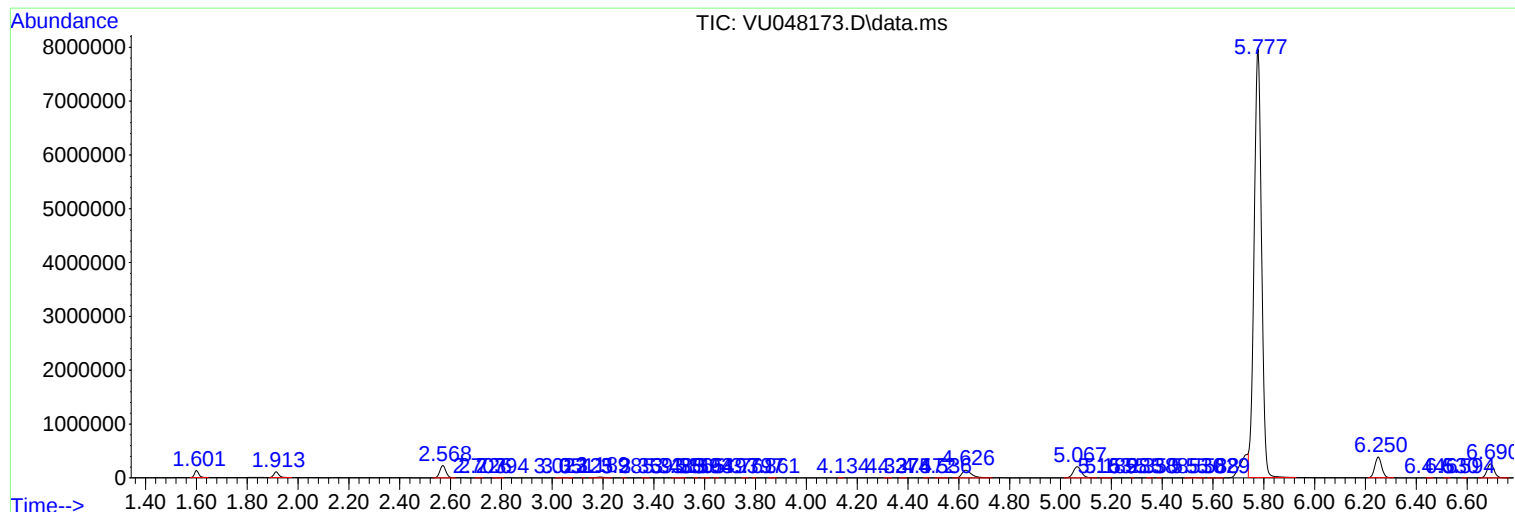

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048173.D
Acq On : 21 Apr 2022 15:19
Operator : SY/MD
Sample : N2486-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048173.D
Acq On : 21 Apr 2022 15:19
Operator : SY/MD
Sample : N2486-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc