

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048175.D
 Acq On : 21 Apr 2022 16:05
 Operator : SY/MD
 Sample : N2486-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	125471	146324	13.30%	1.643%
2	1.916	170	179	202	rVB	103941	147667	13.42%	1.659%
3	2.568	369	382	399	rBV	214207	358901	32.63%	4.031%
4	2.787	438	450	453	rBV	4869	8374	0.76%	0.094%
5	2.948	497	500	501	rBV	346	183	0.02%	0.002%
6	2.980	508	510	515	rVB2	389	301	0.03%	0.003%
7	3.006	515	518	523	rBV3	433	379	0.03%	0.004%
8	3.051	523	532	542	rVB3	2120	3460	0.31%	0.039%
9	3.105	545	549	551	rBV2	363	208	0.02%	0.002%
10	3.189	561	575	592	rBV2	11099	27013	2.46%	0.303%
11	3.295	600	608	609	rBV	225	296	0.03%	0.003%
12	3.327	614	618	621	rBV2	392	369	0.03%	0.004%
13	3.359	625	628	631	rBV2	336	240	0.02%	0.003%
14	3.417	641	646	648	rBV2	314	278	0.03%	0.003%
15	3.604	702	704	707	rVB	336	199	0.02%	0.002%
16	3.652	716	719	723	rVB2	265	180	0.02%	0.002%
17	3.671	723	725	728	rBV2	248	178	0.02%	0.002%
18	3.771	751	756	759	rBV2	235	208	0.02%	0.002%
19	3.809	767	768	775	rVB2	193	173	0.02%	0.002%
20	3.877	786	789	791	rBV	267	185	0.02%	0.002%
21	3.922	801	803	806	rBV	225	169	0.02%	0.002%
22	3.999	824	827	836	rVB2	234	334	0.03%	0.004%
23	4.124	861	866	869	rBV2	212	208	0.02%	0.002%
24	4.227	895	898	904	rVB2	267	354	0.03%	0.004%
25	4.256	904	907	912	rBV	281	353	0.03%	0.004%
26	4.356	934	938	941	rBV2	246	195	0.02%	0.002%
27	4.430	957	961	966	rVB2	209	195	0.02%	0.002%
28	4.481	973	977	982	rVB2	230	271	0.02%	0.003%
29	4.523	982	990	995	rBV2	293	460	0.04%	0.005%
30	4.552	995	999	1001	rBV2	261	171	0.02%	0.002%
31	4.629	1008	1023	1058	rBV2	137405	365135	33.20%	4.101%
32	4.925	1114	1115	1120	rBV3	285	171	0.02%	0.002%
33	5.067	1139	1159	1184	rBV	200788	440117	40.01%	4.943%
34	5.250	1212	1216	1219	rBV	881	859	0.08%	0.010%
35	5.295	1224	1230	1236	rVB3	598	934	0.08%	0.010%
36	5.378	1253	1256	1262	rVB2	333	325	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048175.D
 Acq On : 21 Apr 2022 16:05
 Operator : SY/MD
 Sample : N2486-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.597	1320	1324	1327	rBV	184	176	0.02%	0.002%
38	5.729	1342	1365	1395	rBV2	396981	1099944	100.00%	12.354%
39	5.957	1432	1436	1439	rVB2	237	190	0.02%	0.002%
40	5.980	1439	1443	1445	rBV2	406	243	0.02%	0.003%
41	6.044	1459	1463	1466	rBV	228	178	0.02%	0.002%
42	6.250	1513	1527	1554	rBV	347961	664815	60.44%	7.467%
43	6.497	1601	1604	1607	rBV2	303	266	0.02%	0.003%
44	6.529	1607	1614	1624	rVB3	1370	2544	0.23%	0.029%
45	6.693	1647	1665	1685	rBV	256123	501968	45.64%	5.638%
46	6.780	1690	1692	1696	rVV	573	389	0.04%	0.004%
47	6.806	1696	1700	1706	rVB3	685	876	0.08%	0.010%
48	7.185	1810	1818	1833	rBV4	2762	4888	0.44%	0.055%
49	7.507	1910	1918	1920	rBV2	357	448	0.04%	0.005%
50	7.568	1924	1937	1954	rBV	114597	204923	18.63%	2.302%
51	7.690	1968	1975	1987	rVB5	1722	3191	0.29%	0.036%
52	7.899	2024	2040	2056	rBV	452445	786993	71.55%	8.839%
53	8.140	2112	2115	2116	rBV2	486	270	0.02%	0.003%
54	8.182	2116	2128	2146	rVV	81075	140667	12.79%	1.580%
55	8.636	2256	2269	2299	rBV	380599	702736	63.89%	7.893%
56	8.893	2347	2349	2353	rVB2	327	240	0.02%	0.003%
57	8.963	2368	2371	2374	rVB3	307	240	0.02%	0.003%
58	9.057	2396	2400	2405	rVB2	304	349	0.03%	0.004%
59	9.127	2419	2422	2428	rVB	384	393	0.04%	0.004%
60	9.169	2428	2435	2439	rBV3	651	680	0.06%	0.008%
61	9.417	2496	2512	2553	rBV	510921	924701	84.07%	10.386%
62	9.565	2553	2558	2563	rBV3	376	465	0.04%	0.005%
63	9.645	2580	2583	2588	rVB3	332	287	0.03%	0.003%
64	9.700	2594	2600	2606	rVB4	843	880	0.08%	0.010%
65	9.809	2632	2634	2639	rVB	301	205	0.02%	0.002%
66	9.873	2650	2654	2656	rBV	237	190	0.02%	0.002%
67	9.912	2662	2666	2670	rBV2	317	336	0.03%	0.004%
68	10.375	2805	2810	2812	rBV	239	233	0.02%	0.003%
69	10.465	2835	2838	2843	rBV	174	172	0.02%	0.002%
70	10.549	2860	2864	2866	rBV	222	193	0.02%	0.002%
71	10.671	2898	2902	2910	rVB3	1044	1303	0.12%	0.015%
72	10.709	2910	2914	2916	rBV2	220	166	0.02%	0.002%
73	10.758	2916	2929	2953	rVB	400157	643954	58.54%	7.233%
74	10.864	2958	2962	2965	rBV2	298	251	0.02%	0.003%
75	10.925	2978	2981	2984	rVB	324	209	0.02%	0.002%
76	10.954	2984	2990	2992	rBV2	189	215	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048175.D
 Acq On : 21 Apr 2022 16:05
 Operator : SY/MD
 Sample : N2486-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.394	3122	3127	3131	rBV2	254	241	0.02%	0.003%
78	11.423	3132	3136	3139	rVV2	291	217	0.02%	0.002%
79	11.449	3143	3144	3146	rVV	408	194	0.02%	0.002%
80	11.465	3146	3149	3160	rVB4	616	961	0.09%	0.011%
81	11.658	3202	3209	3212	rBV2	343	427	0.04%	0.005%
82	11.703	3217	3223	3227	rBV2	301	341	0.03%	0.004%
83	11.748	3229	3237	3244	rBV3	2721	3563	0.32%	0.040%
84	11.812	3244	3257	3281	rBV	513156	865406	78.68%	9.720%
85	11.915	3287	3289	3293	rVB	542	289	0.03%	0.003%
86	11.941	3293	3297	3300	rBV3	596	547	0.05%	0.006%
87	12.192	3362	3375	3397	rBV	477397	813369	73.95%	9.136%
88	12.391	3433	3437	3440	rBV2	335	308	0.03%	0.003%
89	12.426	3445	3448	3449	rBV2	335	194	0.02%	0.002%
90	12.587	3494	3498	3501	rBV2	257	257	0.02%	0.003%
91	12.651	3516	3518	3521	rBV2	252	165	0.02%	0.002%
92	12.732	3540	3543	3549	rVB2	361	384	0.03%	0.004%
93	12.870	3584	3586	3589	rBV	270	174	0.02%	0.002%
94	13.069	3643	3648	3650	rBV2	383	337	0.03%	0.004%
95	13.127	3662	3666	3669	rBV2	432	367	0.03%	0.004%
96	13.844	3880	3889	3902	rVB4	8825	14656	1.33%	0.165%
97	14.192	3995	3997	4001	rVB	391	226	0.02%	0.003%
98	14.327	4034	4039	4049	rBV5	2147	3434	0.31%	0.039%
99	14.905	4217	4219	4223	rBV2	474	241	0.02%	0.003%
100	15.259	4327	4329	4332	rBV3	499	290	0.03%	0.003%




Sum of corrected areas: 8903322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048175.D
Acq On : 21 Apr 2022 16:05
Operator : SY/MD
Sample : N2486-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

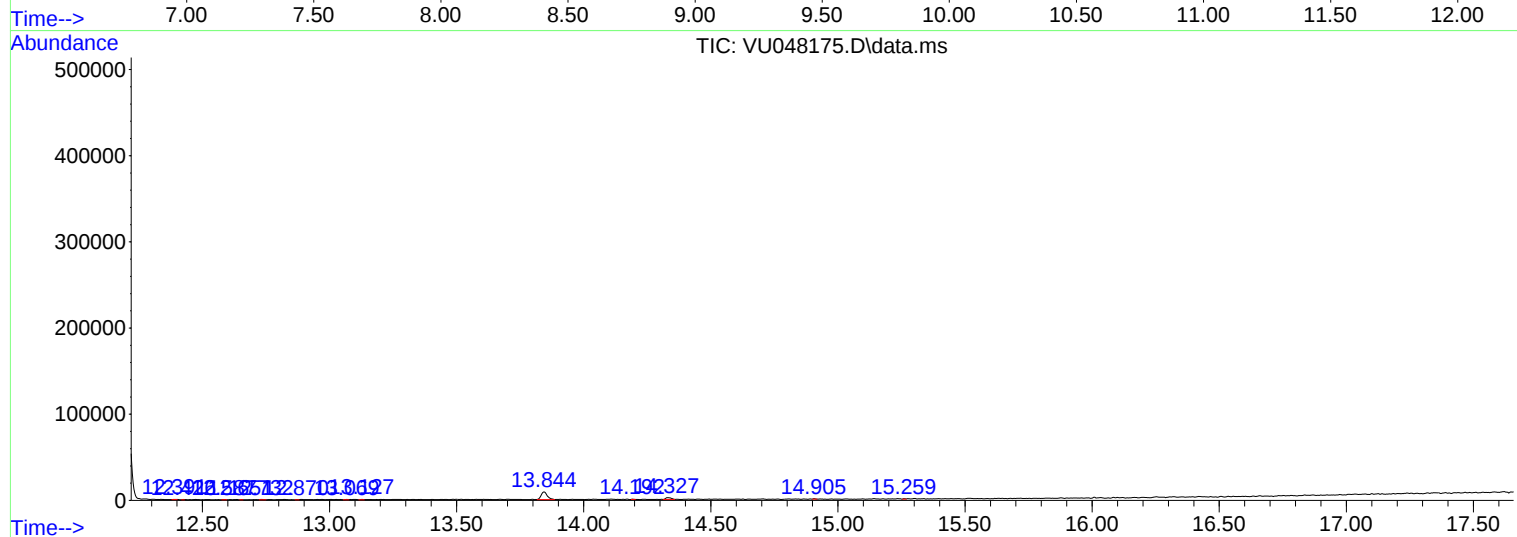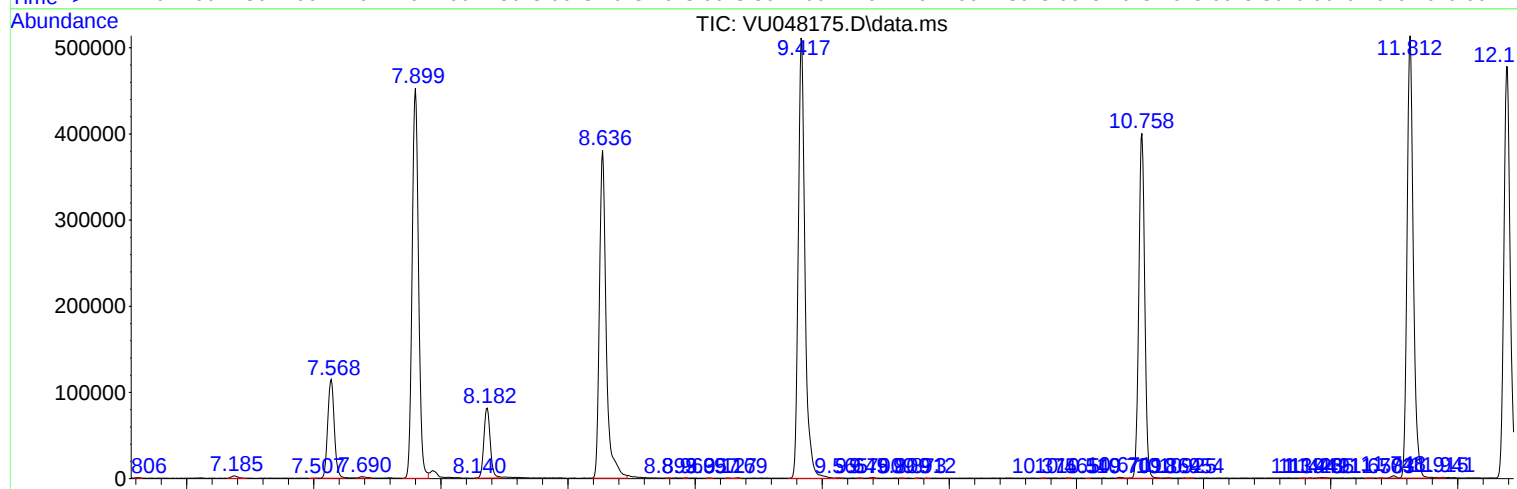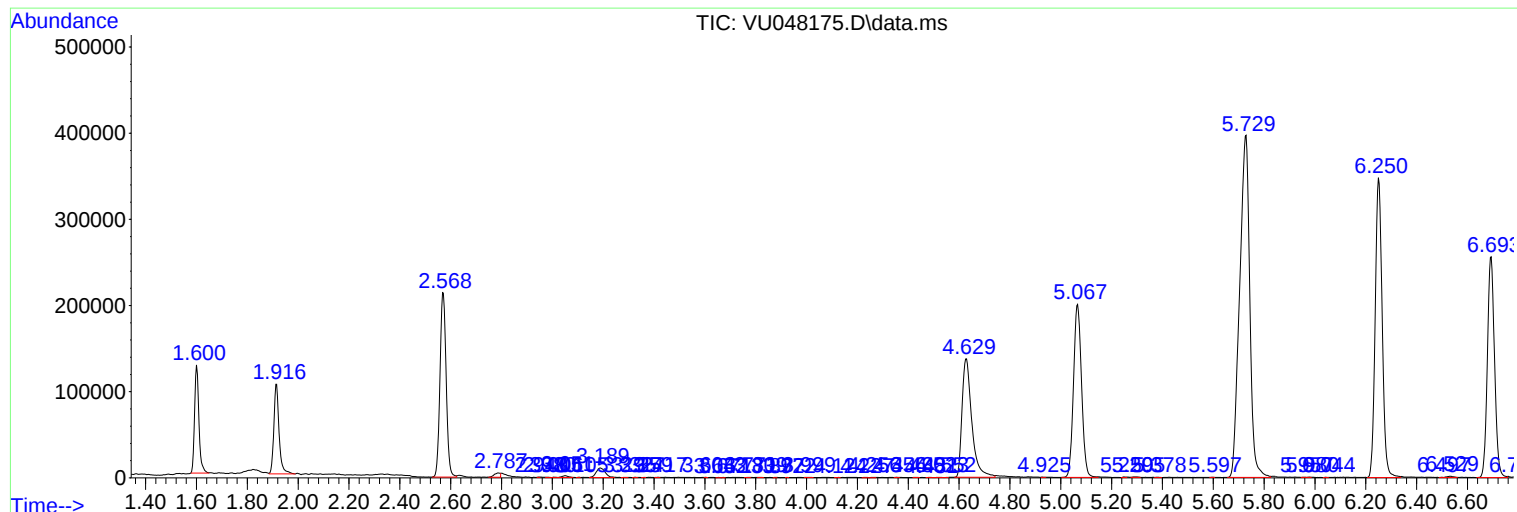

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048175.D
Acq On : 21 Apr 2022 16:05
Operator : SY/MD
Sample : N2486-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048175.D
Acq On : 21 Apr 2022 16:05
Operator : SY/MD
Sample : N2486-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------