

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048176.D
 Acq On : 21 Apr 2022 16:29
 Operator : SY/MD
 Sample : N2486-18 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rBV	133620	160365	7.45%	1.468%
2	1.916	171	179	203	rVB	110427	156093	7.25%	1.429%
3	2.572	370	383	400	rBV	228098	385061	17.88%	3.526%
4	2.681	415	417	425	rVB3	686	617	0.03%	0.006%
5	2.755	437	440	443	rBV2	384	245	0.01%	0.002%
6	2.806	447	456	458	rBV4	1708	2411	0.11%	0.022%
7	3.051	524	532	540	rBV7	1161	2208	0.10%	0.020%
8	3.128	550	556	558	rBV2	275	232	0.01%	0.002%
9	3.189	562	575	595	rVV	8592	19699	0.91%	0.180%
10	3.353	620	626	627	rBV	191	185	0.01%	0.002%
11	3.649	710	718	722	rBV2	261	313	0.01%	0.003%
12	3.668	722	724	729	rVB	354	208	0.01%	0.002%
13	3.809	765	768	771	rVB	339	241	0.01%	0.002%
14	3.832	771	775	779	rBV2	393	281	0.01%	0.003%
15	4.115	859	863	865	rBV	225	186	0.01%	0.002%
16	4.218	888	895	899	rBV2	355	406	0.02%	0.004%
17	4.288	914	917	925	rVB2	197	217	0.01%	0.002%
18	4.446	957	966	968	rBV2	202	262	0.01%	0.002%
19	4.504	979	984	987	rBV2	260	284	0.01%	0.003%
20	4.571	998	1005	1009	rBV	291	292	0.01%	0.003%
21	4.629	1009	1023	1066	rBV2	134036	381791	17.73%	3.496%
22	4.948	1120	1122	1126	rVB3	292	236	0.01%	0.002%
23	5.067	1143	1159	1186	rBV	205756	452615	21.02%	4.144%
24	5.221	1204	1207	1213	rVB4	411	394	0.02%	0.004%
25	5.295	1225	1230	1231	rBV2	435	321	0.01%	0.003%
26	5.350	1241	1247	1250	rBV	282	293	0.01%	0.003%
27	5.549	1302	1309	1312	rBV	196	192	0.01%	0.002%
28	5.729	1343	1365	1400	rBV2	417699	1136373	52.77%	10.405%
29	5.983	1442	1444	1450	rBV3	298	261	0.01%	0.002%
30	6.015	1451	1454	1459	rVB2	285	231	0.01%	0.002%
31	6.115	1481	1485	1486	rBV2	347	258	0.01%	0.002%
32	6.153	1492	1497	1503	rBV2	335	417	0.02%	0.004%
33	6.250	1513	1527	1561	rBV	364446	702184	32.61%	6.429%
34	6.497	1596	1604	1606	rBV3	278	358	0.02%	0.003%
35	6.530	1609	1614	1626	rVB5	1929	2853	0.13%	0.026%
36	6.694	1648	1665	1687	rBV	265071	518268	24.07%	4.745%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048176.D
 Acq On : 21 Apr 2022 16:29
 Operator : SY/MD
 Sample : N2486-18 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.041	1769	1773	1777	rBV3	366	413	0.02%	0.004%
38	7.192	1808	1820	1831	rVB5	2506	4866	0.23%	0.045%
39	7.240	1831	1835	1838	rBV2	290	285	0.01%	0.003%
40	7.276	1841	1846	1849	rVV2	242	183	0.01%	0.002%
41	7.298	1850	1853	1863	rVB2	438	599	0.03%	0.005%
42	7.362	1869	1873	1879	rVB2	230	220	0.01%	0.002%
43	7.427	1889	1893	1897	rBV2	205	255	0.01%	0.002%
44	7.491	1909	1913	1917	rVB3	245	210	0.01%	0.002%
45	7.568	1924	1937	1954	rBV2	117300	211156	9.81%	1.933%
46	7.645	1959	1961	1966	rVV3	474	484	0.02%	0.004%
47	7.690	1966	1975	1985	rVV4	1737	2908	0.14%	0.027%
48	7.832	2015	2019	2026	rVB3	342	449	0.02%	0.004%
49	7.899	2026	2040	2056	rBV	483378	841607	39.09%	7.706%
50	8.131	2109	2112	2114	rBV2	266	202	0.01%	0.002%
51	8.179	2116	2127	2143	rVV	82921	144155	6.69%	1.320%
52	8.359	2181	2183	2188	rVB2	400	268	0.01%	0.002%
53	8.574	2246	2250	2254	rVB3	334	229	0.01%	0.002%
54	8.636	2254	2269	2301	rBV	380110	726799	33.75%	6.655%
55	8.828	2326	2329	2335	rVB3	251	272	0.01%	0.002%
56	8.893	2344	2349	2352	rVB2	539	409	0.02%	0.004%
57	8.919	2352	2357	2358	rBV	333	197	0.01%	0.002%
58	9.169	2433	2435	2439	rVV3	393	269	0.01%	0.002%
59	9.205	2442	2446	2451	rVB2	269	251	0.01%	0.002%
60	9.279	2467	2469	2475	rVB2	366	257	0.01%	0.002%
61	9.417	2499	2512	2519	rBV	546070	994347	46.18%	9.104%
62	9.642	2579	2582	2589	rVB2	456	459	0.02%	0.004%
63	9.693	2589	2598	2599	rBV2	589	586	0.03%	0.005%
64	9.735	2607	2611	2615	rVB2	244	199	0.01%	0.002%
65	9.793	2625	2629	2631	rBV3	306	232	0.01%	0.002%
66	10.224	2759	2763	2766	rBV2	211	191	0.01%	0.002%
67	10.243	2766	2769	2772	rVB	253	197	0.01%	0.002%
68	10.520	2851	2855	2859	rVB2	295	289	0.01%	0.003%
69	10.571	2868	2871	2881	rVB2	250	306	0.01%	0.003%
70	10.671	2895	2902	2913	rVB5	755	1062	0.05%	0.010%
71	10.758	2913	2929	2948	rBV	407240	657688	30.54%	6.022%
72	10.986	2995	3000	3001	rBV	441	289	0.01%	0.003%
73	11.053	3019	3021	3024	rVB	337	181	0.01%	0.002%
74	11.137	3043	3047	3054	rVB3	322	322	0.01%	0.003%
75	11.468	3144	3150	3158	rVB3	722	1154	0.05%	0.011%
76	11.748	3226	3237	3245	rBV	20910	33230	1.54%	0.304%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048176.D
 Acq On : 21 Apr 2022 16:29
 Operator : SY/MD
 Sample : N2486-18 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.812	3245	3257	3280	rVB2	551300	1037271	48.17%	9.497%
78	11.970	3304	3306	3310	rVB2	672	358	0.02%	0.003%
79	12.021	3318	3322	3323	rBV	272	212	0.01%	0.002%
80	12.066	3333	3336	3341	rVB2	388	354	0.02%	0.003%
81	12.098	3342	3346	3350	rBV2	485	359	0.02%	0.003%
82	12.121	3350	3353	3357	rBV2	338	213	0.01%	0.002%
83	12.208	3361	3380	3406	rBV2	960268	2153265	100.00%	19.715%
84	12.378	3430	3433	3436	rBV2	448	278	0.01%	0.003%
85	12.404	3439	3441	3445	rBV2	266	235	0.01%	0.002%
86	12.426	3445	3448	3449	rBV	339	229	0.01%	0.002%
87	12.658	3517	3520	3523	rBV3	284	239	0.01%	0.002%
88	12.719	3537	3539	3543	rBV3	292	185	0.01%	0.002%
89	12.748	3546	3548	3551	rBV2	317	203	0.01%	0.002%
90	12.976	3616	3619	3622	rBV4	542	455	0.02%	0.004%
91	13.076	3647	3650	3653	rBV	283	234	0.01%	0.002%
92	13.150	3671	3673	3676	rBV2	270	202	0.01%	0.002%
93	13.208	3687	3691	3692	rBV2	318	258	0.01%	0.002%
94	13.288	3711	3716	3718	rBV3	452	456	0.02%	0.004%
95	13.317	3722	3725	3728	rVV2	352	256	0.01%	0.002%
96	13.455	3764	3768	3770	rBV	290	251	0.01%	0.002%
97	13.841	3877	3888	3912	rVB	92779	148184	6.88%	1.357%
98	14.095	3963	3967	3973	rVB4	713	824	0.04%	0.008%
99	14.333	4030	4041	4050	rBV3	14910	22440	1.04%	0.205%
100	14.761	4172	4174	4176	rBV2	465	265	0.01%	0.002%




Sum of corrected areas: 10921752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048176.D
Acq On : 21 Apr 2022 16:29
Operator : SY/MD
Sample : N2486-18 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

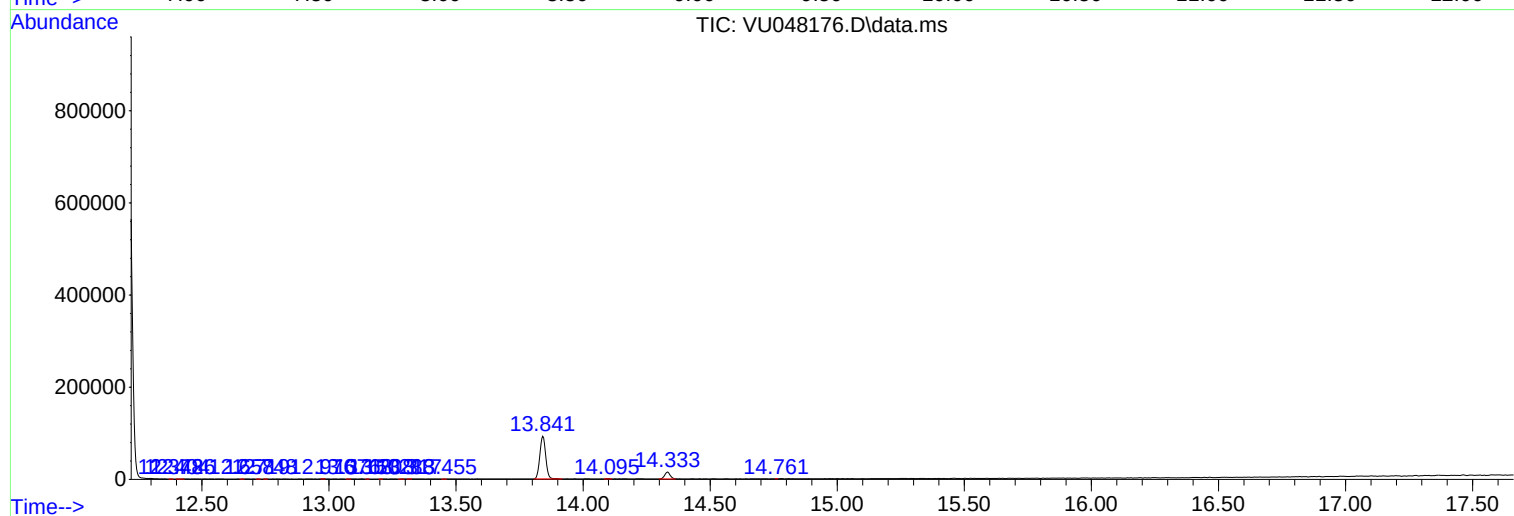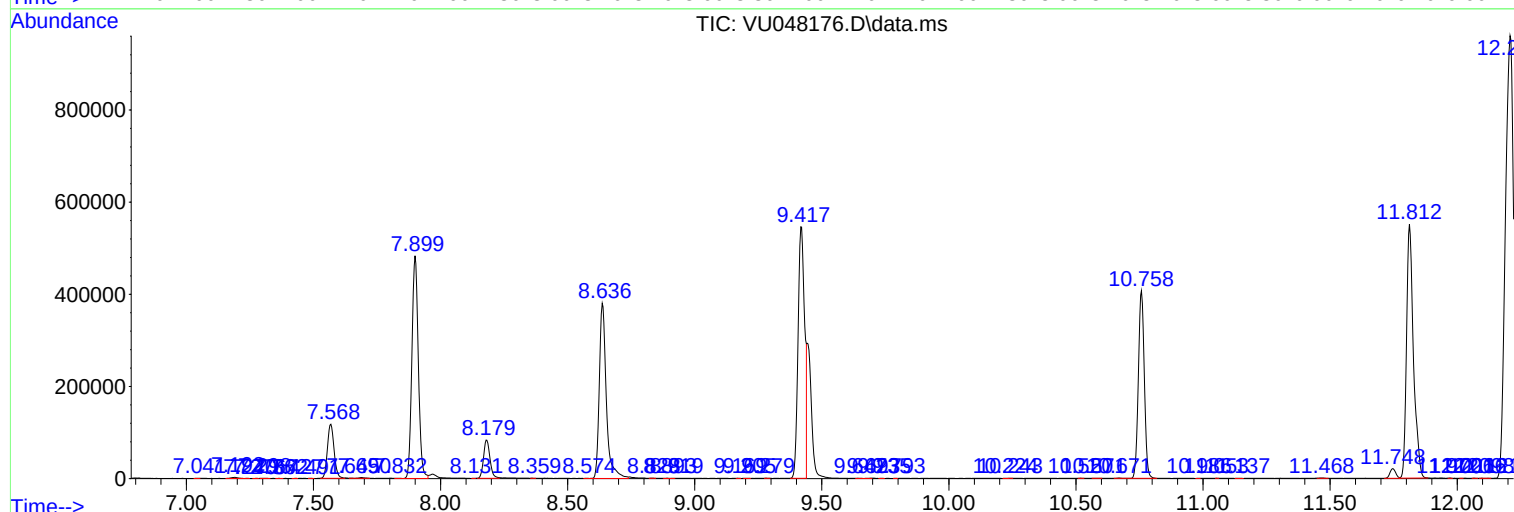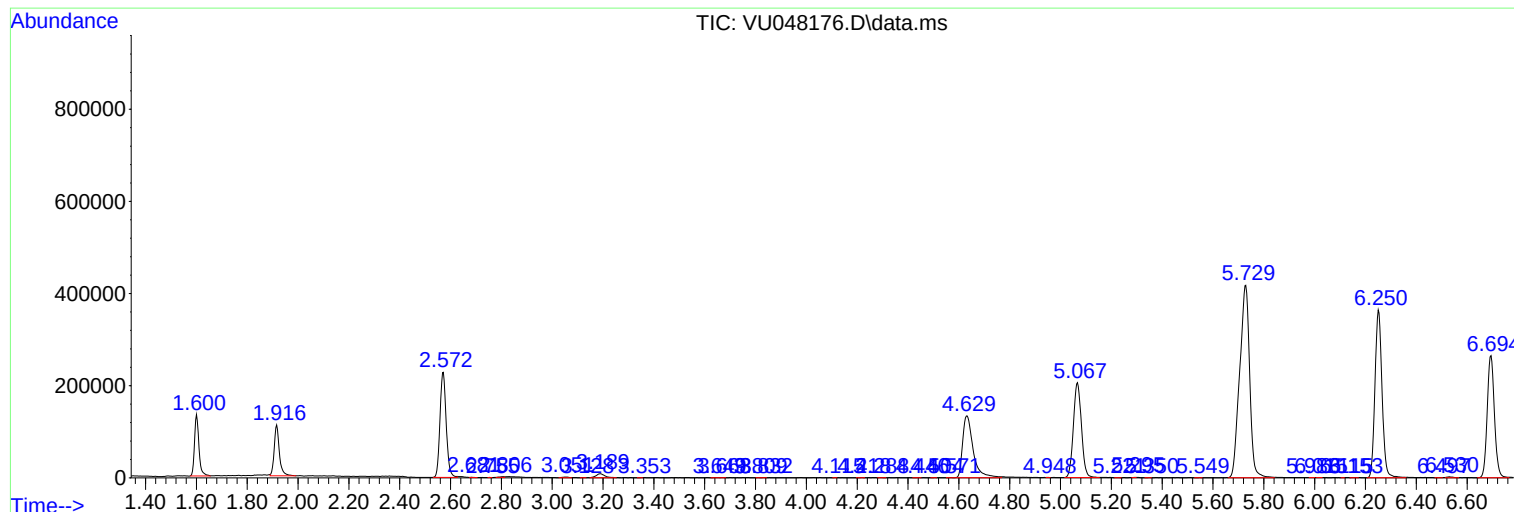

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048176.D
Acq On : 21 Apr 2022 16:29
Operator : SY/MD
Sample : N2486-18 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048176.D
Acq On : 21 Apr 2022 16:29
Operator : SY/MD
Sample : N2486-18 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------