

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048177.D
 Acq On : 21 Apr 2022 16:53
 Operator : SY/MD
 Sample : N2486-19 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	102	rVB	130369	156689	12.10%	1.603%
2	1.912	170	178	196	rVB	102813	145236	11.21%	1.486%
3	2.530	367	370	371	rBV2	348	211	0.02%	0.002%
4	2.568	371	382	403	rVV	223672	376671	29.08%	3.854%
5	2.681	414	417	424	rVB3	485	523	0.04%	0.005%
6	2.732	430	433	437	rVB2	361	278	0.02%	0.003%
7	2.790	437	451	475	rVB3	4256	14480	1.12%	0.148%
8	2.877	475	478	484	rVB3	472	475	0.04%	0.005%
9	2.925	490	493	495	rBV	331	216	0.02%	0.002%
10	3.044	524	530	533	rBV4	1290	1478	0.11%	0.015%
11	3.189	561	575	593	rVB2	10729	24958	1.93%	0.255%
12	3.253	593	595	598	rBV2	223	181	0.01%	0.002%
13	3.346	620	624	626	rBV2	193	167	0.01%	0.002%
14	3.517	671	677	680	rBV2	336	421	0.03%	0.004%
15	3.617	707	708	712	rVB2	357	183	0.01%	0.002%
16	3.649	715	718	721	rBV2	203	177	0.01%	0.002%
17	3.684	725	729	731	rBV	259	221	0.02%	0.002%
18	3.777	753	758	759	rBV2	267	165	0.01%	0.002%
19	4.012	828	831	838	rVB2	277	337	0.03%	0.003%
20	4.083	848	853	857	rBV2	287	334	0.03%	0.003%
21	4.108	857	861	865	rBV	277	257	0.02%	0.003%
22	4.195	884	888	891	rBV	210	150	0.01%	0.002%
23	4.340	929	933	939	rBV2	196	262	0.02%	0.003%
24	4.626	1008	1022	1058	rBV2	136212	363076	28.03%	3.715%
25	5.067	1141	1159	1187	rBV	201236	442059	34.13%	4.523%
26	5.186	1194	1196	1199	rVB3	292	178	0.01%	0.002%
27	5.292	1224	1229	1236	rVB4	572	884	0.07%	0.009%
28	5.346	1241	1246	1248	rBV2	248	228	0.02%	0.002%
29	5.639	1334	1337	1340	rBV2	230	222	0.02%	0.002%
30	5.729	1343	1365	1390	rBV2	405843	1102955	85.16%	11.286%
31	6.128	1481	1489	1493	rVB3	522	676	0.05%	0.007%
32	6.147	1493	1495	1498	rBV2	337	237	0.02%	0.002%
33	6.250	1510	1527	1552	rBV	362941	691531	53.39%	7.076%
34	6.530	1606	1614	1626	rVV6	1524	2787	0.22%	0.029%
35	6.571	1626	1627	1631	rVB	371	177	0.01%	0.002%
36	6.597	1632	1635	1638	rBV3	315	160	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048177.D
 Acq On : 21 Apr 2022 16:53
 Operator : SY/MD
 Sample : N2486-19 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1693	rVV	257769	505130	39.00%	5.169%
38	6.790	1693	1695	1699	rVV4	504	466	0.04%	0.005%
39	6.813	1699	1702	1709	rVV3	830	915	0.07%	0.009%
40	6.867	1715	1719	1722	rBV	199	171	0.01%	0.002%
41	6.887	1722	1725	1728	rBV2	244	154	0.01%	0.002%
42	7.038	1769	1772	1775	rBV2	369	285	0.02%	0.003%
43	7.137	1801	1803	1806	rBV2	370	211	0.02%	0.002%
44	7.189	1808	1819	1827	rBV4	2419	3848	0.30%	0.039%
45	7.282	1845	1848	1852	rBV2	225	220	0.02%	0.002%
46	7.446	1895	1899	1901	rBV	411	355	0.03%	0.004%
47	7.568	1923	1937	1954	rBV	113523	203382	15.70%	2.081%
48	7.694	1968	1976	1986	rVV5	1645	2912	0.22%	0.030%
49	7.735	1986	1989	1994	rVB4	372	262	0.02%	0.003%
50	7.793	2001	2007	2008	rBV2	761	660	0.05%	0.007%
51	7.899	2025	2040	2056	rBV	478085	826856	63.84%	8.461%
52	8.124	2107	2110	2113	rBV3	217	155	0.01%	0.002%
53	8.179	2114	2127	2142	rBV	80618	140097	10.82%	1.434%
54	8.330	2171	2174	2175	rBV2	318	173	0.01%	0.002%
55	8.401	2193	2196	2198	rVB3	329	170	0.01%	0.002%
56	8.533	2232	2237	2240	rBV	207	174	0.01%	0.002%
57	8.636	2254	2269	2299	rBV	370551	691408	53.38%	7.075%
58	8.915	2353	2356	2357	rBV	235	155	0.01%	0.002%
59	8.980	2372	2376	2380	rBV2	432	428	0.03%	0.004%
60	9.140	2421	2426	2433	rBV4	289	391	0.03%	0.004%
61	9.288	2466	2472	2476	rBV2	408	421	0.03%	0.004%
62	9.417	2498	2512	2552	rBV2	540017	1086889	83.92%	11.121%
63	9.693	2592	2598	2604	rBV2	434	634	0.05%	0.006%
64	9.825	2635	2639	2642	rBV2	229	181	0.01%	0.002%
65	9.973	2681	2685	2687	rBV2	242	192	0.01%	0.002%
66	10.076	2713	2717	2721	rBV	176	156	0.01%	0.002%
67	10.095	2721	2723	2728	rVB2	323	201	0.02%	0.002%
68	10.150	2733	2740	2742	rBV2	355	452	0.03%	0.005%
69	10.166	2742	2745	2751	rVB3	384	364	0.03%	0.004%
70	10.230	2760	2765	2768	rBV2	209	225	0.02%	0.002%
71	10.311	2788	2790	2795	rVB2	237	158	0.01%	0.002%
72	10.343	2797	2800	2803	rBV	253	206	0.02%	0.002%
73	10.369	2804	2808	2813	rVB3	182	156	0.01%	0.002%
74	10.671	2898	2902	2911	rVV4	974	1099	0.08%	0.011%
75	10.758	2916	2929	2949	rBV	393301	637125	49.19%	6.519%
76	10.857	2958	2960	2964	rBV2	270	171	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048177.D
 Acq On : 21 Apr 2022 16:53
 Operator : SY/MD
 Sample : N2486-19 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.992	3000	3002	3008	rVB	239	206	0.02%	0.002%
78	11.060	3021	3023	3027	rVB3	257	155	0.01%	0.002%
79	11.092	3028	3033	3037	rBV2	236	210	0.02%	0.002%
80	11.131	3039	3045	3047	rBV	230	275	0.02%	0.003%
81	11.195	3064	3065	3071	rVB2	365	317	0.02%	0.003%
82	11.240	3071	3079	3080	rBV	256	301	0.02%	0.003%
83	11.452	3142	3145	3146	rBV	398	185	0.01%	0.002%
84	11.748	3228	3237	3245	rVV2	8147	12249	0.95%	0.125%
85	11.812	3245	3257	3278	rVV	553171	938295	72.44%	9.601%
86	11.947	3297	3299	3303	rVB5	680	353	0.03%	0.004%
87	12.066	3334	3336	3339	rVB2	326	179	0.01%	0.002%
88	12.131	3353	3356	3359	rBV	242	163	0.01%	0.002%
89	12.147	3359	3361	3362	rBV	347	152	0.01%	0.002%
90	12.198	3363	3377	3403	rVV2	560708	1295200	100.00%	13.253%
91	12.590	3496	3499	3505	rBV3	339	430	0.03%	0.004%
92	12.803	3562	3565	3568	rBV2	332	239	0.02%	0.002%
93	13.137	3666	3669	3673	rBV2	379	315	0.02%	0.003%
94	13.156	3673	3675	3680	rBV3	328	316	0.02%	0.003%
95	13.841	3878	3888	3901	rBV3	46108	73829	5.70%	0.755%
96	14.015	3940	3942	3945	rBV2	393	236	0.02%	0.002%
97	14.333	4033	4041	4055	rVB2	7164	11245	0.87%	0.115%
98	14.629	4131	4133	4140	rVB3	498	347	0.03%	0.004%
99	15.256	4326	4328	4331	rBV2	523	340	0.03%	0.003%
100	15.632	4441	4445	4446	rBV	738	571	0.04%	0.006%




Sum of corrected areas: 9772956

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048177.D
Acq On : 21 Apr 2022 16:53
Operator : SY/MD
Sample : N2486-19 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

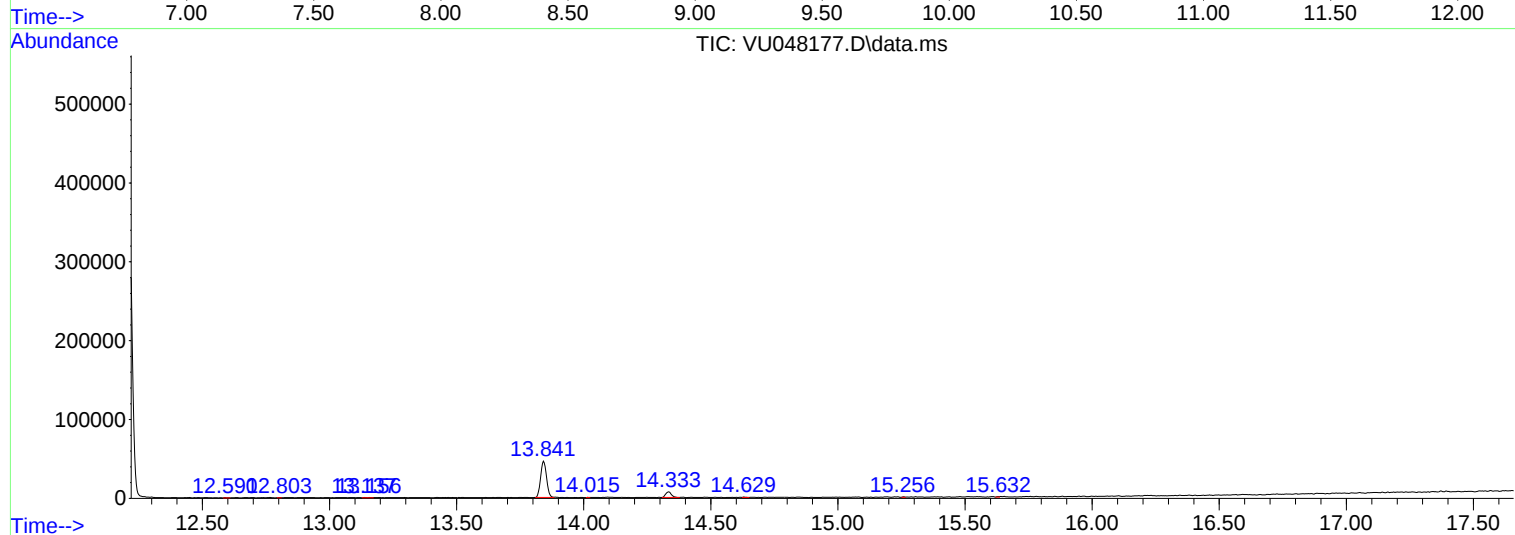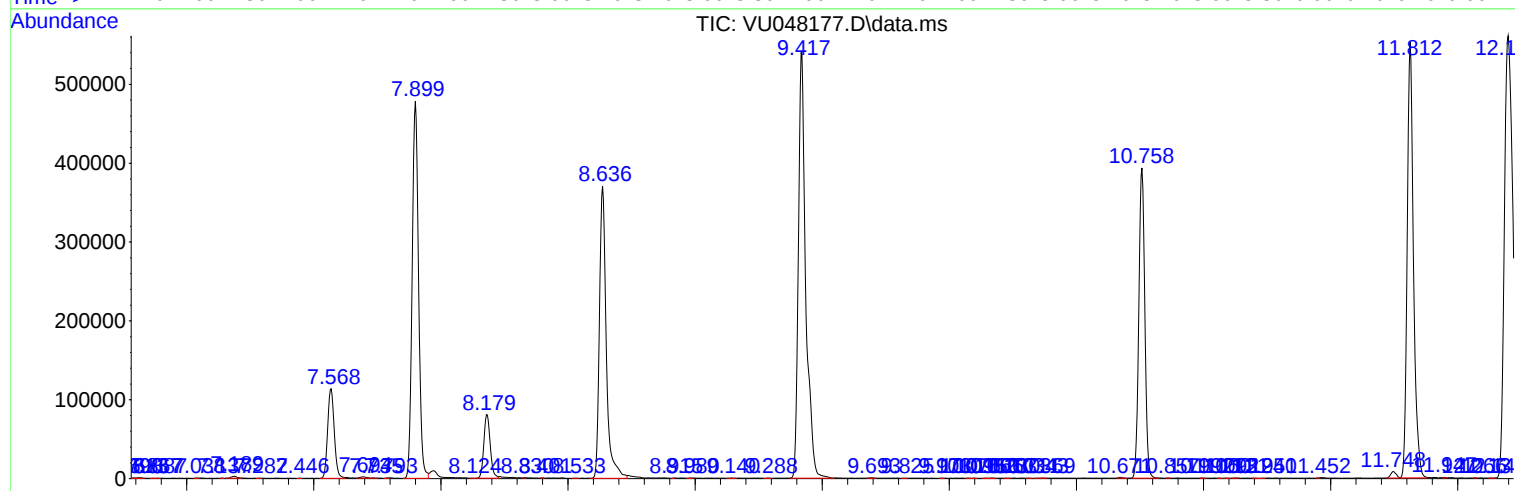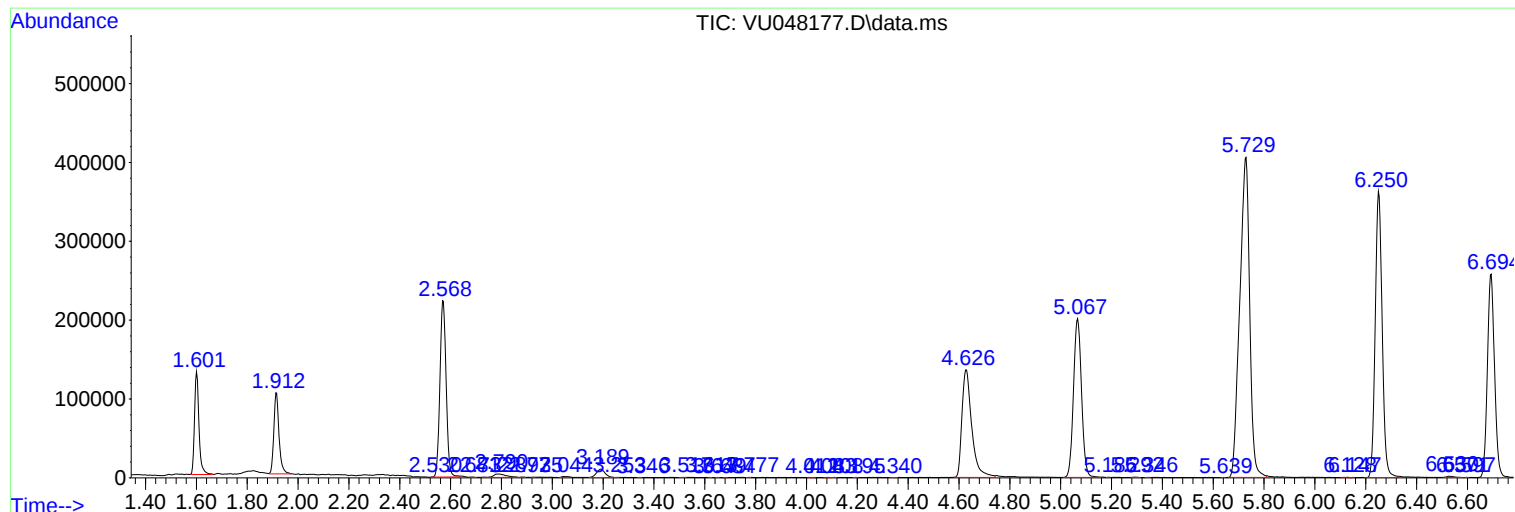

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048177.D
Acq On : 21 Apr 2022 16:53
Operator : SY/MD
Sample : N2486-19 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048177.D
Acq On : 21 Apr 2022 16:53
Operator : SY/MD
Sample : N2486-19 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------