

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048178.D
 Acq On : 21 Apr 2022 17:16
 Operator : SY/MD
 Sample : N2486-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	132875	158692	12.07%	1.592%
2	1.912	170	178	197	rBV	104528	146119	11.12%	1.465%
3	2.568	369	382	402	rBV	234122	384313	29.24%	3.854%
4	2.723	426	430	431	rBV	387	226	0.02%	0.002%
5	2.761	433	442	451	rBV2	5056	10145	0.77%	0.102%
6	2.999	514	516	519	rVB2	283	161	0.01%	0.002%
7	3.019	519	522	524	rBV	314	188	0.01%	0.002%
8	3.051	524	532	542	rVB6	1575	3175	0.24%	0.032%
9	3.102	542	548	550	rBV2	403	419	0.03%	0.004%
10	3.115	550	552	556	rVB2	350	258	0.02%	0.003%
11	3.141	556	560	561	rBV2	264	205	0.02%	0.002%
12	3.189	561	575	592	rVB2	17428	40024	3.04%	0.401%
13	3.301	607	610	613	rBV2	243	156	0.01%	0.002%
14	3.343	620	623	624	rBV2	331	186	0.01%	0.002%
15	3.404	637	642	644	rVB	357	275	0.02%	0.003%
16	3.427	644	649	650	rBV	265	176	0.01%	0.002%
17	3.440	650	653	656	rVB	229	168	0.01%	0.002%
18	3.523	675	679	684	rVB	187	205	0.02%	0.002%
19	3.687	727	730	735	rVB	359	261	0.02%	0.003%
20	3.719	735	740	744	rBV	184	198	0.02%	0.002%
21	3.745	744	748	751	rVB2	205	211	0.02%	0.002%
22	3.768	751	755	761	rVB2	330	386	0.03%	0.004%
23	3.797	761	764	766	rBV2	218	139	0.01%	0.001%
24	3.816	766	770	774	rBV2	316	331	0.03%	0.003%
25	3.855	779	782	786	rBB2	308	185	0.01%	0.002%
26	3.877	786	789	793	rVB2	196	148	0.01%	0.001%
27	3.903	794	797	801	rVB	237	170	0.01%	0.002%
28	3.928	801	805	807	rBV2	204	143	0.01%	0.001%
29	3.941	807	809	814	rVB	289	172	0.01%	0.002%
30	3.967	814	817	820	rBV	218	200	0.02%	0.002%
31	4.009	828	830	837	rVB2	213	256	0.02%	0.003%
32	4.112	857	862	865	rBV2	211	192	0.01%	0.002%
33	4.202	883	890	894	rBV2	417	439	0.03%	0.004%
34	4.224	894	897	899	rBV2	274	212	0.02%	0.002%
35	4.289	913	917	919	rBV2	217	141	0.01%	0.001%
36	4.350	933	936	939	rVB2	356	223	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048178.D
 Acq On : 21 Apr 2022 17:16
 Operator : SY/MD
 Sample : N2486-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	4.369	939	942	948	rBV2	269	343	0.03%	0.003%
38	4.440	960	964	966	rBV	356	198	0.02%	0.002%
39	4.620	1006	1020	1054	rBV	135881	336895	25.63%	3.379%
40	4.864	1093	1096	1098	rBV	248	141	0.01%	0.001%
41	4.970	1125	1129	1136	rBV3	220	334	0.03%	0.003%
42	5.067	1142	1159	1178	rBV	205062	447896	34.07%	4.492%
43	5.285	1224	1227	1229	rBV2	310	234	0.02%	0.002%
44	5.726	1340	1364	1398	rBV2	416985	1131476	86.07%	11.348%
45	6.002	1448	1450	1454	rBV2	302	257	0.02%	0.003%
46	6.166	1497	1501	1506	rVB2	298	294	0.02%	0.003%
47	6.250	1506	1527	1551	rBV	379606	723073	55.01%	7.252%
48	6.472	1594	1596	1601	rVB3	444	237	0.02%	0.002%
49	6.530	1607	1614	1626	rVB4	1576	2897	0.22%	0.029%
50	6.597	1632	1635	1639	rVB3	288	229	0.02%	0.002%
51	6.690	1650	1664	1688	rBV	261166	514161	39.11%	5.157%
52	6.932	1737	1739	1742	rVB	273	177	0.01%	0.002%
53	6.951	1742	1745	1748	rBV2	175	128	0.01%	0.001%
54	7.141	1800	1804	1808	rBV2	185	150	0.01%	0.002%
55	7.186	1808	1818	1828	rVV4	2299	4082	0.31%	0.041%
56	7.314	1855	1858	1860	rBV	272	161	0.01%	0.002%
57	7.385	1875	1880	1882	rBV2	268	240	0.02%	0.002%
58	7.456	1898	1902	1909	rVB	307	353	0.03%	0.004%
59	7.568	1920	1937	1954	rBV	120014	211828	16.11%	2.124%
60	7.684	1967	1973	1985	rVB6	1600	2885	0.22%	0.029%
61	7.735	1985	1989	1992	rVB2	371	255	0.02%	0.003%
62	7.787	2002	2005	2007	rBV2	553	303	0.02%	0.003%
63	7.899	2026	2040	2056	rBV	492658	853065	64.90%	8.555%
64	8.112	2102	2106	2109	rVB2	269	227	0.02%	0.002%
65	8.179	2116	2127	2141	rBV	84225	141780	10.79%	1.422%
66	8.359	2178	2183	2186	rBV4	448	447	0.03%	0.004%
67	8.443	2205	2209	2211	rBV	160	151	0.01%	0.002%
68	8.472	2216	2218	2221	rBV2	272	200	0.02%	0.002%
69	8.488	2221	2223	2225	rVB2	452	200	0.02%	0.002%
70	8.632	2255	2268	2313	rBV	362033	674907	51.34%	6.769%
71	8.838	2330	2332	2334	rVB	384	189	0.01%	0.002%
72	8.993	2377	2380	2383	rVB2	238	161	0.01%	0.002%
73	9.076	2405	2406	2413	rVB2	391	267	0.02%	0.003%
74	9.163	2429	2433	2436	rVB3	333	266	0.02%	0.003%
75	9.298	2472	2475	2480	rBV2	303	244	0.02%	0.002%
76	9.417	2499	2512	2554	rBV2	574526	1134394	86.30%	11.377%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048178.D
 Acq On : 21 Apr 2022 17:16
 Operator : SY/MD
 Sample : N2486-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.658	2585	2587	2592	rVB2	234	125	0.01%	0.001%
78	9.700	2592	2600	2603	rBV4	644	966	0.07%	0.010%
79	10.102	2722	2725	2731	rBV2	322	309	0.02%	0.003%
80	10.205	2755	2757	2763	rVB	381	296	0.02%	0.003%
81	10.234	2763	2766	2768	rBV2	370	238	0.02%	0.002%
82	10.668	2897	2901	2907	rVB3	556	657	0.05%	0.007%
83	10.758	2915	2929	2952	rBV	396273	646637	49.19%	6.485%
84	11.005	3002	3006	3008	rVB2	340	229	0.02%	0.002%
85	11.118	3038	3041	3042	rBV	310	146	0.01%	0.001%
86	11.311	3098	3101	3104	rVB3	328	211	0.02%	0.002%
87	11.359	3112	3116	3121	rBV2	342	428	0.03%	0.004%
88	11.555	3174	3177	3181	rBV2	332	287	0.02%	0.003%
89	11.748	3228	3237	3245	rBV2	7667	12075	0.92%	0.121%
90	11.812	3245	3257	3282	rVV	575547	978317	74.42%	9.812%
91	12.041	3324	3328	3334	rBV4	382	476	0.04%	0.005%
92	12.128	3352	3355	3358	rBV	308	253	0.02%	0.003%
93	12.198	3363	3377	3400	rBV2	580566	1314529	100.00%	13.183%
94	12.333	3416	3419	3420	rBV2	277	200	0.02%	0.002%
95	12.372	3426	3431	3435	rBV3	706	644	0.05%	0.006%
96	12.552	3484	3487	3490	rVB	347	179	0.01%	0.002%
97	13.111	3658	3661	3662	rBV	258	177	0.01%	0.002%
98	13.841	3878	3888	3900	rBV2	41876	67993	5.17%	0.682%
99	14.063	3954	3957	3962	rBV2	435	356	0.03%	0.004%
100	14.333	4034	4041	4053	rVB4	6348	10485	0.80%	0.105%


Sum of corrected areas: 9971036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048178.D
Acq On : 21 Apr 2022 17:16
Operator : SY/MD
Sample : N2486-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

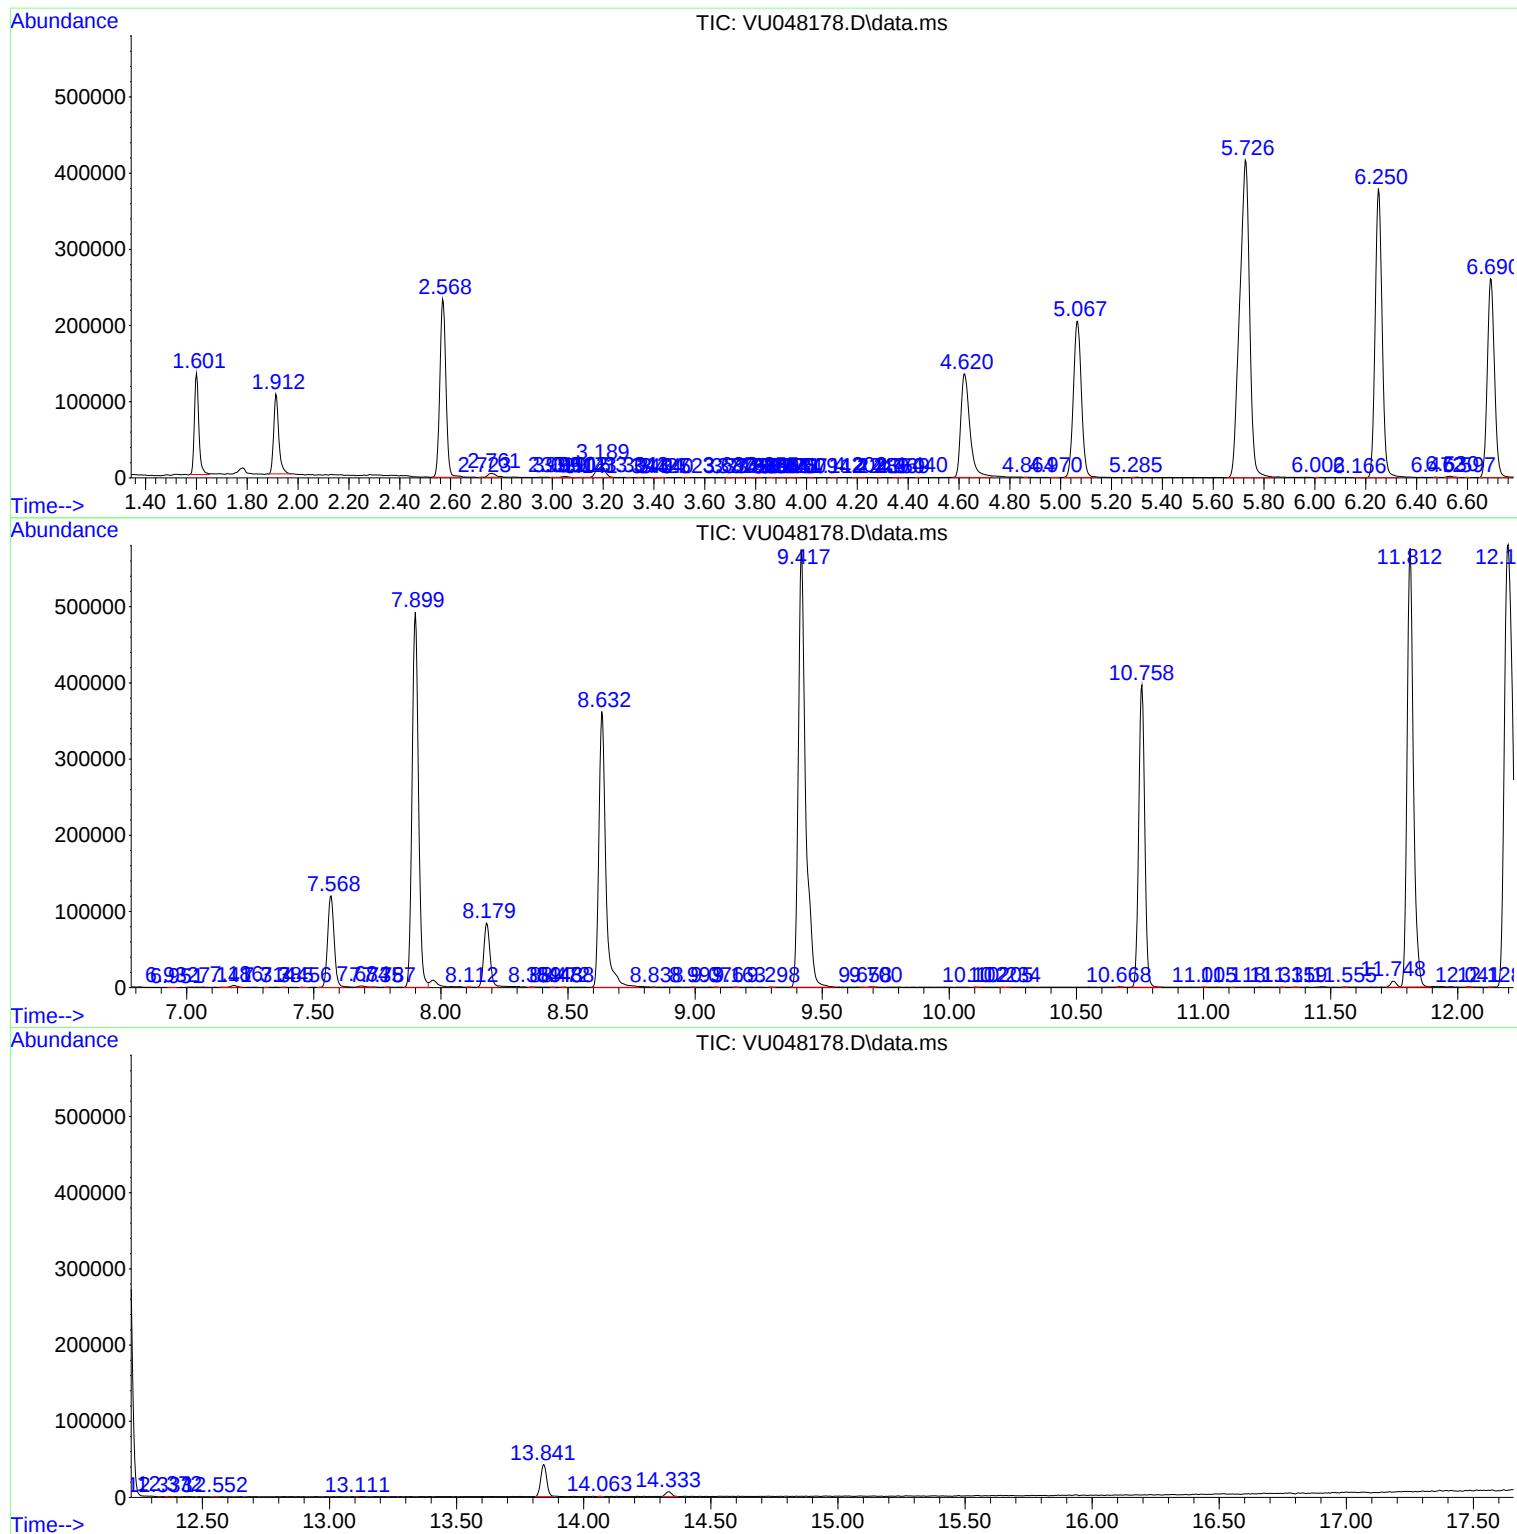

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048178.D
Acq On : 21 Apr 2022 17:16
Operator : SY/MD
Sample : N2486-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048178.D
Acq On : 21 Apr 2022 17:16
Operator : SY/MD
Sample : N2486-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc