

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048179.D
 Acq On : 21 Apr 2022 17:40
 Operator : SY/MD
 Sample : N2485-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	97	rBV	133066	161384	14.21%	1.753%
2	1.912	170	178	197	rVB	107339	149805	13.19%	1.627%
3	2.568	370	382	404	rBV	234849	393298	34.62%	4.271%
4	2.719	426	429	431	rBV	367	242	0.02%	0.003%
5	2.739	431	435	437	rVB4	564	373	0.03%	0.004%
6	2.784	437	449	463	rBV2	5417	14389	1.27%	0.156%
7	2.909	483	488	490	rBV3	405	338	0.03%	0.004%
8	2.951	498	501	504	rVB3	422	211	0.02%	0.002%
9	3.057	524	534	541	rVB3	1616	2851	0.25%	0.031%
10	3.189	562	575	592	rBV	10054	23758	2.09%	0.258%
11	3.272	597	601	604	rBV3	308	300	0.03%	0.003%
12	3.379	629	634	637	rVB2	311	272	0.02%	0.003%
13	3.398	637	640	643	rBV	249	207	0.02%	0.002%
14	3.417	643	646	653	rVB2	310	311	0.03%	0.003%
15	3.591	695	700	703	rBV2	184	176	0.02%	0.002%
16	3.983	819	822	827	rBV3	264	265	0.02%	0.003%
17	4.073	846	850	856	rVB2	177	178	0.02%	0.002%
18	4.102	856	859	863	rBV2	233	242	0.02%	0.003%
19	4.163	871	878	884	rBV2	246	240	0.02%	0.003%
20	4.372	938	943	948	rBV	224	254	0.02%	0.003%
21	4.626	1006	1022	1061	rBV2	139890	366935	32.30%	3.985%
22	5.002	1135	1139	1142	rBV2	235	218	0.02%	0.002%
23	5.067	1142	1159	1180	rBV	205961	451103	39.71%	4.899%
24	5.202	1197	1201	1205	rVB2	436	314	0.03%	0.003%
25	5.234	1205	1211	1215	rBV3	538	560	0.05%	0.006%
26	5.256	1216	1218	1223	rVB2	275	177	0.02%	0.002%
27	5.298	1223	1231	1235	rBV2	679	873	0.08%	0.009%
28	5.507	1293	1296	1301	rVB2	248	226	0.02%	0.002%
29	5.729	1342	1365	1396	rBV2	419334	1136068	100.00%	12.338%
30	5.851	1401	1403	1412	rVB3	822	877	0.08%	0.010%
31	5.967	1435	1439	1447	rVB3	287	342	0.03%	0.004%
32	6.025	1452	1457	1460	rBV2	271	251	0.02%	0.003%
33	6.050	1460	1465	1468	rVB3	506	358	0.03%	0.004%
34	6.115	1480	1485	1489	rBV2	331	339	0.03%	0.004%
35	6.134	1489	1491	1493	rVB	437	207	0.02%	0.002%
36	6.157	1493	1498	1503	rBV2	215	335	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048179.D
 Acq On : 21 Apr 2022 17:40
 Operator : SY/MD
 Sample : N2485-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1508	1527	1549	rBV	366584	700164	61.63%	7.604%
38	6.401	1572	1574	1579	rVB3	389	251	0.02%	0.003%
39	6.533	1607	1615	1623	rBV6	1571	2794	0.25%	0.030%
40	6.694	1646	1665	1691	rBV	261460	515669	45.39%	5.600%
41	6.803	1697	1699	1702	rBV2	428	358	0.03%	0.004%
42	6.841	1708	1711	1720	rVB2	162	202	0.02%	0.002%
43	6.948	1739	1744	1749	rVB2	175	180	0.02%	0.002%
44	7.102	1786	1792	1794	rBV	314	237	0.02%	0.003%
45	7.150	1803	1807	1811	rBV2	317	261	0.02%	0.003%
46	7.185	1811	1818	1830	rVV5	2684	4883	0.43%	0.053%
47	7.337	1856	1865	1869	rVV3	216	323	0.03%	0.004%
48	7.488	1908	1912	1914	rBV	283	214	0.02%	0.002%
49	7.568	1923	1937	1954	rBV	121538	212591	18.71%	2.309%
50	7.687	1968	1974	1986	rVB7	2028	3438	0.30%	0.037%
51	7.796	2002	2008	2015	rBV2	630	713	0.06%	0.008%
52	7.899	2025	2040	2056	rBV	487591	855767	75.33%	9.294%
53	8.182	2116	2128	2148	rBV	83635	145416	12.80%	1.579%
54	8.513	2228	2231	2236	rVB2	202	182	0.02%	0.002%
55	8.636	2256	2269	2303	rBV	374534	696761	61.33%	7.567%
56	8.828	2326	2329	2330	rBV2	336	181	0.02%	0.002%
57	8.857	2335	2338	2340	rVB	425	254	0.02%	0.003%
58	8.873	2340	2343	2346	rBV3	308	269	0.02%	0.003%
59	8.957	2365	2369	2372	rBV2	361	271	0.02%	0.003%
60	8.980	2373	2376	2379	rVV3	492	359	0.03%	0.004%
61	9.009	2383	2385	2391	rVB3	274	221	0.02%	0.002%
62	9.147	2424	2428	2429	rBV2	384	228	0.02%	0.002%
63	9.417	2499	2512	2551	rVV	543229	955115	84.07%	10.373%
64	9.562	2554	2557	2559	rVV2	383	197	0.02%	0.002%
65	9.581	2559	2563	2568	rVB4	365	349	0.03%	0.004%
66	9.693	2594	2598	2602	rBV2	777	767	0.07%	0.008%
67	9.774	2620	2623	2626	rVV	275	201	0.02%	0.002%
68	9.851	2640	2647	2653	rBV2	328	440	0.04%	0.005%
69	9.909	2659	2665	2666	rBV	224	182	0.02%	0.002%
70	10.008	2690	2696	2700	rBV2	218	299	0.03%	0.003%
71	10.063	2706	2713	2717	rBV2	229	302	0.03%	0.003%
72	10.102	2721	2725	2729	rVB3	422	409	0.04%	0.004%
73	10.475	2838	2841	2845	rBV	296	313	0.03%	0.003%
74	10.584	2870	2875	2878	rBV2	249	221	0.02%	0.002%
75	10.674	2897	2903	2912	rVB3	1344	1689	0.15%	0.018%
76	10.758	2916	2929	2951	rVV	397743	644542	56.73%	7.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048179.D
 Acq On : 21 Apr 2022 17:40
 Operator : SY/MD
 Sample : N2485-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.886	2966	2969	2975	rBV2	314	321	0.03%	0.003%
78	10.918	2976	2979	2982	rVV	297	215	0.02%	0.002%
79	11.008	3004	3007	3012	rVB	386	389	0.03%	0.004%
80	11.034	3012	3015	3017	rBV	277	226	0.02%	0.002%
81	11.098	3030	3035	3041	rBV2	149	213	0.02%	0.002%
82	11.147	3047	3050	3052	rBV2	330	222	0.02%	0.002%
83	11.391	3122	3126	3129	rBV	317	289	0.03%	0.003%
84	11.459	3141	3147	3151	rBV6	848	931	0.08%	0.010%
85	11.697	3217	3221	3224	rBV2	442	315	0.03%	0.003%
86	11.745	3231	3236	3244	rBV3	1056	1386	0.12%	0.015%
87	11.812	3244	3257	3280	rBV	538933	891729	78.49%	9.685%
88	11.967	3302	3305	3306	rBV2	292	176	0.02%	0.002%
89	12.005	3315	3317	3321	rVB2	398	231	0.02%	0.003%
90	12.028	3321	3324	3326	rBV2	409	212	0.02%	0.002%
91	12.195	3362	3376	3396	rBV	499214	843125	74.21%	9.157%
92	12.362	3426	3428	3432	rBV2	339	245	0.02%	0.003%
93	12.391	3435	3437	3442	rVB2	463	264	0.02%	0.003%
94	12.536	3479	3482	3486	rVB2	281	219	0.02%	0.002%
95	12.581	3490	3496	3498	rBV3	325	328	0.03%	0.004%
96	12.619	3505	3508	3509	rBV	360	186	0.02%	0.002%
97	12.639	3513	3514	3520	rVB2	257	210	0.02%	0.002%
98	12.722	3536	3540	3545	rBV3	249	275	0.02%	0.003%
99	12.787	3556	3560	3563	rBV3	395	317	0.03%	0.003%
100	13.848	3881	3890	3905	rVB5	5849	10246	0.90%	0.111%


Sum of corrected areas: 9207760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048179.D
Acq On : 21 Apr 2022 17:40
Operator : SY/MD
Sample : N2485-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

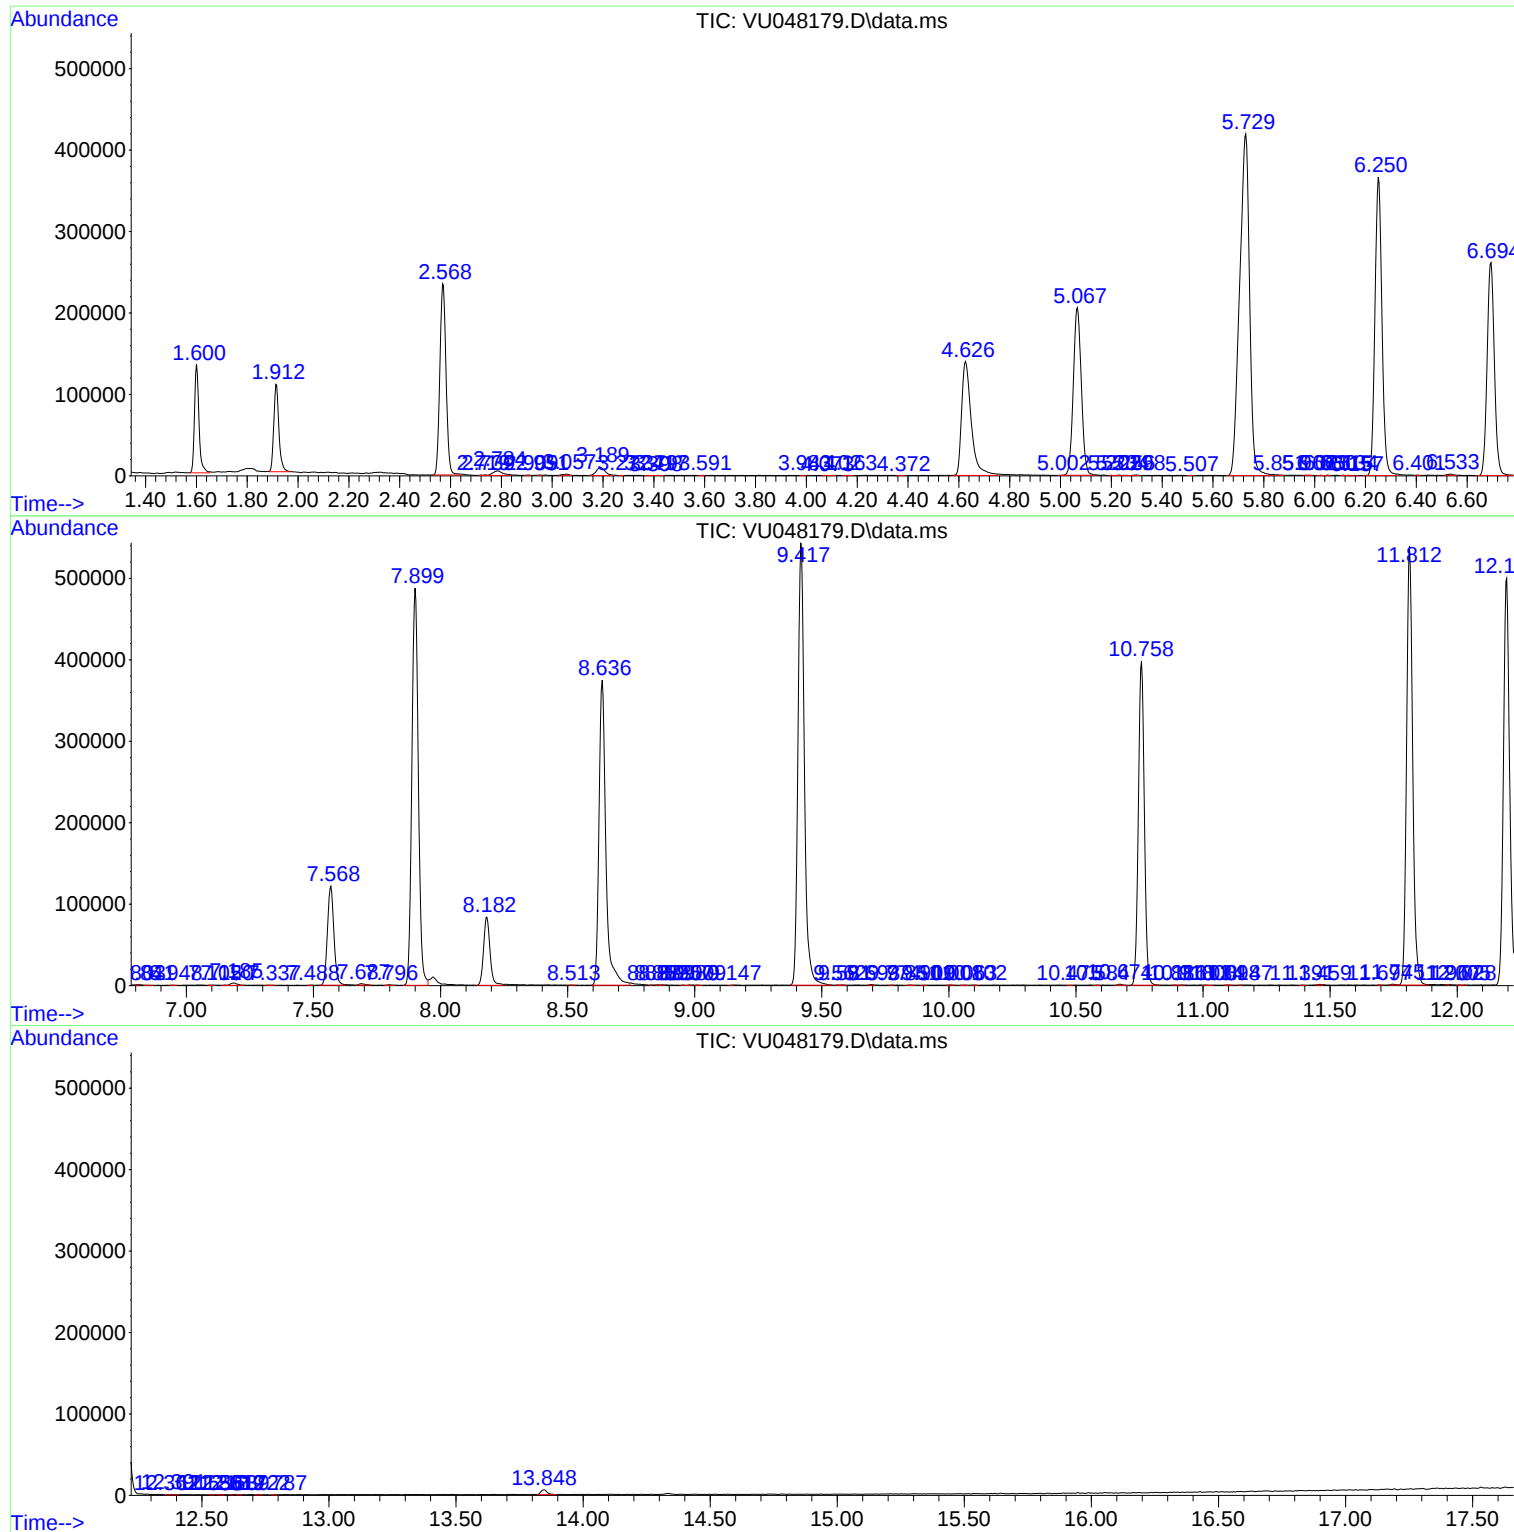

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048179.D
Acq On : 21 Apr 2022 17:40
Operator : SY/MD
Sample : N2485-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048179.D
Acq On : 21 Apr 2022 17:40
Operator : SY/MD
Sample : N2485-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------