

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048183.D
 Acq On : 21 Apr 2022 19:15
 Operator : SY/MD
 Sample : N2486-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	97	rBV	130495	153332	10.59%	1.525%
2	1.916	170	179	198	rVB	106970	149512	10.32%	1.487%
3	2.520	365	367	370	rBV	297	215	0.01%	0.002%
4	2.568	370	382	400	rBV	229578	384609	26.55%	3.826%
5	2.758	438	441	442	rBV2	558	313	0.02%	0.003%
6	2.780	442	448	449	rBV3	3063	2763	0.19%	0.027%
7	2.938	494	497	499	rBV2	301	185	0.01%	0.002%
8	2.951	499	501	504	rVV3	370	233	0.02%	0.002%
9	2.970	504	507	509	rVV2	350	236	0.02%	0.002%
10	3.044	525	530	535	rBV5	921	1024	0.07%	0.010%
11	3.189	562	575	595	rBV2	6825	15758	1.09%	0.157%
12	3.282	600	604	611	rBB2	168	191	0.01%	0.002%
13	3.436	649	652	658	rVB2	305	270	0.02%	0.003%
14	3.504	670	673	677	rVB2	258	203	0.01%	0.002%
15	3.600	695	703	705	rBV2	400	454	0.03%	0.005%
16	3.671	722	725	728	rBV	322	298	0.02%	0.003%
17	3.790	758	762	768	rBV2	216	222	0.02%	0.002%
18	4.089	849	855	858	rBV	257	288	0.02%	0.003%
19	4.134	864	869	873	rBV	247	303	0.02%	0.003%
20	4.243	893	903	905	rBV2	222	332	0.02%	0.003%
21	4.629	1007	1023	1066	rBV2	132200	358468	24.75%	3.566%
22	4.977	1127	1131	1135	rBV3	369	233	0.02%	0.002%
23	5.067	1142	1159	1184	rBV	206530	472457	32.62%	4.699%
24	5.211	1201	1204	1209	rBV3	456	414	0.03%	0.004%
25	5.279	1223	1225	1227	rBV	315	210	0.01%	0.002%
26	5.366	1248	1252	1255	rVB2	344	275	0.02%	0.003%
27	5.385	1255	1258	1259	rBV	284	178	0.01%	0.002%
28	5.523	1292	1301	1302	rBV2	3787	4131	0.29%	0.041%
29	5.729	1343	1365	1399	rBV2	409927	1165648	80.47%	11.594%
30	5.867	1404	1408	1411	rVV2	686	484	0.03%	0.005%
31	5.886	1411	1414	1419	rVB3	297	231	0.02%	0.002%
32	5.976	1439	1442	1447	rBV2	200	180	0.01%	0.002%
33	6.095	1476	1479	1481	rBV	314	176	0.01%	0.002%
34	6.163	1493	1500	1503	rBV2	481	515	0.04%	0.005%
35	6.250	1511	1527	1549	rBV	377195	715648	49.40%	7.118%
36	6.488	1598	1601	1603	rBV2	370	176	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048183.D
 Acq On : 21 Apr 2022 19:15
 Operator : SY/MD
 Sample : N2486-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.526	1607	1613	1614	rBV3	1191	964	0.07%	0.010%
38	6.694	1650	1665	1686	rBV	259846	508235	35.09%	5.055%
39	6.803	1696	1699	1701	rBV2	628	431	0.03%	0.004%
40	6.812	1701	1702	1711	rVB4	1161	1050	0.07%	0.010%
41	6.854	1711	1715	1719	rBV2	387	435	0.03%	0.004%
42	6.960	1745	1748	1752	rBV2	269	223	0.02%	0.002%
43	7.005	1757	1762	1764	rBV2	173	171	0.01%	0.002%
44	7.054	1773	1777	1779	rBV3	368	296	0.02%	0.003%
45	7.102	1787	1792	1795	rBV	222	228	0.02%	0.002%
46	7.185	1810	1818	1827	rBV5	2399	4087	0.28%	0.041%
47	7.369	1872	1875	1879	rVB	265	178	0.01%	0.002%
48	7.449	1897	1900	1903	rVB2	358	251	0.02%	0.002%
49	7.478	1903	1909	1911	rBV2	219	227	0.02%	0.002%
50	7.568	1925	1937	1957	rBV	114381	206820	14.28%	2.057%
51	7.693	1969	1976	1990	rVB5	1838	3947	0.27%	0.039%
52	7.771	1997	2000	2004	rVB3	273	177	0.01%	0.002%
53	7.793	2004	2007	2011	rVB2	224	207	0.01%	0.002%
54	7.899	2020	2040	2057	rBV	487317	843827	58.25%	8.393%
55	8.182	2116	2128	2142	rBV	81513	142194	9.82%	1.414%
56	8.414	2196	2200	2203	rVB2	367	258	0.02%	0.003%
57	8.472	2214	2218	2222	rBV3	462	431	0.03%	0.004%
58	8.578	2249	2251	2256	rVB	287	250	0.02%	0.002%
59	8.636	2256	2269	2310	rBV	359683	694859	47.97%	6.911%
60	8.951	2360	2367	2370	rBV3	470	486	0.03%	0.005%
61	9.420	2499	2513	2515	rBV	602211	819771	56.59%	8.154%
62	9.600	2567	2569	2574	rVB2	646	478	0.03%	0.005%
63	9.671	2587	2591	2593	rBV2	333	236	0.02%	0.002%
64	9.697	2593	2599	2605	rVV3	983	1277	0.09%	0.013%
65	9.754	2613	2617	2619	rBV	344	196	0.01%	0.002%
66	10.092	2719	2722	2724	rBV	316	221	0.02%	0.002%
67	10.147	2735	2739	2743	rVV3	189	172	0.01%	0.002%
68	10.250	2768	2771	2774	rBV	261	186	0.01%	0.002%
69	10.671	2894	2902	2909	rBV3	996	1492	0.10%	0.015%
70	10.758	2915	2929	2950	rBV	396416	642355	44.34%	6.389%
71	10.889	2965	2970	2971	rBV	624	501	0.03%	0.005%
72	11.095	3031	3034	3037	rVB2	305	196	0.01%	0.002%
73	11.340	3105	3110	3116	rVB3	294	324	0.02%	0.003%
74	11.465	3143	3149	3151	rBV5	588	600	0.04%	0.006%
75	11.558	3173	3178	3179	rBV2	254	218	0.02%	0.002%
76	11.745	3226	3236	3245	rBV	26702	41681	2.88%	0.415%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048183.D
 Acq On : 21 Apr 2022 19:15
 Operator : SY/MD
 Sample : N2486-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.812	3245	3257	3280	rVB2	572827	1146423	79.14%	11.403%
78	11.922	3288	3291	3293	rBV2	368	211	0.01%	0.002%
79	11.960	3299	3303	3304	rBV2	365	266	0.02%	0.003%
80	12.069	3331	3337	3343	rBV3	1781	2169	0.15%	0.022%
81	12.115	3348	3351	3355	rVB2	341	303	0.02%	0.003%
82	12.198	3362	3377	3400	rBV2	609012	1448578	100.00%	14.408%
83	12.372	3429	3431	3434	rBV2	349	196	0.01%	0.002%
84	12.426	3446	3448	3451	rVB2	398	196	0.01%	0.002%
85	12.446	3451	3454	3456	rBV	241	176	0.01%	0.002%
86	12.539	3480	3483	3484	rBV2	342	174	0.01%	0.002%
87	12.696	3527	3532	3534	rBV3	549	554	0.04%	0.006%
88	12.741	3543	3546	3549	rBV3	369	249	0.02%	0.002%
89	12.780	3555	3558	3560	rBV2	384	238	0.02%	0.002%
90	12.886	3587	3591	3595	rBV2	263	223	0.02%	0.002%
91	12.909	3595	3598	3601	rVB2	434	321	0.02%	0.003%
92	12.954	3610	3612	3617	rVB2	298	197	0.01%	0.002%
93	13.092	3652	3655	3657	rBV2	282	186	0.01%	0.002%
94	13.378	3741	3744	3749	rBV	345	351	0.02%	0.003%
95	13.774	3864	3867	3868	rBV2	382	234	0.02%	0.002%
96	13.841	3877	3888	3904	rBV	49582	77739	5.37%	0.773%
97	14.333	4031	4041	4053	rVB2	15613	23424	1.62%	0.233%
98	14.674	4145	4147	4151	rBV2	402	285	0.02%	0.003%
99	15.278	4332	4335	4336	rBV2	471	290	0.02%	0.003%
100	15.397	4368	4372	4374	rBV3	592	480	0.03%	0.005%



Sum of corrected areas: 10053764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048183.D
Acq On : 21 Apr 2022 19:15
Operator : SY/MD
Sample : N2486-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

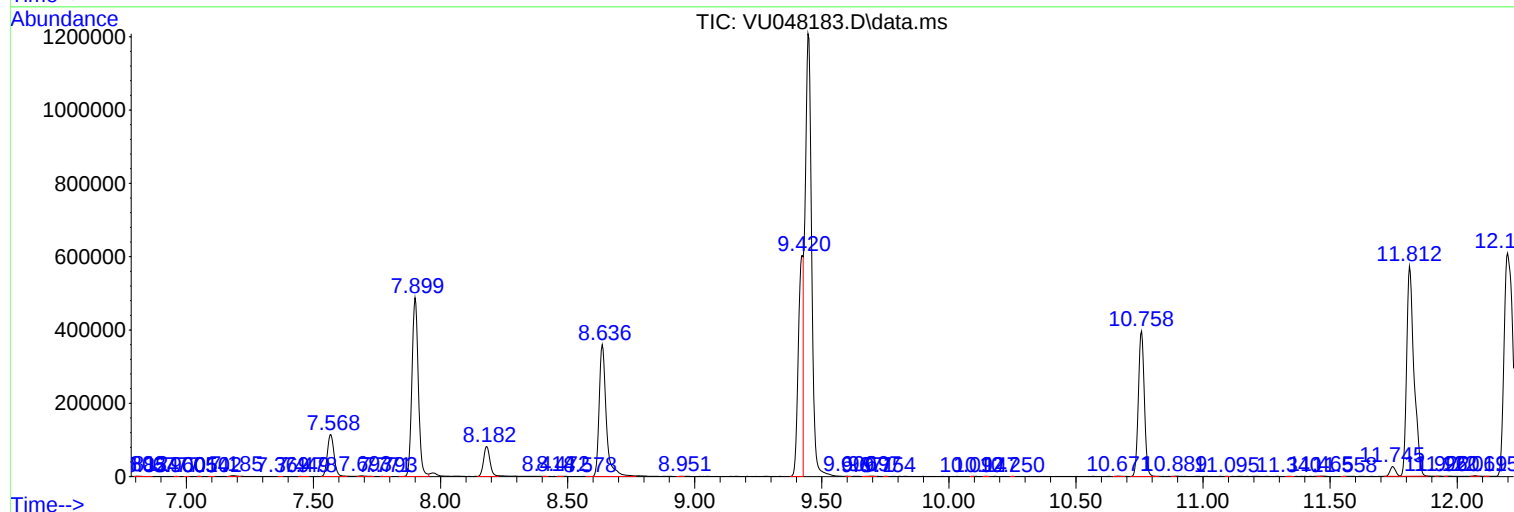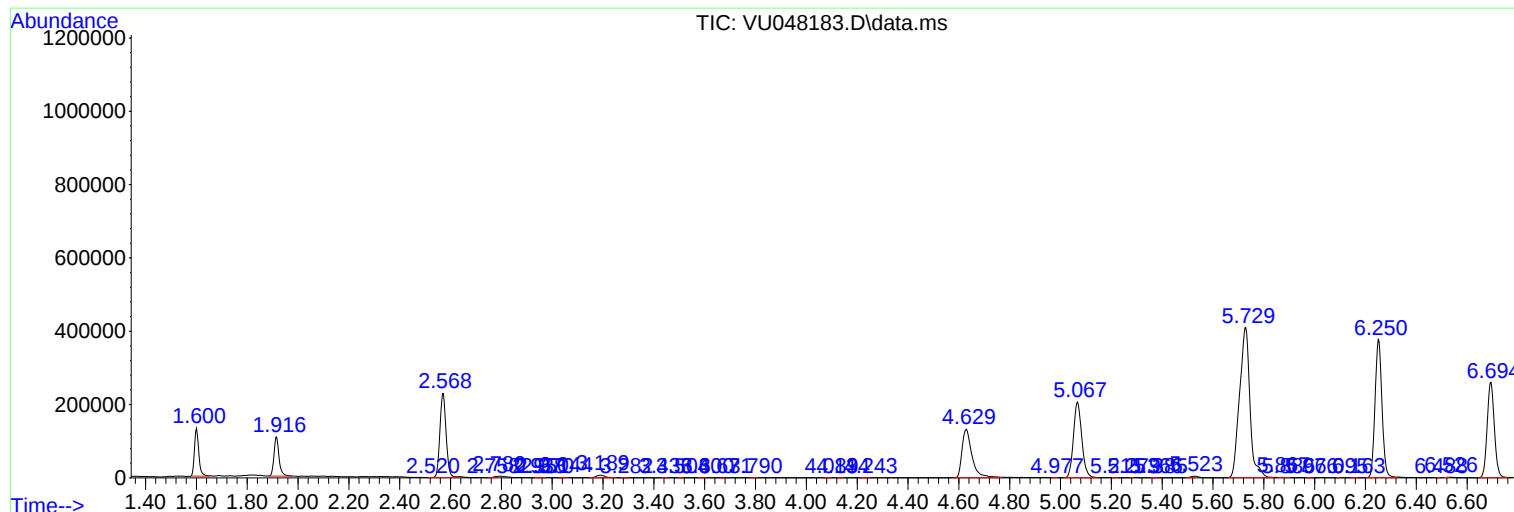

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048183.D
Acq On : 21 Apr 2022 19:15
Operator : SY/MD
Sample : N2486-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048183.D
Acq On : 21 Apr 2022 19:15
Operator : SY/MD
Sample : N2486-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc