

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048184.D
 Acq On : 21 Apr 2022 19:39
 Operator : SY/MD
 Sample : N2486-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	128076	150756	13.36%	1.635%
2	1.916	171	179	201	rVB	111322	154551	13.70%	1.676%
3	2.494	356	359	362	rBV3	410	365	0.03%	0.004%
4	2.568	371	382	408	rBV	226614	383384	33.98%	4.157%
5	2.742	433	436	440	rBV2	246	192	0.02%	0.002%
6	2.893	481	483	487	rBV	273	176	0.02%	0.002%
7	2.961	499	504	506	rVB3	298	216	0.02%	0.002%
8	3.002	514	517	519	rBV	259	178	0.02%	0.002%
9	3.044	523	530	535	rBV4	628	895	0.08%	0.010%
10	3.134	554	558	561	rBV3	473	344	0.03%	0.004%
11	3.186	565	574	575	rBV2	2108	2470	0.22%	0.027%
12	3.327	613	618	622	rBV	266	192	0.02%	0.002%
13	3.347	622	624	629	rBV	254	197	0.02%	0.002%
14	3.395	635	639	642	rBV	314	222	0.02%	0.002%
15	3.469	659	662	664	rBV	265	190	0.02%	0.002%
16	3.658	715	721	725	rVB2	254	327	0.03%	0.004%
17	3.700	731	734	739	rBV2	219	172	0.02%	0.002%
18	3.761	748	753	758	rVB2	256	314	0.03%	0.003%
19	3.790	758	762	763	rBV	306	237	0.02%	0.003%
20	3.822	768	772	775	rVV2	372	287	0.03%	0.003%
21	3.855	778	782	787	rVB2	399	400	0.04%	0.004%
22	3.880	787	790	792	rBV	198	153	0.01%	0.002%
23	4.015	826	832	834	rBV	207	231	0.02%	0.003%
24	4.035	834	838	842	rBV	219	293	0.03%	0.003%
25	4.089	849	855	857	rBV	181	197	0.02%	0.002%
26	4.305	920	922	926	rVB2	217	166	0.01%	0.002%
27	4.498	978	982	986	rVB	189	184	0.02%	0.002%
28	4.575	1001	1006	1010	rBV2	204	243	0.02%	0.003%
29	4.633	1010	1024	1069	rBV	118948	333674	29.57%	3.618%
30	5.067	1142	1159	1188	rBV	202743	445825	39.51%	4.834%
31	5.282	1222	1226	1227	rBV	446	256	0.02%	0.003%
32	5.565	1311	1314	1316	rBV	256	220	0.02%	0.002%
33	5.729	1340	1365	1400	rBV2	411642	1128303	100.00%	12.235%
34	6.141	1489	1493	1498	rBV2	161	184	0.02%	0.002%
35	6.250	1510	1527	1559	rVV	383432	732779	64.95%	7.946%
36	6.485	1597	1600	1603	rBV2	229	160	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048184.D
 Acq On : 21 Apr 2022 19:39
 Operator : SY/MD
 Sample : N2486-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.533	1609	1615	1623	rVB5	1548	2325	0.21%	0.025%
38	6.581	1628	1630	1632	rBV	422	197	0.02%	0.002%
39	6.694	1650	1665	1683	rBV	258161	507811	45.01%	5.507%
40	6.806	1696	1700	1704	rBV3	437	499	0.04%	0.005%
41	7.028	1765	1769	1772	rBV2	183	171	0.02%	0.002%
42	7.047	1772	1775	1782	rVV2	216	194	0.02%	0.002%
43	7.128	1796	1800	1801	rBV	259	179	0.02%	0.002%
44	7.186	1811	1818	1828	rBV2	2037	3699	0.33%	0.040%
45	7.289	1843	1850	1853	rBV2	380	460	0.04%	0.005%
46	7.462	1900	1904	1909	rBV2	221	251	0.02%	0.003%
47	7.568	1924	1937	1956	rBV	117411	209243	18.54%	2.269%
48	7.655	1961	1964	1967	rBV3	365	292	0.03%	0.003%
49	7.694	1968	1976	1978	rBV4	1065	1338	0.12%	0.015%
50	7.899	2026	2040	2056	rBV	478613	837873	74.26%	9.086%
51	8.137	2109	2114	2115	rBV	261	182	0.02%	0.002%
52	8.179	2115	2127	2146	rBV	80142	144289	12.79%	1.565%
53	8.314	2166	2169	2171	rVB2	536	314	0.03%	0.003%
54	8.559	2243	2245	2250	rVB2	458	335	0.03%	0.004%
55	8.584	2250	2253	2256	rBV	170	158	0.01%	0.002%
56	8.636	2256	2269	2302	rBV2	354231	703400	62.34%	7.628%
57	9.054	2396	2399	2403	rVB3	283	251	0.02%	0.003%
58	9.141	2422	2426	2430	rBV3	256	241	0.02%	0.003%
59	9.243	2455	2458	2461	rVV	273	183	0.02%	0.002%
60	9.417	2499	2512	2537	rBV	568210	1004593	89.04%	10.894%
61	9.616	2570	2574	2580	rBV3	226	228	0.02%	0.002%
62	9.700	2592	2600	2604	rBV4	850	1037	0.09%	0.011%
63	9.732	2607	2610	2614	rBV3	214	165	0.01%	0.002%
64	9.915	2664	2667	2670	rBV	161	174	0.02%	0.002%
65	10.099	2720	2724	2731	rVB2	435	579	0.05%	0.006%
66	10.134	2731	2735	2742	rBV3	288	420	0.04%	0.005%
67	10.314	2790	2791	2794	rBV2	311	165	0.01%	0.002%
68	10.346	2799	2801	2806	rVB2	342	252	0.02%	0.003%
69	10.491	2843	2846	2849	rVB	279	196	0.02%	0.002%
70	10.530	2851	2858	2862	rBV2	333	401	0.04%	0.004%
71	10.575	2870	2872	2879	rVB	262	221	0.02%	0.002%
72	10.610	2879	2883	2886	rBV	187	166	0.01%	0.002%
73	10.668	2896	2901	2909	rVB3	762	1059	0.09%	0.011%
74	10.758	2915	2929	2949	rBV	397628	646243	57.28%	7.008%
75	10.893	2963	2971	2980	rBV3	1107	1856	0.16%	0.020%
76	11.182	3058	3061	3066	rVB2	290	280	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048184.D
 Acq On : 21 Apr 2022 19:39
 Operator : SY/MD
 Sample : N2486-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.211	3066	3070	3074	rBV3	445	509	0.05%	0.006%
78	11.449	3142	3144	3148	rVV3	419	372	0.03%	0.004%
79	11.472	3149	3151	3155	rVV2	648	485	0.04%	0.005%
80	11.639	3200	3203	3206	rBV	211	162	0.01%	0.002%
81	11.697	3216	3221	3227	rVB3	350	451	0.04%	0.005%
82	11.745	3229	3236	3245	rBV4	2876	3812	0.34%	0.041%
83	11.812	3245	3257	3277	rBV	562812	936804	83.03%	10.159%
84	12.066	3329	3336	3346	rBV7	3010	5366	0.48%	0.058%
85	12.144	3356	3360	3362	rBV2	273	191	0.02%	0.002%
86	12.195	3362	3376	3397	rBV	494836	847528	75.12%	9.191%
87	12.324	3414	3416	3419	rVB	453	205	0.02%	0.002%
88	12.394	3433	3438	3440	rBV3	433	384	0.03%	0.004%
89	12.494	3466	3469	3473	rBV	237	208	0.02%	0.002%
90	12.774	3554	3556	3559	rVB2	342	151	0.01%	0.002%
91	12.828	3568	3573	3577	rBV	484	492	0.04%	0.005%
92	12.854	3578	3581	3585	rBV2	450	386	0.03%	0.004%
93	12.928	3601	3604	3605	rBV2	257	166	0.01%	0.002%
94	12.992	3621	3624	3627	rBV2	294	261	0.02%	0.003%
95	13.845	3882	3889	3900	rVB2	6208	8946	0.79%	0.097%
96	14.336	4035	4042	4051	rVB5	2231	3068	0.27%	0.033%
97	14.735	4163	4166	4168	rBV	434	203	0.02%	0.002%
98	14.761	4172	4174	4178	rVB	431	205	0.02%	0.002%
99	14.909	4217	4220	4223	rBV	458	305	0.03%	0.003%
100	15.153	4294	4296	4299	rBV3	451	230	0.02%	0.002%




Sum of corrected areas: 9221743

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048184.D
Acq On : 21 Apr 2022 19:39
Operator : SY/MD
Sample : N2486-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

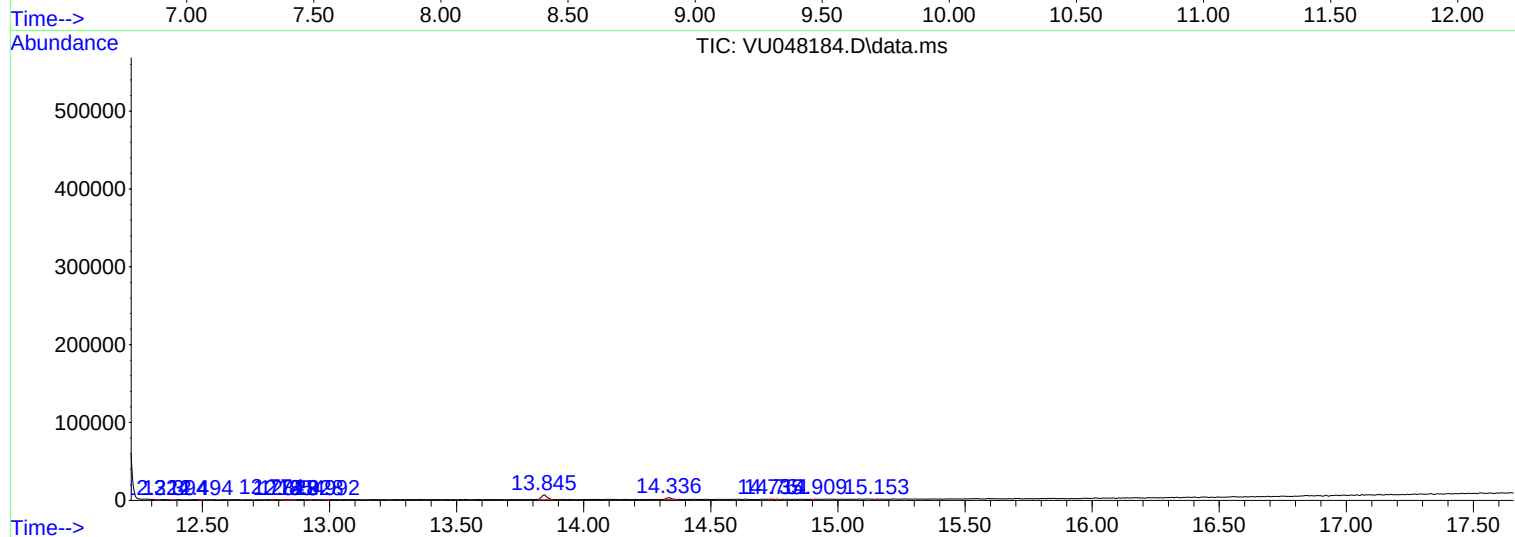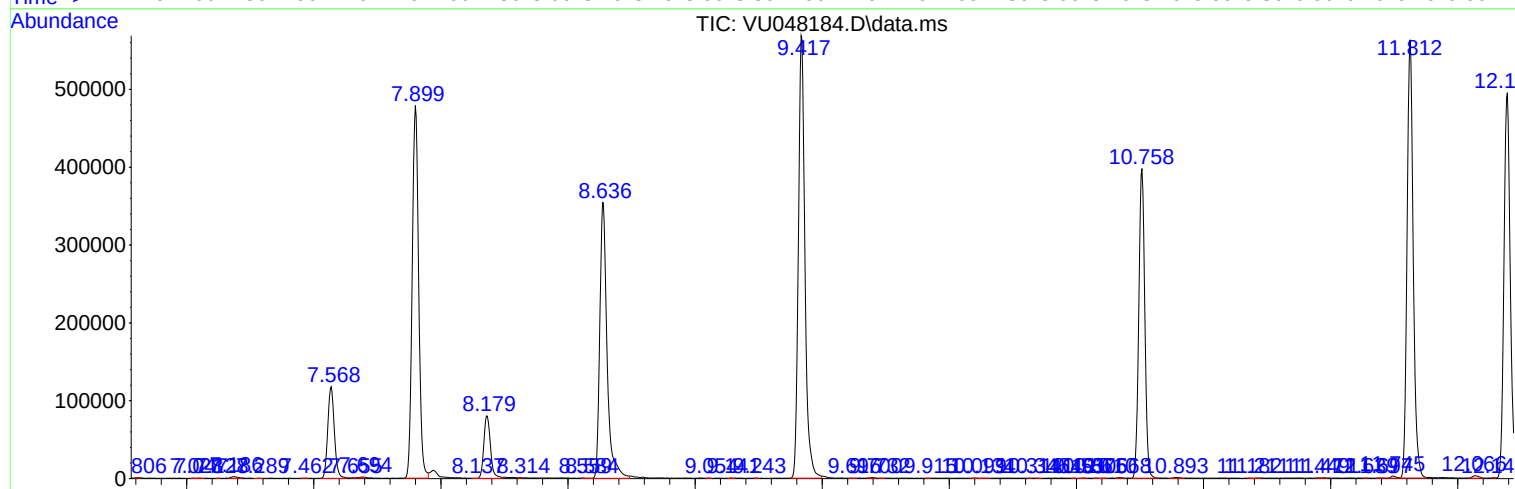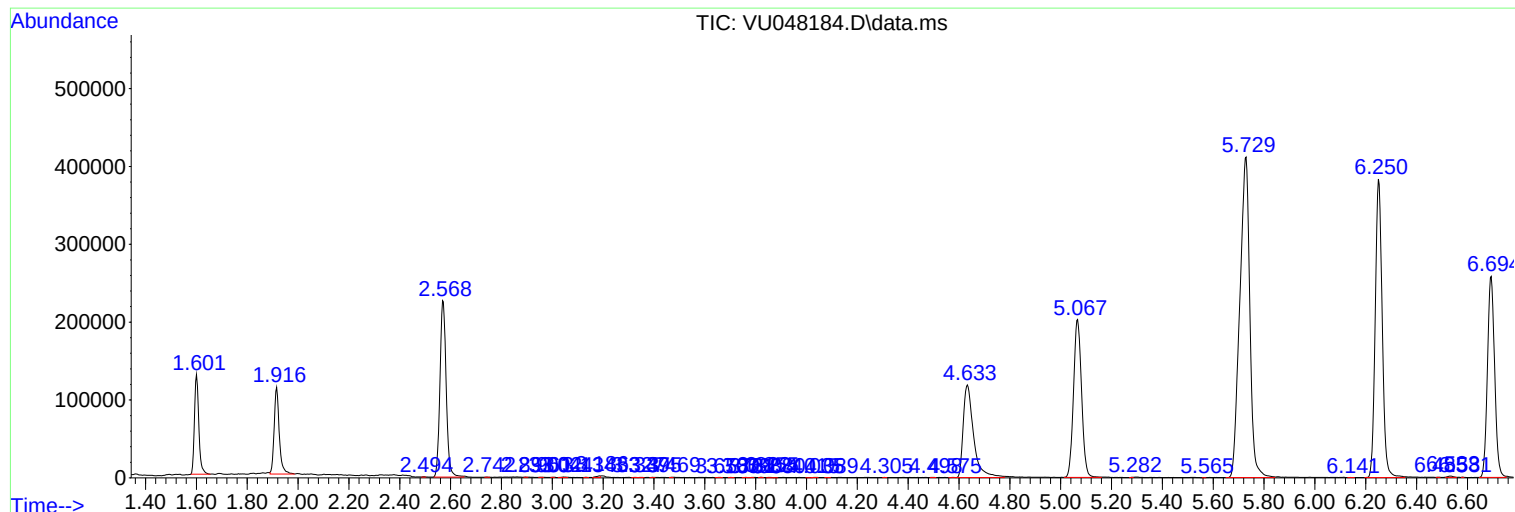

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048184.D
Acq On : 21 Apr 2022 19:39
Operator : SY/MD
Sample : N2486-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048184.D
Acq On : 21 Apr 2022 19:39
Operator : SY/MD
Sample : N2486-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------