

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048185.D
 Acq On : 21 Apr 2022 20:02
 Operator : SY/MD
 Sample : N2486-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	19	rVB	7361	8055	0.21%	0.059%
2	1.601	73	81	95	rBV	129913	153998	3.99%	1.132%
3	1.916	171	179	195	rVB	105647	145329	3.76%	1.068%
4	2.568	370	382	399	rBV	224676	377559	9.77%	2.774%
5	2.790	446	451	454	rBV3	666	690	0.02%	0.005%
6	2.848	467	469	471	rBV3	306	193	0.00%	0.001%
7	2.893	480	483	490	rVB3	381	305	0.01%	0.002%
8	2.964	501	505	511	rVB3	521	499	0.01%	0.004%
9	3.044	524	530	542	rBV5	822	1366	0.04%	0.010%
10	3.096	543	546	550	rVV2	260	212	0.01%	0.002%
11	3.189	565	575	587	rBV2	1106	2321	0.06%	0.017%
12	4.205	885	891	894	rBV	241	270	0.01%	0.002%
13	4.327	925	929	937	rVB2	215	293	0.01%	0.002%
14	4.629	1010	1023	1065	rBV	116553	312447	8.09%	2.296%
15	4.851	1087	1092	1096	rBV2	414	386	0.01%	0.003%
16	4.932	1112	1117	1126	rBV2	395	727	0.02%	0.005%
17	5.067	1141	1159	1177	rBV	196620	436610	11.30%	3.208%
18	5.215	1199	1205	1206	rBV2	362	263	0.01%	0.002%
19	5.237	1210	1212	1218	rVB2	419	256	0.01%	0.002%
20	5.295	1226	1230	1232	rBV2	421	336	0.01%	0.002%
21	5.465	1276	1283	1286	rBV2	244	401	0.01%	0.003%
22	5.523	1298	1301	1306	rVV2	263	265	0.01%	0.002%
23	5.549	1306	1309	1316	rVB	318	335	0.01%	0.002%
24	5.587	1316	1321	1325	rBV2	246	280	0.01%	0.002%
25	5.729	1342	1365	1399	rBV2	407049	1106411	28.64%	8.130%
26	6.025	1453	1457	1461	rVV2	211	240	0.01%	0.002%
27	6.073	1467	1472	1477	rBV3	234	278	0.01%	0.002%
28	6.112	1481	1484	1488	rBV2	496	374	0.01%	0.003%
29	6.250	1512	1527	1547	rBV	373778	714752	18.50%	5.252%
30	6.388	1567	1570	1573	rVB2	394	218	0.01%	0.002%
31	6.533	1608	1615	1624	rVB5	1933	2887	0.07%	0.021%
32	6.626	1641	1644	1648	rBV2	297	250	0.01%	0.002%
33	6.694	1649	1665	1686	rBV	258076	502876	13.02%	3.695%
34	6.803	1696	1699	1706	rVB3	668	600	0.02%	0.004%
35	7.095	1787	1790	1795	rVB	259	183	0.00%	0.001%
36	7.179	1809	1816	1819	rBV5	2121	2509	0.06%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048185.D
 Acq On : 21 Apr 2022 20:02
 Operator : SY/MD
 Sample : N2486-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.259	1835	1841	1843	rBV2	229	223	0.01%	0.002%
38	7.276	1843	1846	1850	rVB	300	214	0.01%	0.002%
39	7.333	1856	1864	1866	rBV2	306	469	0.01%	0.003%
40	7.391	1874	1882	1883	rBV2	195	257	0.01%	0.002%
41	7.568	1924	1937	1954	rBV	112278	201949	5.23%	1.484%
42	7.687	1968	1974	1976	rBV3	1190	1040	0.03%	0.008%
43	7.790	2003	2006	2012	rBV2	311	266	0.01%	0.002%
44	7.899	2026	2040	2056	rBV	480587	827598	21.42%	6.081%
45	8.112	2104	2106	2114	rVB3	298	298	0.01%	0.002%
46	8.182	2116	2128	2144	rBV	79711	138787	3.59%	1.020%
47	8.259	2149	2152	2160	rVB6	928	978	0.03%	0.007%
48	8.420	2200	2202	2205	rVB2	504	272	0.01%	0.002%
49	8.526	2230	2235	2240	rBV4	313	402	0.01%	0.003%
50	8.558	2242	2245	2252	rVB2	342	259	0.01%	0.002%
51	8.636	2256	2269	2314	rBV2	355101	690153	17.86%	5.071%
52	8.790	2314	2317	2319	rVV4	814	482	0.01%	0.004%
53	8.829	2326	2329	2331	rBV2	380	249	0.01%	0.002%
54	8.899	2346	2351	2353	rBV2	456	285	0.01%	0.002%
55	9.079	2404	2407	2410	rBV2	324	225	0.01%	0.002%
56	9.166	2430	2434	2437	rBV2	324	271	0.01%	0.002%
57	9.189	2437	2441	2446	rBV2	334	250	0.01%	0.002%
58	9.317	2479	2481	2486	rVB2	338	205	0.01%	0.002%
59	9.420	2498	2513	2519	rBV	574368	1056213	27.34%	7.761%
60	9.568	2555	2559	2564	rVB2	550	537	0.01%	0.004%
61	9.591	2564	2566	2568	rBV2	482	275	0.01%	0.002%
62	9.690	2591	2597	2598	rBV4	832	622	0.02%	0.005%
63	9.828	2638	2640	2646	rBV2	253	193	0.00%	0.001%
64	9.922	2664	2669	2671	rBV2	213	191	0.00%	0.001%
65	10.436	2825	2829	2833	rVB3	284	217	0.01%	0.002%
66	10.655	2892	2897	2898	rBV	515	366	0.01%	0.003%
67	10.668	2899	2901	2908	rVB3	928	937	0.02%	0.007%
68	10.758	2916	2929	2945	rBV	395565	630528	16.32%	4.633%
69	10.886	2963	2969	2970	rBV2	1292	958	0.02%	0.007%
70	10.983	2994	2999	3000	rBV3	997	744	0.02%	0.005%
71	11.099	3030	3035	3037	rBV2	320	317	0.01%	0.002%
72	11.217	3070	3072	3075	rVB2	392	186	0.00%	0.001%
73	11.472	3146	3151	3154	rBV3	553	434	0.01%	0.003%
74	11.558	3175	3178	3180	rBV	385	233	0.01%	0.002%
75	11.690	3215	3219	3220	rBV	358	262	0.01%	0.002%
76	11.745	3224	3236	3247	rBV	457302	737888	19.10%	5.422%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048185.D
 Acq On : 21 Apr 2022 20:02
 Operator : SY/MD
 Sample : N2486-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.835	3247	3264	3287	rVB2	1880350	3863367	100.00%	28.387%
78	12.066	3328	3336	3349	rBV2	7907	13538	0.35%	0.099%
79	12.195	3362	3376	3396	rBV2	546794	1056745	27.35%	7.765%
80	12.404	3438	3441	3443	rBV2	330	254	0.01%	0.002%
81	12.504	3468	3472	3475	rVB2	453	324	0.01%	0.002%
82	12.523	3475	3478	3482	rBV3	232	209	0.01%	0.002%
83	12.542	3482	3484	3487	rBV3	345	195	0.01%	0.001%
84	12.565	3488	3491	3495	rVB3	470	426	0.01%	0.003%
85	12.590	3495	3499	3500	rBV3	325	200	0.01%	0.001%
86	12.706	3532	3535	3537	rBV2	519	354	0.01%	0.003%
87	12.828	3569	3573	3578	rBV3	474	622	0.02%	0.005%
88	12.922	3597	3602	3606	rBV2	385	420	0.01%	0.003%
89	12.973	3611	3618	3626	rVB4	2567	4054	0.10%	0.030%
90	13.063	3643	3646	3652	rVB2	373	315	0.01%	0.002%
91	13.150	3662	3673	3686	rBV2	6521	14110	0.37%	0.104%
92	13.224	3689	3696	3703	rVB3	3047	4788	0.12%	0.035%
93	13.330	3726	3729	3732	rBV2	318	253	0.01%	0.002%
94	13.568	3798	3803	3806	rBV5	686	735	0.02%	0.005%
95	13.841	3876	3888	3909	rBV	255441	408196	10.57%	2.999%
96	14.330	4028	4040	4058	rBV	98762	157672	4.08%	1.159%
97	14.603	4122	4125	4129	rBV	627	494	0.01%	0.004%
98	15.031	4255	4258	4259	rBV2	693	349	0.01%	0.003%
99	15.417	4372	4378	4387	rVB5	3222	4984	0.13%	0.037%
100	15.999	4555	4559	4572	rVB8	3869	5857	0.15%	0.043%




Sum of corrected areas: 13609668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048185.D
Acq On : 21 Apr 2022 20:02
Operator : SY/MD
Sample : N2486-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

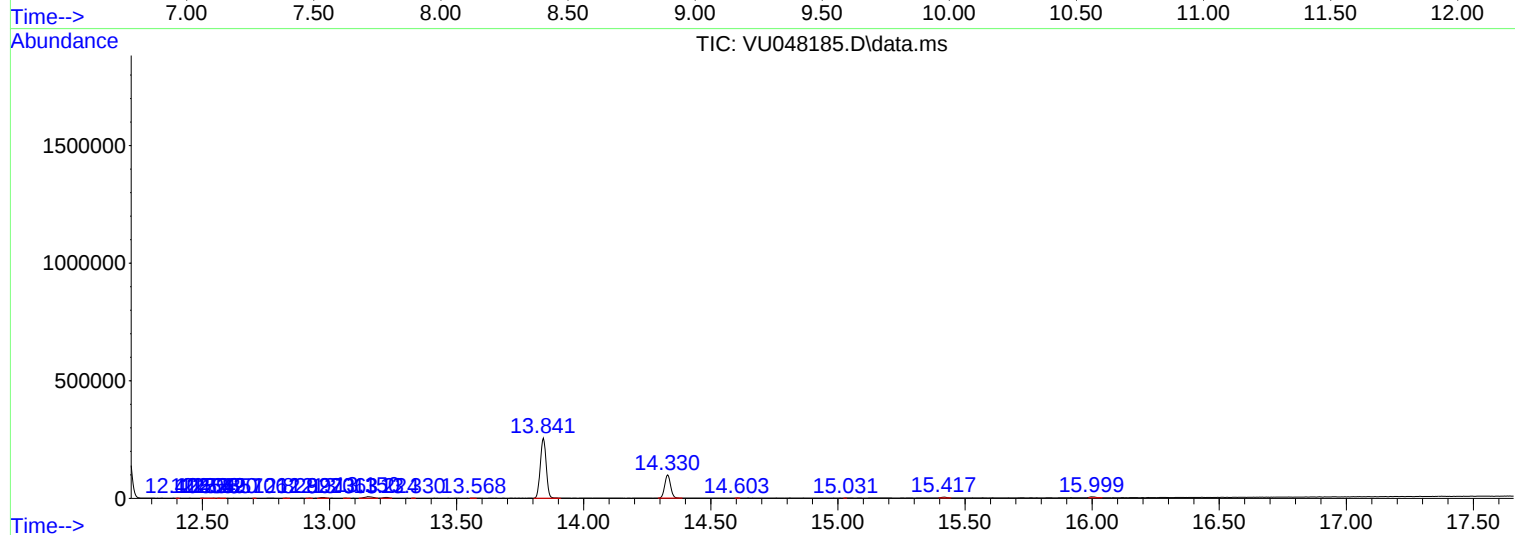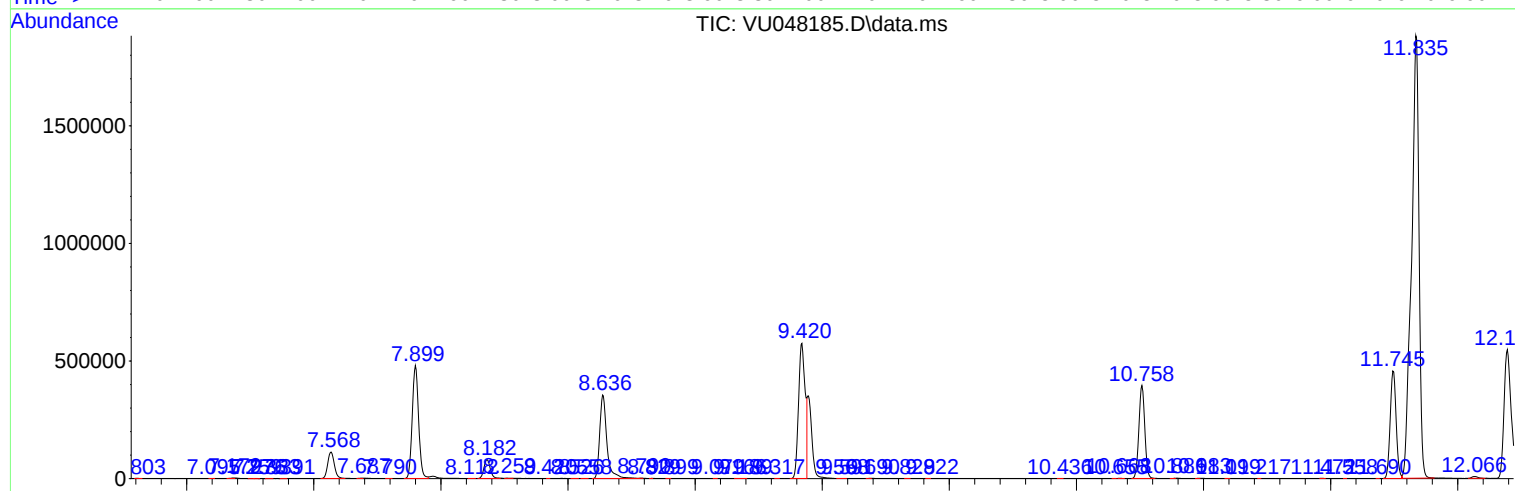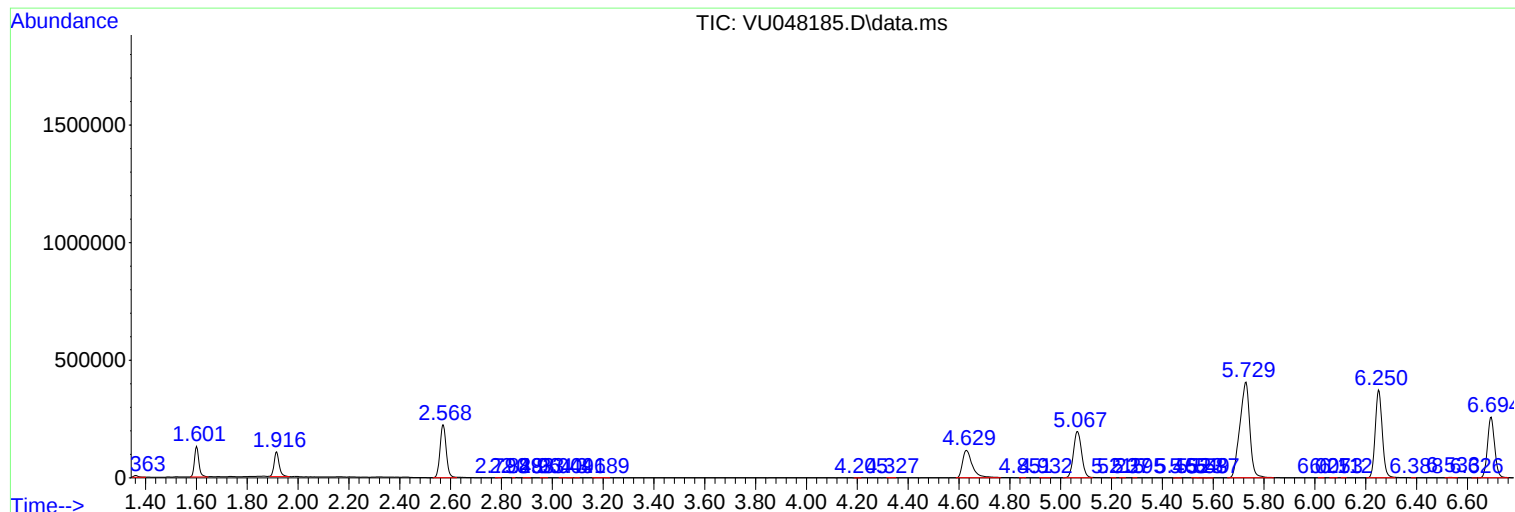

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048185.D
Acq On : 21 Apr 2022 20:02
Operator : SY/MD
Sample : N2486-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048185.D
Acq On : 21 Apr 2022 20:02
Operator : SY/MD
Sample : N2486-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------