

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048187.D
 Acq On : 21 Apr 2022 21:19
 Operator : SY/MD
 Sample : VU0421WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	104	rVB	131355	156796	13.35%	1.682%
2	1.916	170	179	200	rVB	107075	154314	13.14%	1.655%
3	2.568	370	382	400	rVV	236230	393791	33.52%	4.224%
4	2.797	446	453	459	rVB	732	898	0.08%	0.010%
5	2.954	497	502	503	rBV	201	170	0.01%	0.002%
6	2.999	513	516	518	rBV2	327	224	0.02%	0.002%
7	3.051	523	532	541	rBV4	1888	3431	0.29%	0.037%
8	3.147	559	562	564	rVB	281	180	0.02%	0.002%
9	3.182	564	573	575	rBV5	2175	2776	0.24%	0.030%
10	3.382	631	635	636	rBV2	327	215	0.02%	0.002%
11	3.768	747	755	757	rBV2	223	317	0.03%	0.003%
12	3.835	770	776	780	rBB2	204	213	0.02%	0.002%
13	3.909	796	799	802	rBV2	184	168	0.01%	0.002%
14	4.173	876	881	885	rBV	178	182	0.02%	0.002%
15	4.279	911	914	917	rVB2	258	168	0.01%	0.002%
16	4.308	917	923	927	rBV2	212	268	0.02%	0.003%
17	4.452	965	968	973	rVB2	262	244	0.02%	0.003%
18	4.481	973	977	980	rBV2	282	201	0.02%	0.002%
19	4.536	990	994	1000	rVB2	210	242	0.02%	0.003%
20	4.626	1008	1022	1056	rBV	135003	346620	29.50%	3.718%
21	5.067	1141	1159	1181	rBV	215626	471912	40.17%	5.062%
22	5.378	1251	1256	1259	rBV2	469	472	0.04%	0.005%
23	5.729	1343	1365	1399	rVV2	430688	1174829	100.00%	12.601%
24	5.845	1399	1401	1406	rVB3	791	511	0.04%	0.005%
25	6.015	1449	1454	1457	rBV2	199	212	0.02%	0.002%
26	6.076	1471	1473	1478	rVB2	243	174	0.01%	0.002%
27	6.112	1481	1484	1485	rBV2	309	178	0.02%	0.002%
28	6.121	1485	1487	1491	rVB2	366	267	0.02%	0.003%
29	6.250	1513	1527	1561	rBV	346766	667933	56.85%	7.164%
30	6.526	1607	1613	1615	rBV4	1846	1945	0.17%	0.021%
31	6.694	1649	1665	1683	rBV	270974	532960	45.36%	5.717%
32	6.976	1749	1753	1755	rBV	225	219	0.02%	0.002%
33	7.054	1770	1777	1782	rBV2	463	766	0.07%	0.008%
34	7.185	1810	1818	1828	rVV4	2519	4555	0.39%	0.049%
35	7.269	1841	1844	1847	rVV	341	209	0.02%	0.002%
36	7.465	1902	1905	1914	rVB2	272	259	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048187.D
 Acq On : 21 Apr 2022 21:19
 Operator : SY/MD
 Sample : VU0421WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.568	1924	1937	1954	rBV	132142	236553	20.14%	2.537%
38	7.687	1968	1974	1976	rBV4	1508	1547	0.13%	0.017%
39	7.800	1999	2009	2018	rVV6	1541	2362	0.20%	0.025%
40	7.899	2026	2040	2057	rBV	508680	888380	75.62%	9.529%
41	8.089	2096	2099	2101	rBV3	293	250	0.02%	0.003%
42	8.182	2115	2128	2141	rBV	92678	160297	13.64%	1.719%
43	8.343	2176	2178	2181	rVB3	452	221	0.02%	0.002%
44	8.385	2186	2191	2195	rBV3	403	526	0.04%	0.006%
45	8.404	2195	2197	2200	rVB2	348	192	0.02%	0.002%
46	8.636	2256	2269	2311	rVV	392825	739432	62.94%	7.931%
47	9.057	2396	2400	2406	rBV4	378	324	0.03%	0.003%
48	9.092	2408	2411	2416	rBB2	378	277	0.02%	0.003%
49	9.163	2430	2433	2437	rBV	309	222	0.02%	0.002%
50	9.285	2468	2471	2475	rVV	311	206	0.02%	0.002%
51	9.417	2499	2512	2548	rVV	520247	906965	77.20%	9.728%
52	9.536	2548	2549	2553	rVV2	573	310	0.03%	0.003%
53	9.562	2554	2557	2558	rVV	428	232	0.02%	0.002%
54	9.571	2558	2560	2568	rVB3	754	720	0.06%	0.008%
55	9.610	2569	2572	2578	rVB3	315	251	0.02%	0.003%
56	9.639	2578	2581	2583	rBV2	335	173	0.01%	0.002%
57	9.697	2588	2599	2607	rBV4	1412	2248	0.19%	0.024%
58	9.767	2618	2621	2626	rVB2	241	207	0.02%	0.002%
59	9.796	2626	2630	2633	rBV	335	229	0.02%	0.002%
60	9.944	2672	2676	2681	rBV2	156	194	0.02%	0.002%
61	10.111	2719	2728	2737	rBV4	1291	1706	0.15%	0.018%
62	10.163	2738	2744	2747	rBV	179	189	0.02%	0.002%
63	10.243	2766	2769	2772	rBV2	207	182	0.02%	0.002%
64	10.369	2805	2808	2813	rVB	384	311	0.03%	0.003%
65	10.398	2813	2817	2823	rVB3	357	339	0.03%	0.004%
66	10.430	2823	2827	2831	rBV	326	327	0.03%	0.004%
67	10.488	2839	2845	2851	rVB	811	898	0.08%	0.010%
68	10.671	2893	2902	2907	rBV2	1880	2299	0.20%	0.025%
69	10.758	2916	2929	2947	rBV	420618	683375	58.17%	7.330%
70	10.873	2959	2965	2969	rVB4	325	364	0.03%	0.004%
71	10.893	2969	2971	2972	rBV	410	167	0.01%	0.002%
72	10.925	2979	2981	2985	rBV2	315	261	0.02%	0.003%
73	10.980	2994	2998	3000	rBV2	224	195	0.02%	0.002%
74	11.089	3028	3032	3040	rVB4	518	703	0.06%	0.008%
75	11.160	3051	3054	3058	rVB3	282	192	0.02%	0.002%
76	11.246	3077	3081	3084	rBV3	233	174	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048187.D
 Acq On : 21 Apr 2022 21:19
 Operator : SY/MD
 Sample : VU0421WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.465	3141	3149	3160	rVB6	1723	2728	0.23%	0.029%
78	11.745	3229	3236	3245	rBV3	3061	4359	0.37%	0.047%
79	11.812	3245	3257	3277	rBV	518254	853351	72.64%	9.153%
80	11.970	3304	3306	3309	rBV3	482	254	0.02%	0.003%
81	12.063	3331	3335	3337	rBV2	303	277	0.02%	0.003%
82	12.195	3362	3376	3397	rBV	513603	858431	73.07%	9.208%
83	12.356	3422	3426	3428	rVB3	429	257	0.02%	0.003%
84	12.500	3466	3471	3474	rBV3	368	329	0.03%	0.004%
85	12.623	3507	3509	3511	rBV2	347	185	0.02%	0.002%
86	12.658	3517	3520	3523	rBV2	414	256	0.02%	0.003%
87	12.700	3528	3533	3534	rBV2	333	330	0.03%	0.004%
88	12.783	3557	3559	3565	rVB2	431	317	0.03%	0.003%
89	12.812	3565	3568	3572	rVB	449	305	0.03%	0.003%
90	12.841	3572	3577	3586	rBV3	357	678	0.06%	0.007%
91	12.880	3587	3589	3592	rBV	286	186	0.02%	0.002%
92	12.899	3593	3595	3601	rVB2	321	166	0.01%	0.002%
93	13.002	3623	3627	3633	rBV3	326	390	0.03%	0.004%
94	13.066	3640	3647	3653	rBV3	520	706	0.06%	0.008%
95	13.224	3690	3696	3705	rVB4	2311	3000	0.26%	0.032%
96	13.500	3778	3782	3787	rBV3	276	349	0.03%	0.004%
97	13.844	3881	3889	3904	rVB4	8678	13346	1.14%	0.143%
98	14.092	3957	3966	3979	rBV2	10969	17783	1.51%	0.191%
99	14.333	4032	4041	4053	rBV3	7532	11791	1.00%	0.126%
100	14.581	4114	4118	4122	rBV3	514	511	0.04%	0.005%




Sum of corrected areas: 9323104

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048187.D
Acq On : 21 Apr 2022 21:19
Operator : SY/MD
Sample : VU0421WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

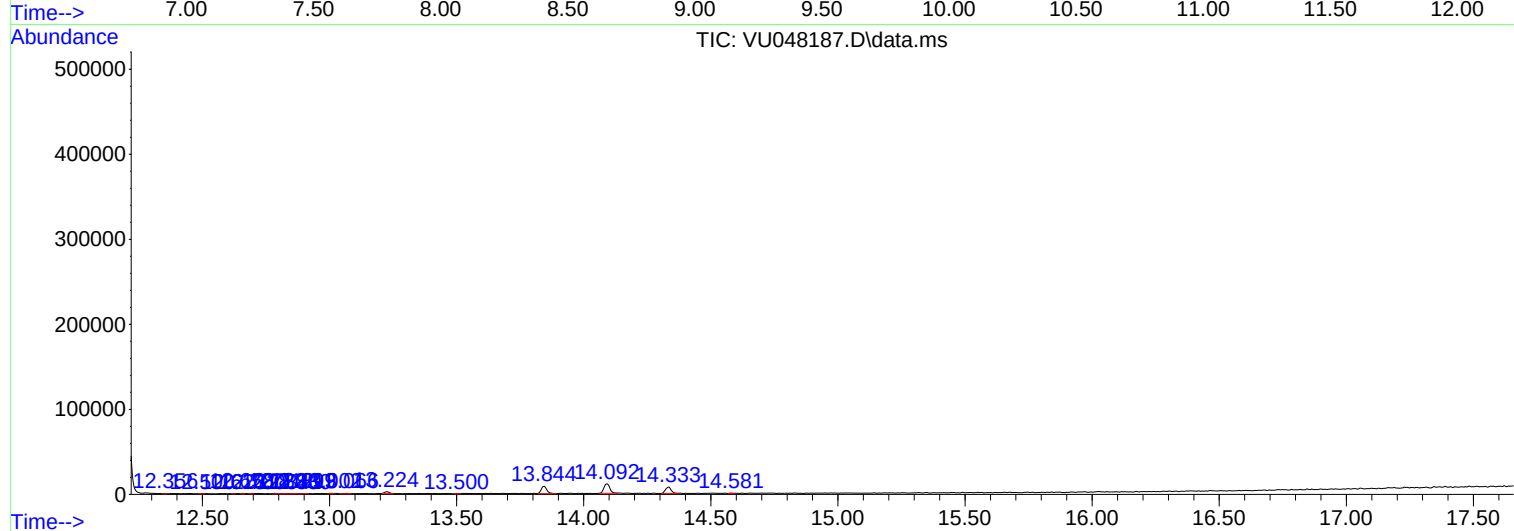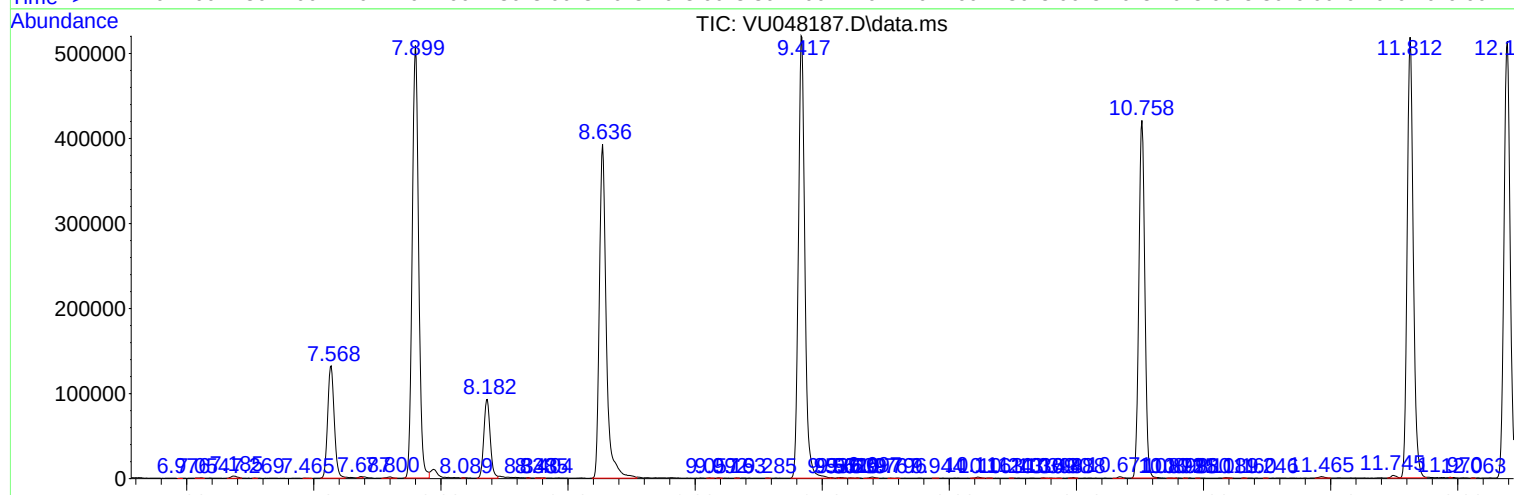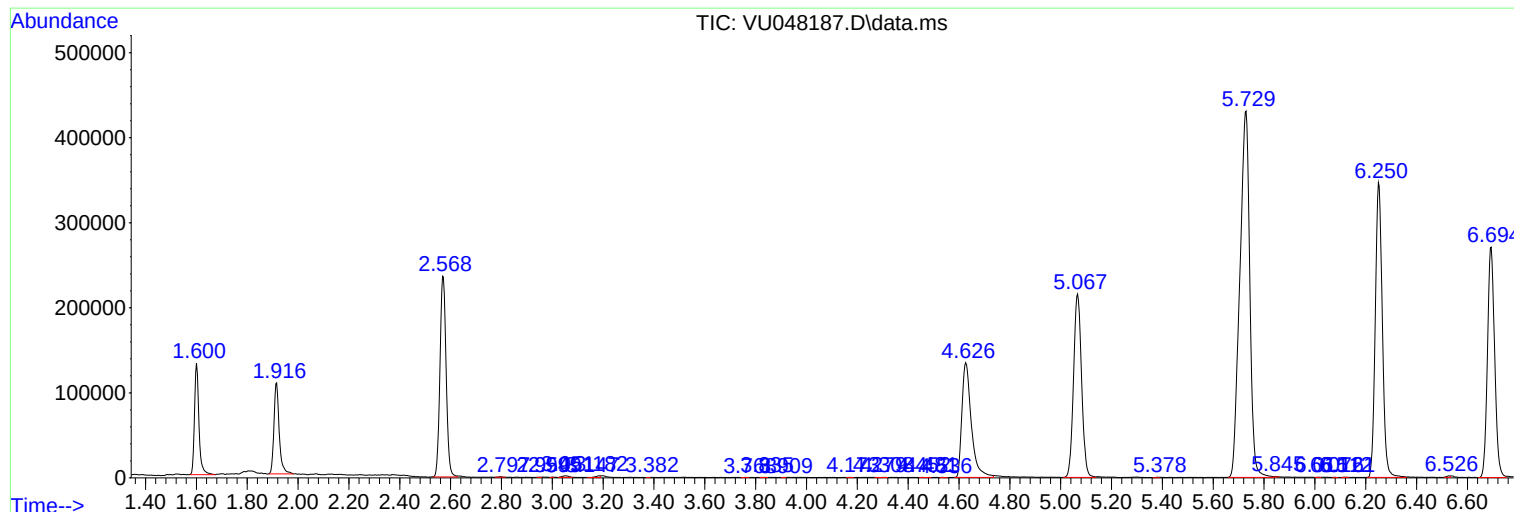

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048187.D
Acq On : 21 Apr 2022 21:19
Operator : SY/MD
Sample : VU0421WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048187.D
Acq On : 21 Apr 2022 21:19
Operator : SY/MD
Sample : VU0421WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------