

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048191.D
 Acq On : 21 Apr 2022 22:54
 Operator : SY/MD
 Sample : N2485-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.360	3	6	31	rVB2	17093	22438	2.08%	0.214%
2	1.491	42	47	51	rBV3	3810	4170	0.39%	0.040%
3	1.601	72	81	93	rBV	132864	165152	15.32%	1.577%
4	1.913	171	178	197	rVB	99994	139947	12.98%	1.336%
5	2.469	349	351	359	rVB4	1014	795	0.07%	0.008%
6	2.569	367	382	398	rBV	216379	361202	33.51%	3.448%
7	2.704	423	424	429	rVB3	358	221	0.02%	0.002%
8	2.732	429	433	435	rBV	379	304	0.03%	0.003%
9	2.768	435	444	450	rBV2	4946	9311	0.86%	0.089%
10	2.845	464	468	472	rVB3	464	366	0.03%	0.003%
11	2.890	478	482	485	rBV3	490	364	0.03%	0.003%
12	2.977	505	509	510	rBV3	558	338	0.03%	0.003%
13	3.051	527	532	536	rBV6	975	1023	0.09%	0.010%
14	3.179	568	572	574	rBV4	695	562	0.05%	0.005%
15	3.279	600	603	608	rVB2	191	178	0.02%	0.002%
16	3.350	621	625	627	rBV2	1050	895	0.08%	0.009%
17	3.533	679	682	683	rBV2	284	184	0.02%	0.002%
18	3.700	724	734	744	rVB5	1602	2845	0.26%	0.027%
19	3.916	799	801	806	rVB2	252	189	0.02%	0.002%
20	4.147	863	873	880	rBV2	301	655	0.06%	0.006%
21	4.183	880	884	890	rBV2	265	358	0.03%	0.003%
22	4.546	993	997	1006	rVB2	266	444	0.04%	0.004%
23	4.626	1006	1022	1054	rBV	119474	300710	27.90%	2.871%
24	4.941	1116	1120	1121	rBV2	244	185	0.02%	0.002%
25	4.996	1132	1137	1142	rBV2	331	467	0.04%	0.004%
26	5.064	1142	1158	1179	rVV	196638	437863	40.63%	4.180%
27	5.205	1198	1202	1208	rVB3	481	644	0.06%	0.006%
28	5.289	1222	1228	1229	rBV	497	469	0.04%	0.004%
29	5.408	1262	1265	1268	rVV	234	189	0.02%	0.002%
30	5.523	1293	1301	1304	rBV	233	271	0.03%	0.003%
31	5.588	1316	1321	1324	rVB	328	219	0.02%	0.002%
32	5.726	1343	1364	1398	rBV2	391025	1077786	100.00%	10.289%
33	6.115	1479	1485	1487	rBV2	317	344	0.03%	0.003%
34	6.250	1513	1527	1549	rBV	362982	687192	63.76%	6.560%
35	6.530	1607	1614	1625	rBV5	1737	3167	0.29%	0.030%
36	6.626	1639	1644	1647	rBV2	304	239	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048191.D
 Acq On : 21 Apr 2022 22:54
 Operator : SY/MD
 Sample : N2485-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.691	1650	1664	1692	rBV	249763	493322	45.77%	4.709%
38	6.800	1696	1698	1700	rBV3	441	259	0.02%	0.002%
39	6.864	1714	1718	1725	rBV3	256	277	0.03%	0.003%
40	7.044	1770	1774	1776	rBV2	353	287	0.03%	0.003%
41	7.112	1791	1795	1800	rBV3	232	222	0.02%	0.002%
42	7.186	1810	1818	1834	rVB3	2573	4677	0.43%	0.045%
43	7.449	1896	1900	1903	rBV	201	195	0.02%	0.002%
44	7.565	1924	1936	1963	rBV	121303	215795	20.02%	2.060%
45	7.691	1968	1975	1983	rBV3	1284	2206	0.20%	0.021%
46	7.803	2005	2010	2015	rVB2	474	527	0.05%	0.005%
47	7.845	2016	2023	2024	rBV3	230	198	0.02%	0.002%
48	7.899	2025	2040	2057	rBV	461787	805584	74.74%	7.690%
49	8.179	2116	2127	2143	rBV	85105	146490	13.59%	1.398%
50	8.337	2174	2176	2179	rVB2	342	193	0.02%	0.002%
51	8.430	2201	2205	2207	rBV	285	209	0.02%	0.002%
52	8.636	2255	2269	2307	rBV	353769	668207	62.00%	6.379%
53	8.928	2355	2360	2361	rVV2	279	201	0.02%	0.002%
54	8.983	2371	2377	2379	rVB3	248	221	0.02%	0.002%
55	9.063	2396	2402	2404	rBV	329	270	0.03%	0.003%
56	9.163	2428	2433	2438	rBV2	292	306	0.03%	0.003%
57	9.301	2474	2476	2480	rBV2	223	184	0.02%	0.002%
58	9.417	2496	2512	2517	rBV	562091	936246	86.87%	8.938%
59	9.600	2566	2569	2575	rVB4	792	648	0.06%	0.006%
60	9.661	2586	2588	2592	rBV2	320	256	0.02%	0.002%
61	9.687	2592	2596	2597	rBV	814	470	0.04%	0.004%
62	10.105	2724	2726	2731	rVB	403	232	0.02%	0.002%
63	10.182	2747	2750	2753	rBV	277	181	0.02%	0.002%
64	10.369	2801	2808	2813	rBV2	271	362	0.03%	0.003%
65	10.417	2820	2823	2826	rBV2	303	212	0.02%	0.002%
66	10.555	2864	2866	2872	rVB2	325	297	0.03%	0.003%
67	10.587	2872	2876	2880	rBV2	262	256	0.02%	0.002%
68	10.610	2880	2883	2886	rBV2	351	260	0.02%	0.002%
69	10.674	2895	2903	2913	rVB6	1166	1583	0.15%	0.015%
70	10.758	2915	2929	2949	rBV	394008	631934	58.63%	6.033%
71	10.832	2949	2952	2957	rVB2	410	338	0.03%	0.003%
72	10.864	2958	2962	2963	rBV	261	184	0.02%	0.002%
73	10.890	2964	2970	2979	rVB5	1109	1756	0.16%	0.017%
74	10.989	2991	3001	3013	rVB	5514	7895	0.73%	0.075%
75	11.047	3015	3019	3020	rBV3	484	373	0.03%	0.004%
76	11.102	3029	3036	3050	rVB	1879	2884	0.27%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048191.D
 Acq On : 21 Apr 2022 22:54
 Operator : SY/MD
 Sample : N2485-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.353	3112	3114	3119	rVB2	319	232	0.02%	0.002%
78	11.459	3140	3147	3149	rBV4	938	973	0.09%	0.009%
79	11.578	3182	3184	3191	rVB3	267	294	0.03%	0.003%
80	11.687	3215	3218	3221	rVB2	280	202	0.02%	0.002%
81	11.745	3221	3236	3247	rBV	424178	678969	63.00%	6.482%
82	11.816	3247	3258	3259	rBV	657245	790058	73.30%	7.542%
83	11.973	3303	3307	3312	rVB4	1282	1308	0.12%	0.012%
84	12.070	3327	3337	3345	rBV5	3082	5184	0.48%	0.049%
85	12.195	3362	3376	3398	rVV2	545921	1067638	99.06%	10.192%
86	12.333	3417	3419	3426	rVB3	417	346	0.03%	0.003%
87	12.687	3524	3529	3539	rVB4	648	969	0.09%	0.009%
88	12.742	3543	3546	3548	rBV2	412	260	0.02%	0.002%
89	12.857	3580	3582	3588	rBV2	300	192	0.02%	0.002%
90	12.973	3609	3618	3625	rBV4	2584	3589	0.33%	0.034%
91	13.157	3663	3675	3686	rVB6	6438	15393	1.43%	0.147%
92	13.221	3686	3695	3707	rVB	18127	27179	2.52%	0.259%
93	13.282	3711	3714	3718	rBV2	404	255	0.02%	0.002%
94	13.542	3793	3795	3799	rVB2	350	231	0.02%	0.002%
95	13.565	3799	3802	3804	rBV2	344	301	0.03%	0.003%
96	13.841	3875	3888	3904	rBV	401210	629110	58.37%	6.006%
97	14.089	3960	3965	3966	rBV3	1094	866	0.08%	0.008%
98	14.330	4030	4040	4054	rVB	54942	88084	8.17%	0.841%
99	15.420	4372	4379	4389	rVB5	3715	5898	0.55%	0.056%
100	16.002	4553	4560	4570	rVB5	6533	10014	0.93%	0.096%




Sum of corrected areas: 10475428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048191.D
Acq On : 21 Apr 2022 22:54
Operator : SY/MD
Sample : N2485-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

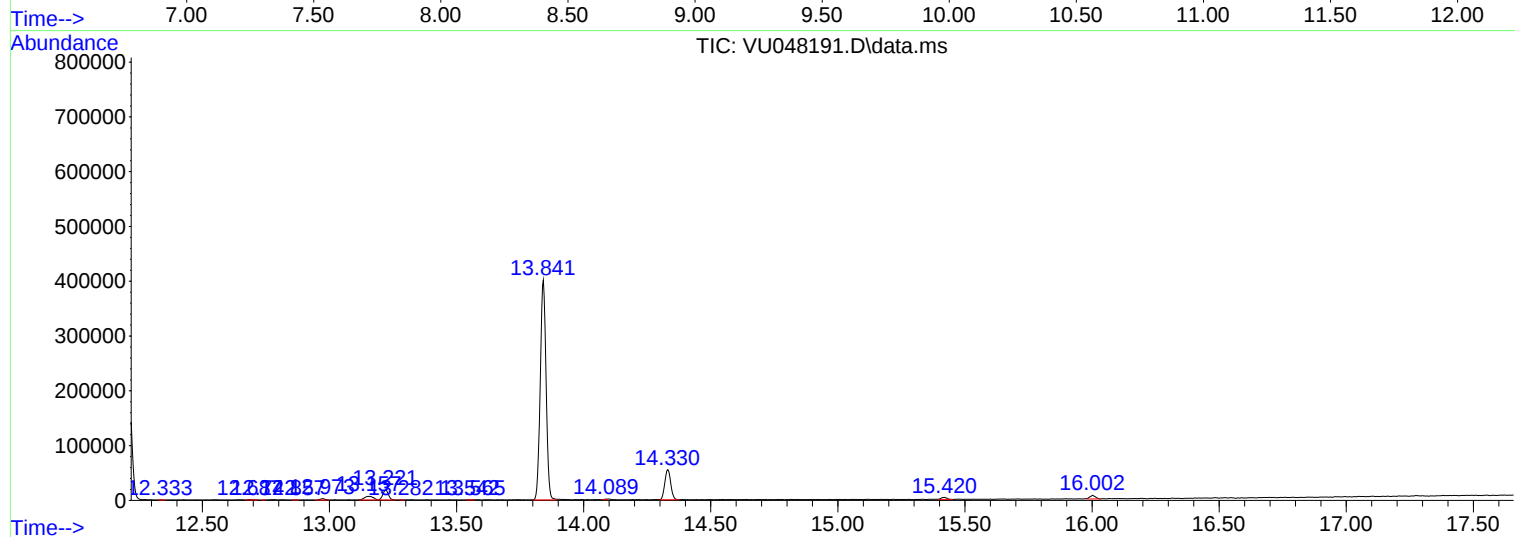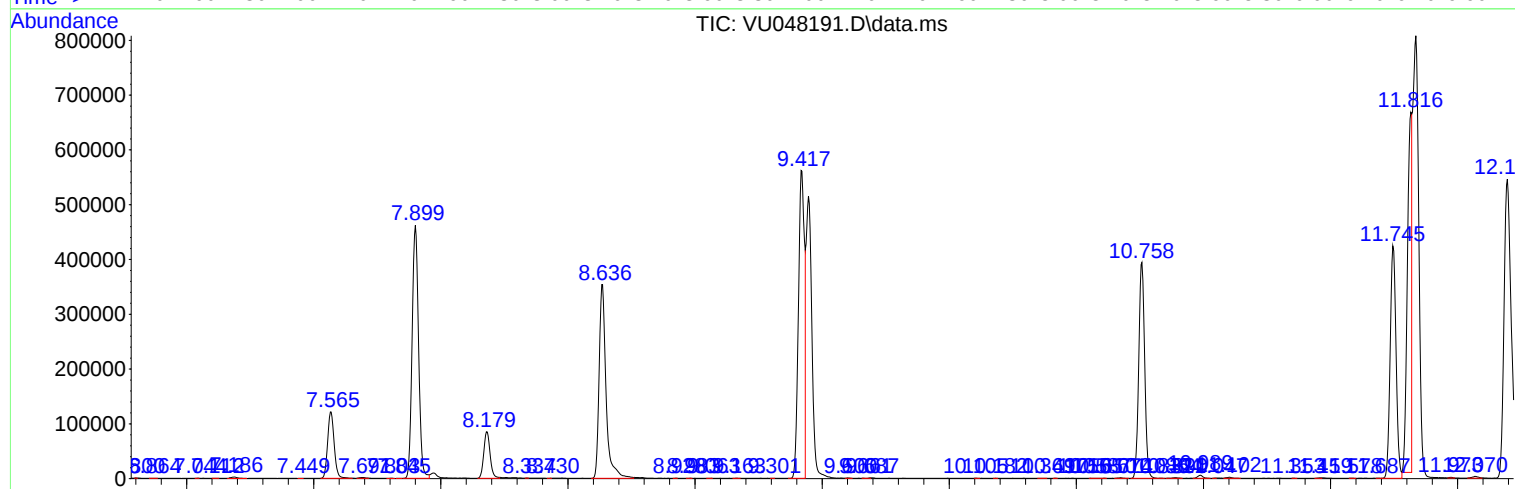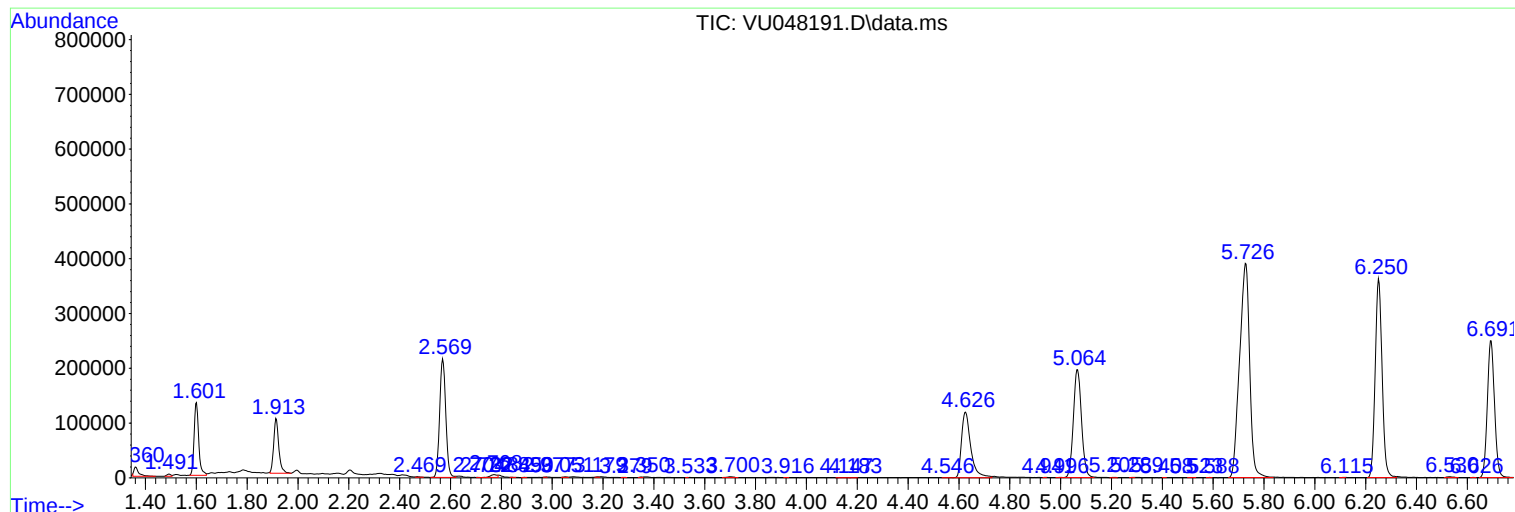

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048191.D
Acq On : 21 Apr 2022 22:54
Operator : SY/MD
Sample : N2485-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048191.D
Acq On : 21 Apr 2022 22:54
Operator : SY/MD
Sample : N2485-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------