

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048197.D
 Acq On : 22 Apr 2022 01:50
 Operator : SY/MD
 Sample : N2488-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rBV	119449	143765	0.76%	0.244%
2	1.912	170	178	200	rVB	97493	142712	0.75%	0.242%
3	2.568	370	382	397	rBV	225847	367695	1.94%	0.624%
4	2.851	466	470	475	rVB3	273	234	0.00%	0.000%
5	2.957	500	503	508	rVB2	390	420	0.00%	0.001%
6	3.047	524	531	539	rVB4	723	1317	0.01%	0.002%
7	3.189	561	575	591	rVB	2961	6070	0.03%	0.010%
8	3.308	607	612	614	rBV	198	203	0.00%	0.000%
9	3.362	621	629	630	rBV2	563	578	0.00%	0.001%
10	3.446	648	655	658	rBV2	301	464	0.00%	0.001%
11	3.999	819	827	830	rBV2	258	324	0.00%	0.001%
12	4.073	844	850	855	rVB2	186	226	0.00%	0.000%
13	4.288	913	917	921	rVV2	202	198	0.00%	0.000%
14	4.372	935	943	948	rBV	187	289	0.00%	0.000%
15	4.620	1008	1020	1064	rBV	119824	296302	1.56%	0.503%
16	4.812	1077	1080	1083	rBV2	330	220	0.00%	0.000%
17	4.964	1125	1127	1133	rBV2	315	229	0.00%	0.000%
18	5.066	1141	1159	1189	rBV3	220930	596662	3.15%	1.012%
19	5.221	1204	1207	1214	rVB3	354	312	0.00%	0.001%
20	5.295	1224	1230	1234	rBV2	454	547	0.00%	0.001%
21	5.382	1253	1257	1266	rVB3	409	526	0.00%	0.001%
22	5.488	1284	1290	1291	rBV	213	208	0.00%	0.000%
23	5.530	1291	1303	1314	rVB2	5736	11592	0.06%	0.020%
24	5.597	1321	1324	1332	rVB3	260	275	0.00%	0.000%
25	5.636	1332	1336	1341	rBV2	319	298	0.00%	0.001%
26	5.729	1342	1365	1369	rBV2	410399	999774	5.27%	1.696%
27	5.777	1370	1380	1414	rVB	2370033	4785579	25.24%	8.119%
28	6.250	1513	1527	1550	rBV	379514	722647	3.81%	1.226%
29	6.462	1588	1593	1596	rVB4	258	222	0.00%	0.000%
30	6.533	1606	1615	1616	rBV4	1871	2388	0.01%	0.004%
31	6.693	1650	1665	1689	rBV	260286	508067	2.68%	0.862%
32	7.105	1789	1793	1796	rVV4	202	203	0.00%	0.000%
33	7.185	1809	1818	1830	rBV3	2610	4399	0.02%	0.007%
34	7.349	1863	1869	1870	rVV2	223	198	0.00%	0.000%
35	7.568	1924	1937	1958	rBV	124418	220695	1.16%	0.374%
36	7.687	1968	1974	1984	rVB3	1447	2485	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048197.D
 Acq On : 22 Apr 2022 01:50
 Operator : SY/MD
 Sample : N2488-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.732	1984	1988	1991	rVB3	349	257	0.00%	0.000%
38	7.899	2025	2040	2056	rBV	487272	843529	4.45%	1.431%
39	7.970	2056	2062	2074	rVB	8596	15453	0.08%	0.026%
40	8.182	2116	2128	2147	rBV	86565	149950	0.79%	0.254%
41	8.279	2155	2158	2160	rBV2	503	347	0.00%	0.001%
42	8.481	2208	2221	2228	rBV4	720	1524	0.01%	0.003%
43	8.555	2237	2244	2250	rBV5	1479	1749	0.01%	0.003%
44	8.635	2255	2269	2303	rBV	347922	656738	3.46%	1.114%
45	8.925	2354	2359	2364	rBV3	465	466	0.00%	0.001%
46	8.957	2366	2369	2372	rVV	261	197	0.00%	0.000%
47	8.989	2375	2379	2384	rVB	247	231	0.00%	0.000%
48	9.057	2394	2400	2403	rBV2	242	259	0.00%	0.000%
49	9.189	2438	2441	2445	rVV3	212	197	0.00%	0.000%
50	9.362	2488	2495	2498	rBV3	210	212	0.00%	0.000%
51	9.449	2498	2522	2564	rBV	5564725	10047410	53.00%	17.045%
52	9.690	2595	2597	2609	rVB4	1269	1790	0.01%	0.003%
53	9.745	2609	2614	2616	rBV2	359	351	0.00%	0.001%
54	9.819	2634	2637	2641	rVB2	335	250	0.00%	0.000%
55	9.899	2659	2662	2665	rVB	489	273	0.00%	0.000%
56	10.005	2691	2695	2699	rVB	266	204	0.00%	0.000%
57	10.147	2735	2739	2741	rVB	475	338	0.00%	0.001%
58	10.214	2758	2760	2764	rVV	398	268	0.00%	0.000%
59	10.253	2767	2772	2775	rVV2	409	403	0.00%	0.001%
60	10.288	2779	2783	2790	rVV2	382	541	0.00%	0.001%
61	10.336	2796	2798	2804	rVV	326	287	0.00%	0.000%
62	10.365	2804	2807	2817	rVV2	240	397	0.00%	0.001%
63	10.671	2896	2902	2912	rVB4	1344	1796	0.01%	0.003%
64	10.758	2916	2929	2948	rVV	408518	659299	3.48%	1.118%
65	10.893	2965	2971	2978	rVB5	1092	1540	0.01%	0.003%
66	10.989	2995	3001	3009	rVB3	1317	1690	0.01%	0.003%
67	11.066	3019	3025	3028	rBV2	247	300	0.00%	0.001%
68	11.105	3033	3037	3039	rBV3	481	349	0.00%	0.001%
69	11.346	3109	3112	3117	rBV2	226	257	0.00%	0.000%
70	11.375	3117	3121	3127	rVB3	258	233	0.00%	0.000%
71	11.471	3141	3151	3156	rBV5	1098	1694	0.01%	0.003%
72	11.577	3180	3184	3187	rVB3	379	308	0.00%	0.001%
73	11.664	3205	3211	3214	rBV2	233	251	0.00%	0.000%
74	11.696	3215	3221	3223	rBV3	373	399	0.00%	0.001%
75	11.748	3223	3237	3248	rBV	1514551	2377757	12.54%	4.034%
76	11.838	3248	3265	3287	rVB	7708225	12829580	67.68%	21.765%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048197.D
 Acq On : 22 Apr 2022 01:50
 Operator : SY/MD
 Sample : N2488-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	12.073	3330	3338	3344	rVV4	2596	4119	0.02%	0.007%
78	12.214	3363	3382	3402	rBV	11640977	18957577	100.00%	32.161%
79	12.584	3495	3497	3503	rVB2	488	310	0.00%	0.001%
80	12.716	3534	3538	3546	rVB3	675	818	0.00%	0.001%
81	12.783	3546	3559	3562	rBV6	756	1262	0.01%	0.002%
82	12.889	3589	3592	3593	rBV2	542	283	0.00%	0.000%
83	12.973	3609	3618	3627	rBV3	7942	12467	0.07%	0.021%
84	13.143	3668	3671	3673	rBV3	518	407	0.00%	0.001%
85	13.208	3681	3691	3704	rBV2	33005	56503	0.30%	0.096%
86	13.330	3718	3729	3737	rBV4	6257	10018	0.05%	0.017%
87	13.475	3771	3774	3777	rBV	326	202	0.00%	0.000%
88	13.555	3796	3799	3804	rBV3	377	387	0.00%	0.001%
89	13.597	3809	3812	3814	rBV3	335	216	0.00%	0.000%
90	13.655	3828	3830	3839	rVV4	526	693	0.00%	0.001%
91	13.841	3875	3888	3912	rBV	1540098	2372908	12.52%	4.026%
92	14.330	4027	4040	4062	rBV	675793	1075727	5.67%	1.825%
93	14.529	4100	4102	4106	rBV2	340	218	0.00%	0.000%
94	14.680	4147	4149	4151	rBV2	408	200	0.00%	0.000%
95	14.735	4159	4166	4173	rBV4	2707	3861	0.02%	0.007%
96	14.857	4201	4204	4208	rBV2	632	468	0.00%	0.001%
97	14.880	4209	4211	4214	rVV2	534	301	0.00%	0.001%
98	14.934	4225	4228	4234	rBV4	506	594	0.00%	0.001%
99	15.417	4370	4378	4386	rVB2	6538	9295	0.05%	0.016%
100	16.002	4552	4560	4572	rVB3	12973	20216	0.11%	0.034%




Sum of corrected areas: 58946447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048197.D
Acq On : 22 Apr 2022 01:50
Operator : SY/MD
Sample : N2488-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

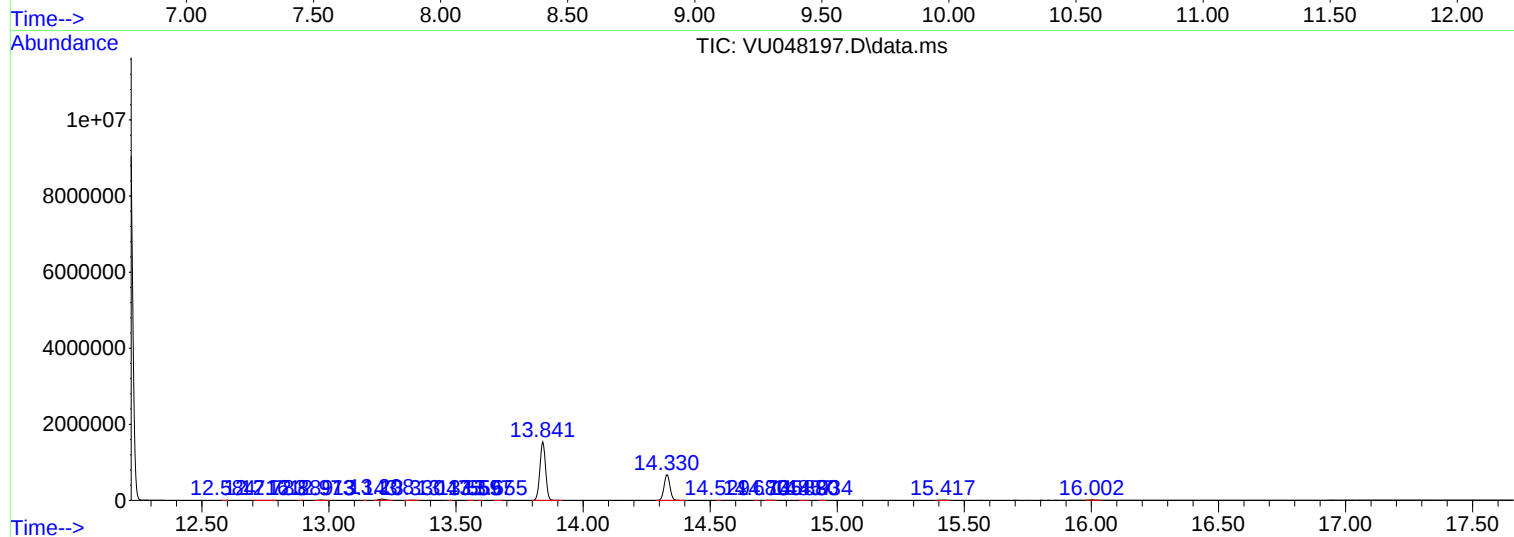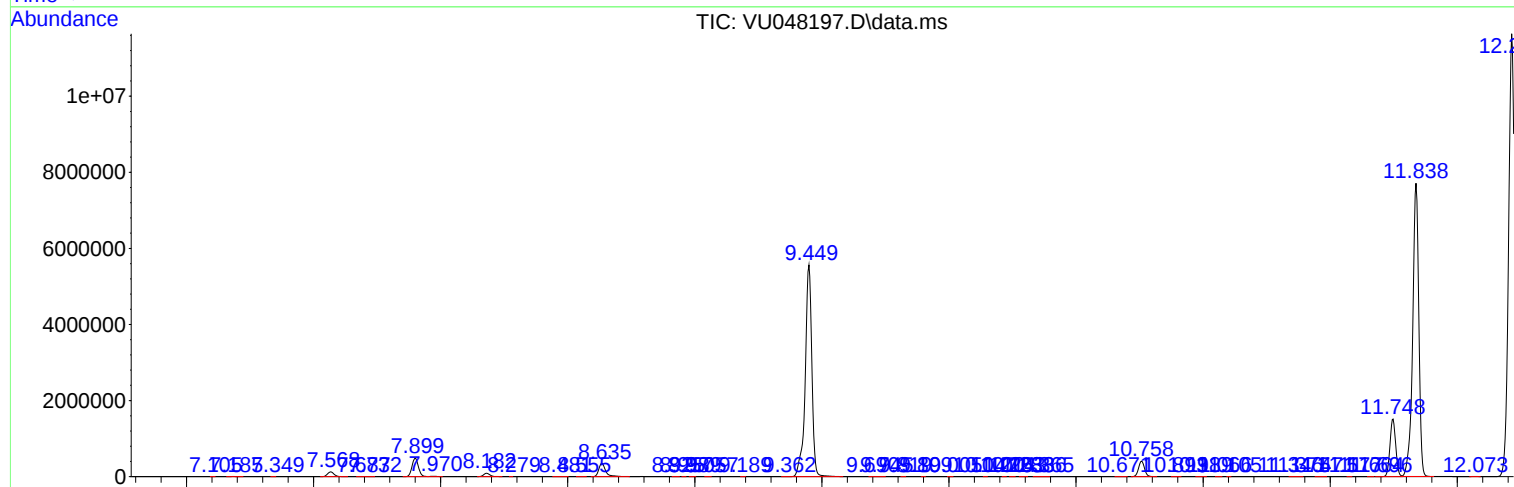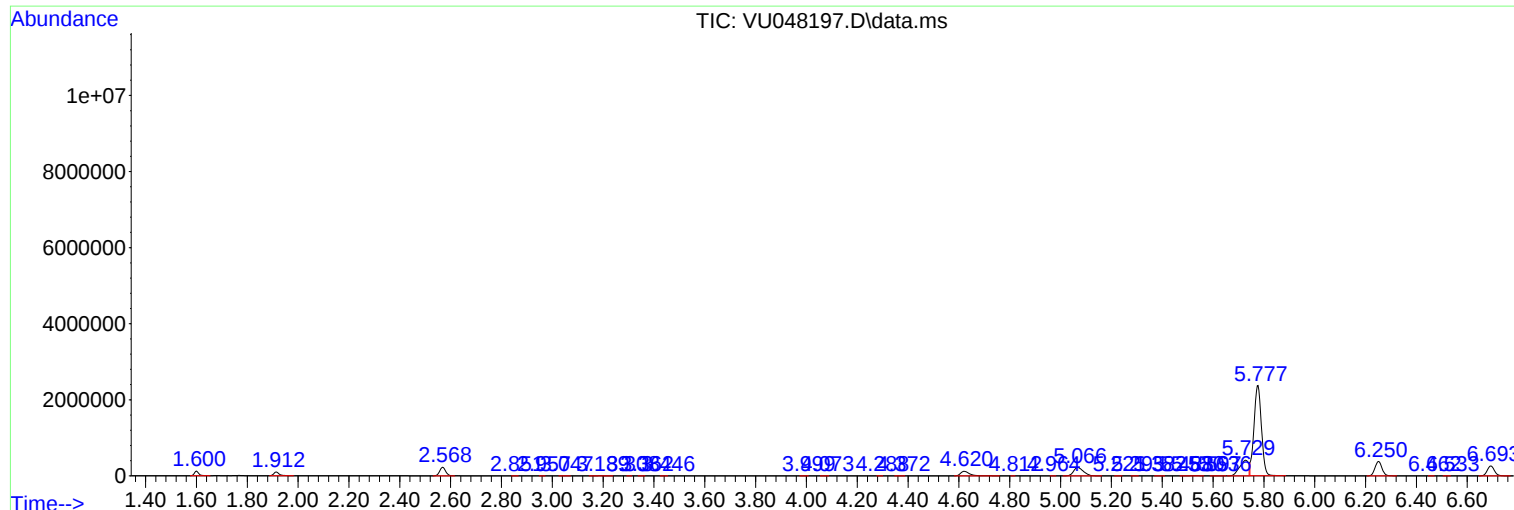

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048197.D
Acq On : 22 Apr 2022 01:50
Operator : SY/MD
Sample : N2488-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048197.D
Acq On : 22 Apr 2022 01:50
Operator : SY/MD
Sample : N2488-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------