

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048199.D
 Acq On : 22 Apr 2022 02:51
 Operator : SY/MD
 Sample : N2488-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rBV	117661	144233	13.05%	1.497%
2	1.913	170	178	196	rBV	97996	135131	12.23%	1.403%
3	2.568	370	382	398	rBV	218885	361244	32.69%	3.750%
4	2.781	439	448	450	rBV3	1117	1255	0.11%	0.013%
5	2.887	478	481	485	rBV3	319	312	0.03%	0.003%
6	2.964	500	505	507	rBV2	613	604	0.05%	0.006%
7	3.048	526	531	534	rBV3	785	913	0.08%	0.009%
8	3.115	545	552	555	rBV2	186	254	0.02%	0.003%
9	3.189	560	575	591	rBV2	7420	16870	1.53%	0.175%
10	3.247	591	593	598	rVB	394	250	0.02%	0.003%
11	3.285	598	605	609	rBV2	307	389	0.04%	0.004%
12	3.440	650	653	662	rBV3	283	354	0.03%	0.004%
13	3.588	695	699	704	rVB3	230	206	0.02%	0.002%
14	3.736	740	745	749	rBV2	238	320	0.03%	0.003%
15	3.986	818	823	828	rVB	273	295	0.03%	0.003%
16	4.575	999	1006	1009	rBV	194	242	0.02%	0.003%
17	4.626	1009	1022	1053	rBV	128364	332838	30.12%	3.455%
18	4.855	1089	1093	1098	rVB4	503	467	0.04%	0.005%
19	5.067	1142	1159	1184	rBV	200669	440331	39.84%	4.570%
20	5.295	1223	1230	1236	rVB2	614	837	0.08%	0.009%
21	5.520	1293	1300	1306	rBV3	494	495	0.04%	0.005%
22	5.726	1342	1364	1394	rBV2	404524	1105156	100.00%	11.471%
23	5.977	1437	1442	1446	rBV2	158	219	0.02%	0.002%
24	6.018	1450	1455	1458	rBV3	247	255	0.02%	0.003%
25	6.038	1458	1461	1465	rVB3	519	331	0.03%	0.003%
26	6.121	1485	1487	1494	rVB3	403	276	0.02%	0.003%
27	6.250	1513	1527	1545	rBV	357458	689835	62.42%	7.160%
28	6.478	1595	1598	1602	rBV2	388	317	0.03%	0.003%
29	6.530	1606	1614	1615	rBV4	2106	2105	0.19%	0.022%
30	6.604	1633	1637	1639	rVB3	412	318	0.03%	0.003%
31	6.694	1651	1665	1691	rBV	254865	502066	45.43%	5.211%
32	6.797	1694	1697	1700	rVV3	360	226	0.02%	0.002%
33	6.851	1709	1714	1718	rBV	308	220	0.02%	0.002%
34	7.054	1772	1777	1778	rBV2	284	225	0.02%	0.002%
35	7.160	1806	1810	1811	rBV2	362	225	0.02%	0.002%
36	7.186	1811	1818	1832	rVB3	2550	4389	0.40%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048199.D
 Acq On : 22 Apr 2022 02:51
 Operator : SY/MD
 Sample : N2488-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.327	1860	1862	1869	rVB2	315	238	0.02%	0.002%
38	7.359	1869	1872	1876	rBV3	237	216	0.02%	0.002%
39	7.488	1903	1912	1914	rBV	329	401	0.04%	0.004%
40	7.568	1924	1937	1958	rBV	122904	221002	20.00%	2.294%
41	7.694	1969	1976	1989	rVB3	1655	3150	0.29%	0.033%
42	7.899	2027	2040	2056	rBV	474672	828685	74.98%	8.601%
43	8.079	2094	2096	2099	rVB	375	213	0.02%	0.002%
44	8.096	2099	2101	2105	rVB3	393	282	0.03%	0.003%
45	8.182	2116	2128	2145	rBV	87520	150579	13.63%	1.563%
46	8.385	2188	2191	2194	rBV2	417	314	0.03%	0.003%
47	8.559	2242	2245	2250	rVB3	609	469	0.04%	0.005%
48	8.636	2256	2269	2299	rBV	354337	667637	60.41%	6.930%
49	8.780	2310	2314	2328	rVB7	2271	4437	0.40%	0.046%
50	8.845	2328	2334	2337	rBV3	474	452	0.04%	0.005%
51	9.051	2395	2398	2402	rBV2	318	225	0.02%	0.002%
52	9.073	2402	2405	2411	rVB	303	226	0.02%	0.002%
53	9.141	2422	2426	2429	rVV2	364	241	0.02%	0.003%
54	9.163	2429	2433	2438	rVV3	412	435	0.04%	0.005%
55	9.202	2442	2445	2450	rVB	313	207	0.02%	0.002%
56	9.420	2498	2513	2547	rVV	539037	983983	89.04%	10.213%
57	9.571	2558	2560	2562	rVV2	413	276	0.02%	0.003%
58	9.607	2566	2571	2574	rBV2	466	419	0.04%	0.004%
59	9.690	2590	2597	2598	rBV3	480	413	0.04%	0.004%
60	9.751	2613	2616	2622	rVB2	243	227	0.02%	0.002%
61	9.845	2641	2645	2651	rVB	272	232	0.02%	0.002%
62	9.877	2651	2655	2659	rVB2	293	311	0.03%	0.003%
63	9.903	2659	2663	2667	rBV2	359	415	0.04%	0.004%
64	10.118	2725	2730	2734	rBV3	275	273	0.02%	0.003%
65	10.449	2830	2833	2835	rBV3	330	208	0.02%	0.002%
66	10.671	2894	2902	2911	rVB6	1305	2119	0.19%	0.022%
67	10.758	2913	2929	2947	rBV	398777	643394	58.22%	6.678%
68	10.848	2952	2957	2964	rBV3	385	594	0.05%	0.006%
69	10.896	2969	2972	2976	rVV3	295	247	0.02%	0.003%
70	11.163	3052	3055	3058	rBV	346	215	0.02%	0.002%
71	11.333	3103	3108	3112	rBV2	345	342	0.03%	0.004%
72	11.462	3140	3148	3152	rBV3	1158	1463	0.13%	0.015%
73	11.504	3158	3161	3167	rBV2	307	241	0.02%	0.003%
74	11.697	3218	3221	3223	rBV2	367	274	0.02%	0.003%
75	11.748	3226	3237	3245	rVV2	19535	30870	2.79%	0.320%
76	11.812	3245	3257	3282	rVB2	546967	1038148	93.94%	10.776%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048199.D
 Acq On : 22 Apr 2022 02:51
 Operator : SY/MD
 Sample : N2488-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	12.015	3318	3320	3323	rBV2	314	211	0.02%	0.002%
78	12.066	3331	3336	3345	rBV7	2717	4122	0.37%	0.043%
79	12.195	3362	3376	3401	rBV2	538720	1090961	98.72%	11.324%
80	12.330	3414	3418	3420	rBV2	388	302	0.03%	0.003%
81	12.420	3442	3446	3447	rBV	312	232	0.02%	0.002%
82	12.462	3456	3459	3463	rBV2	333	357	0.03%	0.004%
83	12.626	3507	3510	3514	rBV3	379	232	0.02%	0.002%
84	12.697	3529	3532	3540	rBV3	458	509	0.05%	0.005%
85	12.960	3611	3614	3617	rVB	301	210	0.02%	0.002%
86	13.214	3686	3693	3694	rBV2	1578	1336	0.12%	0.014%
87	13.256	3704	3706	3709	rBV	318	248	0.02%	0.003%
88	13.288	3713	3716	3721	rVB2	460	351	0.03%	0.004%
89	13.330	3726	3729	3734	rBV2	475	413	0.04%	0.004%
90	13.536	3790	3793	3797	rBV2	340	272	0.02%	0.003%
91	13.674	3834	3836	3839	rVB3	412	212	0.02%	0.002%
92	13.755	3858	3861	3866	rBV2	400	345	0.03%	0.004%
93	13.796	3871	3874	3877	rVV3	574	543	0.05%	0.006%
94	13.841	3877	3888	3915	rVB	78921	127252	11.51%	1.321%
95	14.330	4030	4040	4055	rVB	42122	66293	6.00%	0.688%
96	14.738	4164	4167	4169	rBV	464	330	0.03%	0.003%
97	15.015	4250	4253	4255	rVB	602	361	0.03%	0.004%
98	15.414	4372	4377	4378	rBV3	1605	1289	0.12%	0.013%
99	15.812	4498	4501	4507	rBV4	728	696	0.06%	0.007%
100	16.005	4554	4561	4573	rVB5	5983	9126	0.83%	0.095%




Sum of corrected areas: 9634279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048199.D
Acq On : 22 Apr 2022 02:51
Operator : SY/MD
Sample : N2488-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

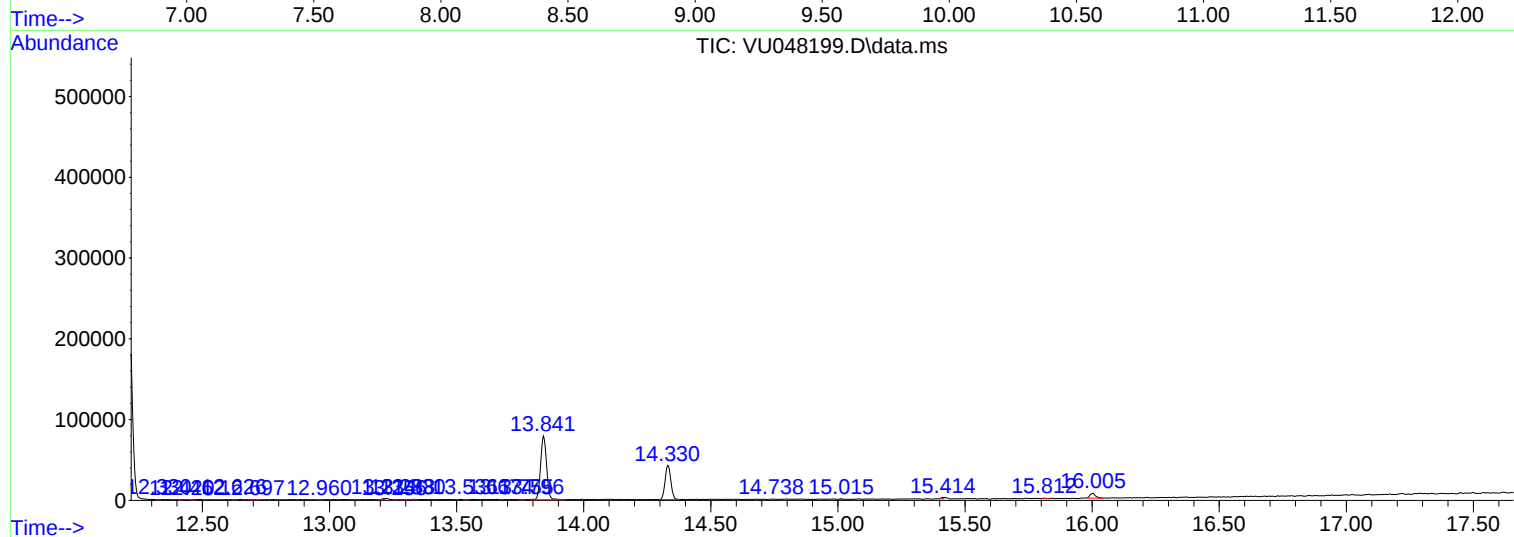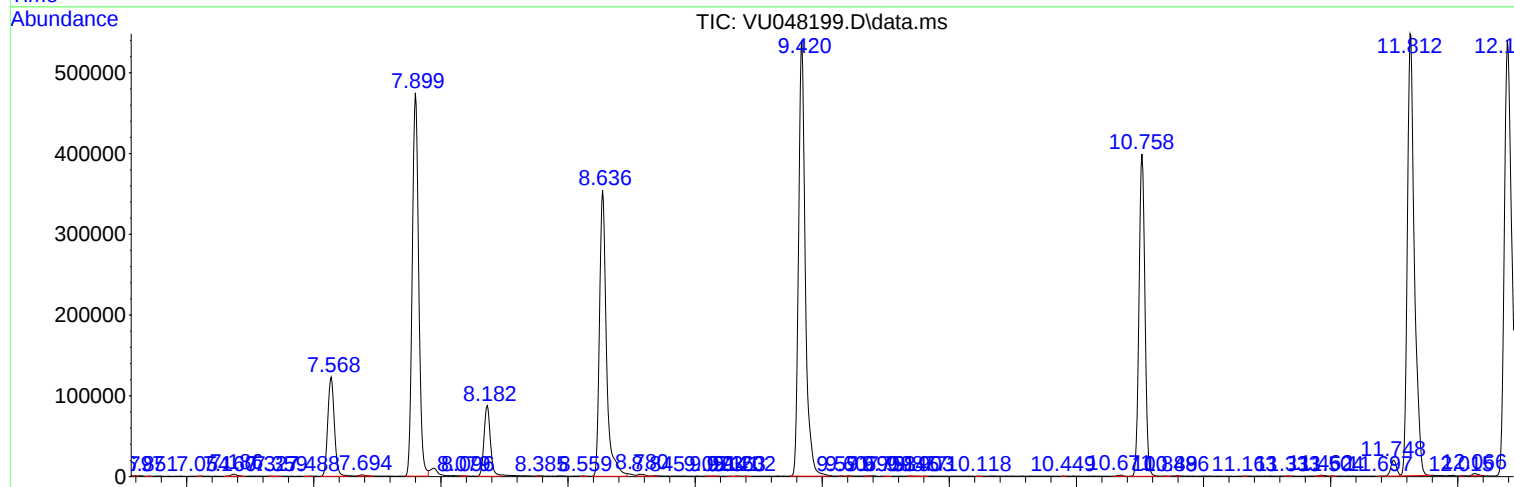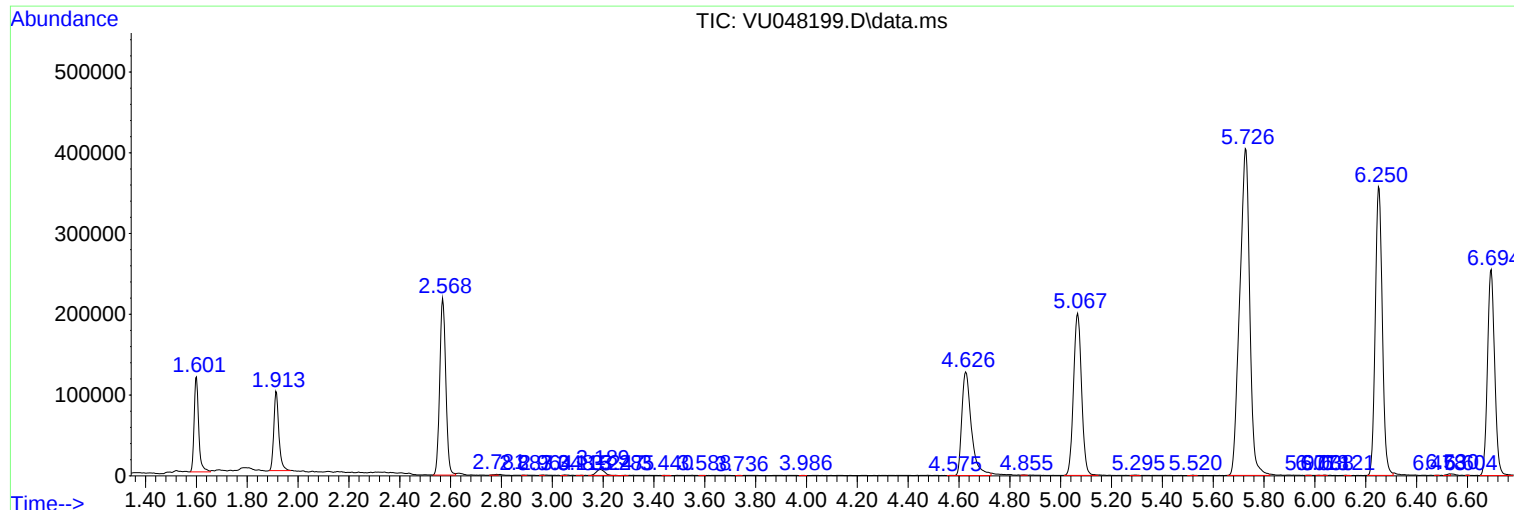

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048199.D
Acq On : 22 Apr 2022 02:51
Operator : SY/MD
Sample : N2488-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048199.D
Acq On : 22 Apr 2022 02:51
Operator : SY/MD
Sample : N2488-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------