

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048200.D
 Acq On : 22 Apr 2022 03:22
 Operator : SY/MD
 Sample : N2488-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rBV	117284	143494	13.22%	1.563%
2	1.913	170	178	199	rVB	98219	139279	12.83%	1.517%
3	2.569	369	382	397	rBV	216880	359292	33.10%	3.913%
4	2.733	431	433	439	rVB2	331	252	0.02%	0.003%
5	2.787	441	450	451	rBV3	1545	1649	0.15%	0.018%
6	2.858	469	472	474	rBV2	364	301	0.03%	0.003%
7	2.964	500	505	508	rBV2	388	392	0.04%	0.004%
8	3.003	513	517	521	rBV3	312	276	0.03%	0.003%
9	3.044	526	530	532	rBV3	586	433	0.04%	0.005%
10	3.189	560	575	589	rBV	12536	29214	2.69%	0.318%
11	3.292	604	607	610	rBV2	296	201	0.02%	0.002%
12	3.343	619	623	627	rBV2	261	174	0.02%	0.002%
13	3.556	686	689	692	rVB2	228	174	0.02%	0.002%
14	3.578	692	696	697	rBV	282	172	0.02%	0.002%
15	3.646	710	717	724	rBV2	226	388	0.04%	0.004%
16	3.755	747	751	757	rBV2	133	200	0.02%	0.002%
17	3.919	799	802	805	rVB2	228	177	0.02%	0.002%
18	3.941	805	809	814	rBV	317	380	0.04%	0.004%
19	4.054	839	844	848	rBV2	146	201	0.02%	0.002%
20	4.337	924	932	936	rBV2	237	372	0.03%	0.004%
21	4.366	938	941	947	rVB2	209	233	0.02%	0.003%
22	4.565	1000	1003	1006	rBV	243	165	0.02%	0.002%
23	4.626	1007	1022	1048	rBV2	133980	349255	32.18%	3.804%
24	5.067	1142	1159	1183	rBV	198007	436952	40.26%	4.759%
25	5.202	1199	1201	1205	rBV3	214	193	0.02%	0.002%
26	5.228	1206	1209	1214	rVB3	540	425	0.04%	0.005%
27	5.298	1224	1231	1238	rVB2	755	1040	0.10%	0.011%
28	5.376	1252	1255	1257	rBV2	285	179	0.02%	0.002%
29	5.584	1317	1320	1324	rBV2	215	161	0.01%	0.002%
30	5.726	1343	1364	1396	rBV2	395832	1085410	100.00%	11.821%
31	6.105	1478	1482	1485	rBV3	315	304	0.03%	0.003%
32	6.250	1513	1527	1558	rBV	367542	701467	64.63%	7.640%
33	6.379	1565	1567	1571	rVB2	353	224	0.02%	0.002%
34	6.485	1597	1600	1603	rBV	337	263	0.02%	0.003%
35	6.533	1607	1615	1617	rBV4	1444	1959	0.18%	0.021%
36	6.694	1650	1665	1695	rBV	253070	498331	45.91%	5.427%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048200.D
 Acq On : 22 Apr 2022 03:22
 Operator : SY/MD
 Sample : N2488-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.912	1729	1733	1738	rVB2	271	229	0.02%	0.002%
38	7.019	1763	1766	1771	rVB3	287	207	0.02%	0.002%
39	7.047	1771	1775	1780	rBV3	338	350	0.03%	0.004%
40	7.186	1809	1818	1829	rVB2	2329	3936	0.36%	0.043%
41	7.244	1829	1836	1840	rVB2	301	322	0.03%	0.004%
42	7.369	1873	1875	1881	rVB	229	163	0.02%	0.002%
43	7.478	1906	1909	1915	rVB3	235	205	0.02%	0.002%
44	7.517	1918	1921	1924	rBV2	285	201	0.02%	0.002%
45	7.568	1924	1937	1961	rBV	120021	214661	19.78%	2.338%
46	7.691	1969	1975	1982	rBV3	1440	1931	0.18%	0.021%
47	7.803	2008	2010	2016	rVB2	291	237	0.02%	0.003%
48	7.835	2016	2020	2022	rBV2	247	201	0.02%	0.002%
49	7.900	2027	2040	2056	rBV	466859	823088	75.83%	8.964%
50	8.128	2109	2111	2115	rBV2	275	189	0.02%	0.002%
51	8.182	2115	2128	2149	rBV	84115	147377	13.58%	1.605%
52	8.636	2257	2269	2305	rBV	349888	666191	61.38%	7.255%
53	9.028	2387	2391	2394	rBV2	232	240	0.02%	0.003%
54	9.160	2428	2432	2439	rVB2	537	557	0.05%	0.006%
55	9.199	2439	2444	2449	rBV	214	232	0.02%	0.003%
56	9.420	2499	2513	2552	rBV	550268	963839	88.80%	10.497%
57	9.571	2556	2560	2563	rVB	338	273	0.03%	0.003%
58	9.690	2595	2597	2605	rVB2	425	331	0.03%	0.004%
59	10.076	2714	2717	2721	rVB2	302	244	0.02%	0.003%
60	10.153	2737	2741	2744	rVB	212	172	0.02%	0.002%
61	10.173	2744	2747	2750	rBV2	207	179	0.02%	0.002%
62	10.353	2798	2803	2806	rVB3	338	283	0.03%	0.003%
63	10.372	2806	2809	2815	rBV2	317	263	0.02%	0.003%
64	10.674	2898	2903	2911	rVB4	922	1158	0.11%	0.013%
65	10.758	2916	2929	2949	rVB	396125	638605	58.84%	6.955%
66	10.835	2949	2953	2957	rVB2	295	246	0.02%	0.003%
67	10.867	2959	2963	2965	rBV	375	302	0.03%	0.003%
68	10.890	2966	2970	2972	rBV	443	373	0.03%	0.004%
69	10.941	2982	2986	2990	rBV2	345	293	0.03%	0.003%
70	11.009	3003	3007	3011	rBV3	380	273	0.03%	0.003%
71	11.231	3073	3076	3079	rBV2	244	188	0.02%	0.002%
72	11.276	3087	3090	3093	rBV	230	197	0.02%	0.002%
73	11.430	3135	3138	3142	rBV	233	193	0.02%	0.002%
74	11.481	3142	3154	3159	rBV5	921	1916	0.18%	0.021%
75	11.568	3178	3181	3183	rBV	327	219	0.02%	0.002%
76	11.616	3192	3196	3200	rBV2	176	192	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048200.D
 Acq On : 22 Apr 2022 03:22
 Operator : SY/MD
 Sample : N2488-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.697	3216	3221	3228	rBV3	552	690	0.06%	0.008%
78	11.751	3228	3238	3245	rBV3	6653	10268	0.95%	0.112%
79	11.813	3245	3257	3280	rVB	556601	963291	88.75%	10.491%
80	11.957	3300	3302	3306	rBV4	467	325	0.03%	0.004%
81	11.999	3313	3315	3320	rVB	283	167	0.02%	0.002%
82	12.028	3320	3324	3326	rBV3	302	240	0.02%	0.003%
83	12.067	3331	3336	3340	rBV3	1504	1296	0.12%	0.014%
84	12.195	3362	3376	3400	rBV2	506583	914844	84.29%	9.964%
85	12.449	3452	3455	3459	rBV4	357	250	0.02%	0.003%
86	12.507	3470	3473	3476	rBV2	275	241	0.02%	0.003%
87	12.558	3486	3489	3490	rBV2	322	158	0.01%	0.002%
88	12.761	3549	3552	3553	rBV2	238	167	0.02%	0.002%
89	12.790	3558	3561	3565	rVB2	463	425	0.04%	0.005%
90	12.816	3565	3569	3572	rBV2	366	303	0.03%	0.003%
91	13.047	3638	3641	3646	rBV3	224	192	0.02%	0.002%
92	13.089	3648	3654	3655	rBV2	256	266	0.02%	0.003%
93	13.263	3702	3708	3711	rBV2	310	399	0.04%	0.004%
94	13.356	3734	3737	3743	rBV2	355	398	0.04%	0.004%
95	13.845	3878	3889	3901	rVB	25811	40913	3.77%	0.446%
96	13.996	3934	3936	3939	rBV3	285	186	0.02%	0.002%
97	14.102	3961	3969	3970	rBV3	651	817	0.08%	0.009%
98	14.333	4031	4041	4054	rVV2	12192	19285	1.78%	0.210%
99	15.478	4394	4397	4399	rBV2	624	483	0.04%	0.005%
100	15.999	4556	4559	4567	rVB6	2184	2461	0.23%	0.027%


Sum of corrected areas: 9181903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048200.D
Acq On : 22 Apr 2022 03:22
Operator : SY/MD
Sample : N2488-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

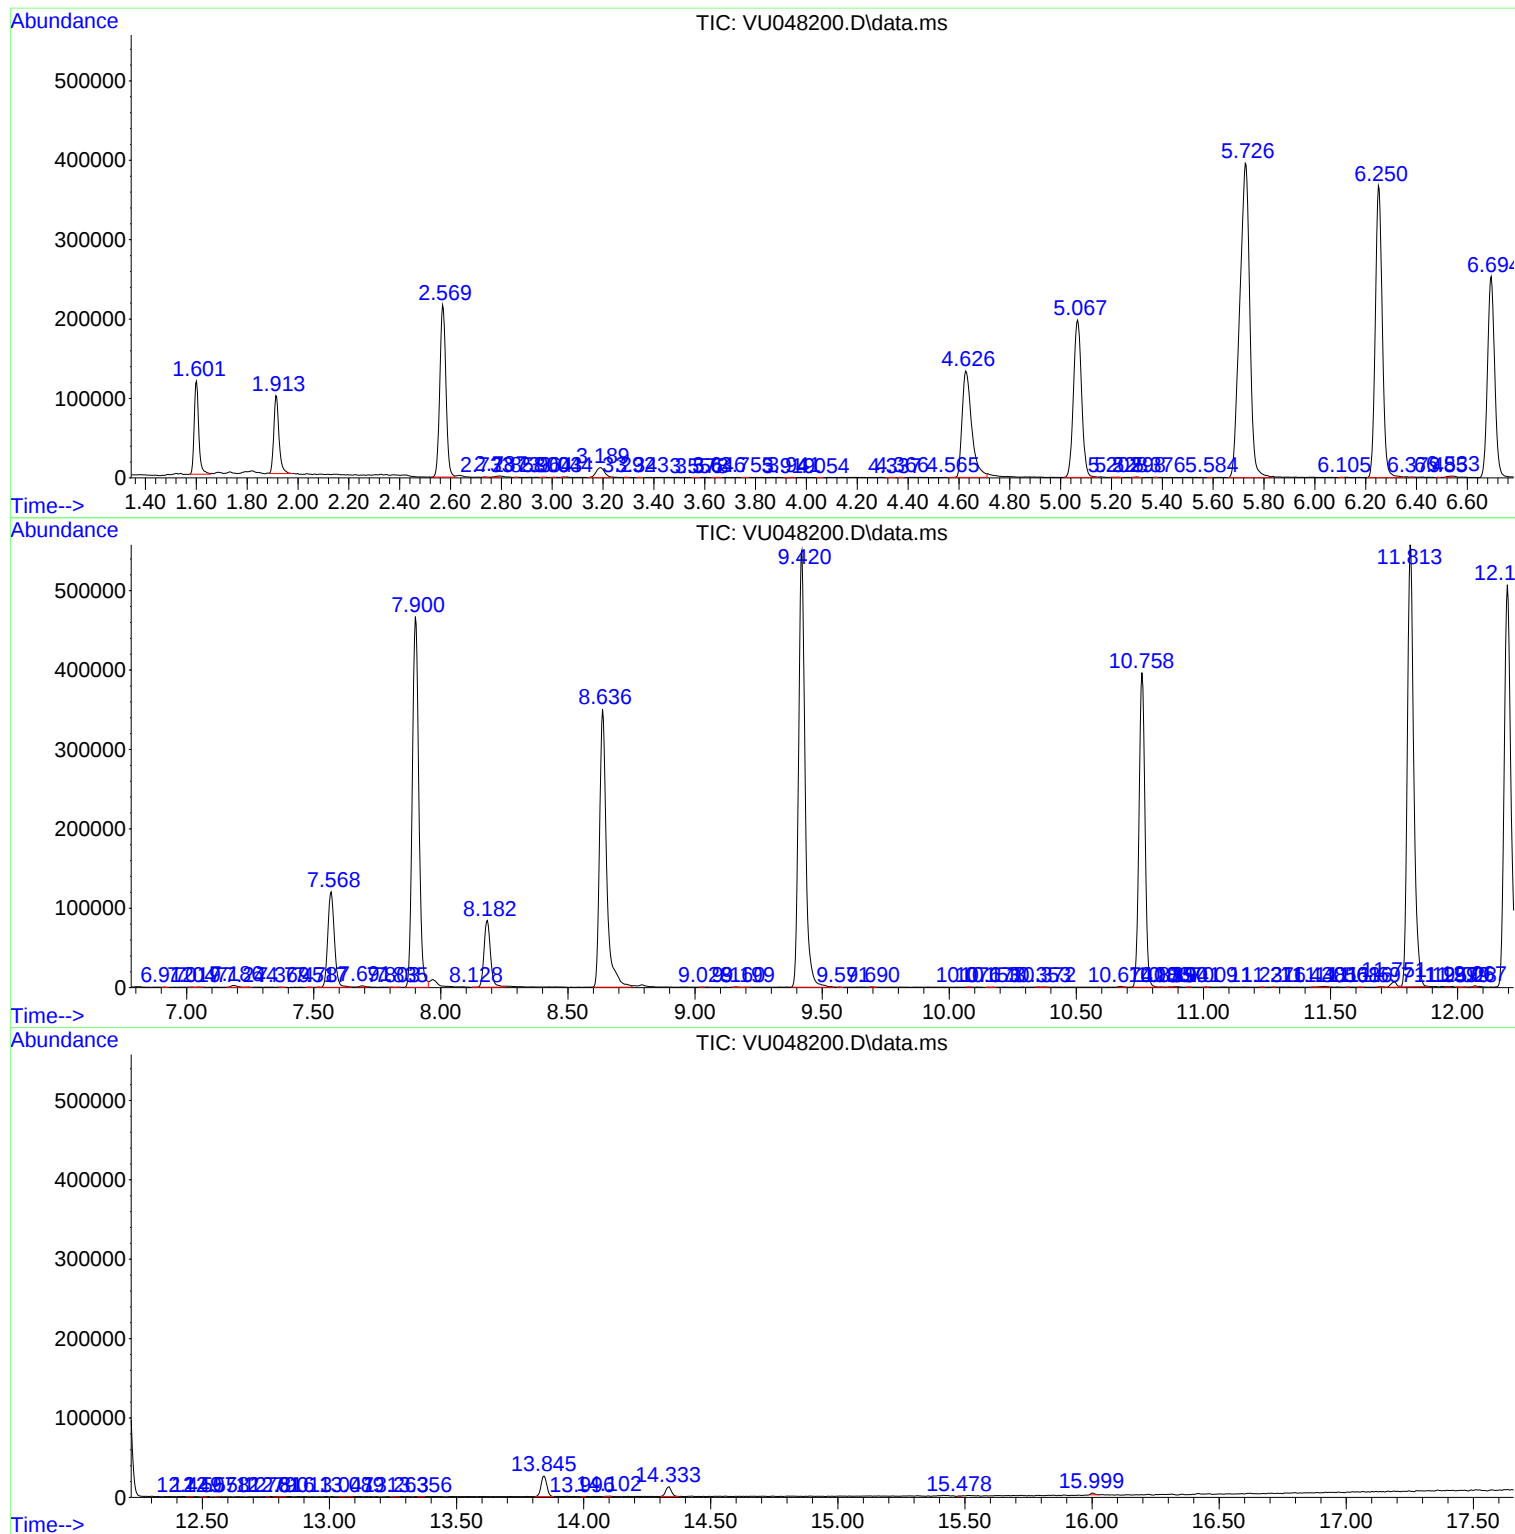

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048200.D
Acq On : 22 Apr 2022 03:22
Operator : SY/MD
Sample : N2488-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048200.D
Acq On : 22 Apr 2022 03:22
Operator : SY/MD
Sample : N2488-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc