

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048201.D
 Acq On : 22 Apr 2022 03:52
 Operator : SY/MD
 Sample : N2488-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	100	rVB	116882	139583	12.59%	1.499%
2	1.916	170	179	195	rBV	97272	139031	12.54%	1.493%
3	2.568	369	382	398	rBV	221218	362195	32.67%	3.889%
4	2.729	428	432	433	rBV3	338	245	0.02%	0.003%
5	2.758	433	441	446	rVV3	1490	2148	0.19%	0.023%
6	2.835	462	465	468	rVV2	307	221	0.02%	0.002%
7	2.893	476	483	485	rBV2	632	517	0.05%	0.006%
8	3.047	521	531	537	rBV5	948	1581	0.14%	0.017%
9	3.189	562	575	592	rVB	4937	11481	1.04%	0.123%
10	3.440	648	653	655	rBV2	237	185	0.02%	0.002%
11	3.520	675	678	683	rBV2	185	223	0.02%	0.002%
12	3.723	736	741	747	rBV2	245	296	0.03%	0.003%
13	3.983	819	822	826	rBV	264	235	0.02%	0.003%
14	4.067	845	848	852	rVB2	252	175	0.02%	0.002%
15	4.324	925	928	931	rBV2	265	177	0.02%	0.002%
16	4.420	954	958	962	rBV2	233	192	0.02%	0.002%
17	4.623	1008	1021	1059	rBV	118894	299124	26.98%	3.212%
18	5.067	1141	1159	1182	rBV	202725	448646	40.47%	4.818%
19	5.215	1203	1205	1212	rVB2	258	196	0.02%	0.002%
20	5.295	1224	1230	1233	rBV2	453	453	0.04%	0.005%
21	5.359	1247	1250	1254	rVB	255	186	0.02%	0.002%
22	5.729	1343	1365	1394	rBV2	397206	1108673	100.00%	11.905%
23	5.877	1407	1411	1417	rVB4	460	369	0.03%	0.004%
24	6.031	1456	1459	1461	rVB3	328	192	0.02%	0.002%
25	6.115	1476	1485	1489	rBV4	458	623	0.06%	0.007%
26	6.250	1513	1527	1560	rBV	364071	696751	62.85%	7.482%
27	6.459	1590	1592	1597	rVB3	369	255	0.02%	0.003%
28	6.504	1601	1606	1607	rBV	236	195	0.02%	0.002%
29	6.530	1607	1614	1625	rVB5	1575	2997	0.27%	0.032%
30	6.571	1625	1627	1630	rBV3	246	176	0.02%	0.002%
31	6.613	1636	1640	1644	rBV2	322	374	0.03%	0.004%
32	6.694	1650	1665	1695	rBV	255016	502142	45.29%	5.392%
33	6.806	1697	1700	1708	rVV4	854	1130	0.10%	0.012%
34	6.922	1733	1736	1739	rBV2	329	204	0.02%	0.002%
35	6.980	1750	1754	1759	rBV2	231	248	0.02%	0.003%
36	7.089	1785	1788	1794	rVB2	324	340	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048201.D
 Acq On : 22 Apr 2022 03:52
 Operator : SY/MD
 Sample : N2488-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.182	1809	1817	1826	rBV4	2308	4070	0.37%	0.044%
38	7.324	1856	1861	1868	rBV2	160	206	0.02%	0.002%
39	7.568	1923	1937	1959	rVV	120241	214241	19.32%	2.301%
40	7.649	1959	1962	1966	rVV2	569	538	0.05%	0.006%
41	7.690	1970	1975	1987	rVB5	1711	2910	0.26%	0.031%
42	7.735	1987	1989	1994	rVB2	342	282	0.03%	0.003%
43	7.761	1994	1997	2002	rBV2	218	187	0.02%	0.002%
44	7.832	2014	2019	2023	rVB2	227	251	0.02%	0.003%
45	7.899	2026	2040	2057	rBV	468306	821273	74.08%	8.819%
46	8.182	2115	2128	2143	rBV	86564	148445	13.39%	1.594%
47	8.298	2160	2164	2168	rBV3	442	435	0.04%	0.005%
48	8.436	2203	2207	2210	rBV3	475	381	0.03%	0.004%
49	8.456	2210	2213	2215	rVV2	404	279	0.03%	0.003%
50	8.475	2216	2219	2226	rVV3	862	844	0.08%	0.009%
51	8.504	2226	2228	2232	rVB	583	374	0.03%	0.004%
52	8.526	2232	2235	2237	rBV2	364	241	0.02%	0.003%
53	8.559	2237	2245	2247	rBV2	585	565	0.05%	0.006%
54	8.632	2256	2268	2301	rBV2	319859	639954	57.72%	6.872%
55	8.967	2369	2372	2376	rBV3	226	226	0.02%	0.002%
56	9.031	2386	2392	2394	rBV2	201	212	0.02%	0.002%
57	9.057	2397	2400	2406	rVB2	463	446	0.04%	0.005%
58	9.089	2406	2410	2412	rBV2	302	255	0.02%	0.003%
59	9.105	2412	2415	2418	rVB2	426	217	0.02%	0.002%
60	9.166	2432	2434	2437	rVV	334	177	0.02%	0.002%
61	9.192	2437	2442	2445	rVV2	208	202	0.02%	0.002%
62	9.237	2452	2456	2460	rBV2	265	319	0.03%	0.003%
63	9.266	2460	2465	2472	rVB3	407	533	0.05%	0.006%
64	9.420	2500	2513	2549	rBV	552902	1023087	92.28%	10.986%
65	9.575	2559	2561	2566	rVB2	213	176	0.02%	0.002%
66	9.636	2577	2580	2583	rBV2	289	199	0.02%	0.002%
67	9.694	2592	2598	2605	rBV3	613	950	0.09%	0.010%
68	9.774	2618	2623	2629	rBV2	356	406	0.04%	0.004%
69	9.874	2649	2654	2659	rBV2	317	296	0.03%	0.003%
70	9.951	2673	2678	2681	rBV	206	232	0.02%	0.002%
71	10.018	2696	2699	2704	rBV2	248	261	0.02%	0.003%
72	10.536	2857	2860	2861	rBV2	317	192	0.02%	0.002%
73	10.616	2877	2885	2887	rBV2	308	418	0.04%	0.004%
74	10.674	2895	2903	2911	rBV3	1285	1726	0.16%	0.019%
75	10.758	2916	2929	2951	rVV	395414	643253	58.02%	6.907%
76	10.880	2965	2967	2969	rBV	444	242	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048201.D
 Acq On : 22 Apr 2022 03:52
 Operator : SY/MD
 Sample : N2488-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.967	2991	2994	2996	rBV2	303	240	0.02%	0.003%
78	11.324	3102	3105	3107	rBV	243	181	0.02%	0.002%
79	11.462	3140	3148	3151	rBV3	770	1007	0.09%	0.011%
80	11.533	3164	3170	3172	rBV	281	326	0.03%	0.004%
81	11.700	3217	3222	3224	rVV3	323	249	0.02%	0.003%
82	11.748	3227	3237	3245	rBV2	15466	23954	2.16%	0.257%
83	11.812	3245	3257	3279	rVB	554837	996810	89.91%	10.704%
84	11.944	3295	3298	3300	rVB	489	300	0.03%	0.003%
85	12.063	3330	3335	3337	rBV3	2289	1916	0.17%	0.021%
86	12.195	3363	3376	3402	rVB2	507742	939545	84.75%	10.089%
87	12.500	3465	3471	3474	rBV3	494	620	0.06%	0.007%
88	12.693	3522	3531	3533	rBV3	390	604	0.05%	0.006%
89	12.729	3536	3542	3546	rBV3	487	541	0.05%	0.006%
90	12.764	3551	3553	3555	rVV2	452	214	0.02%	0.002%
91	12.777	3555	3557	3562	rVB2	342	210	0.02%	0.002%
92	12.915	3597	3600	3602	rBV	273	197	0.02%	0.002%
93	13.028	3632	3635	3640	rBV2	424	382	0.03%	0.004%
94	13.108	3651	3660	3662	rBV3	458	607	0.05%	0.007%
95	13.224	3689	3696	3703	rBV6	1813	2475	0.22%	0.027%
96	13.291	3715	3717	3720	rBV2	316	196	0.02%	0.002%
97	13.423	3756	3758	3764	rVB2	464	309	0.03%	0.003%
98	13.844	3879	3889	3905	rBV	48763	78591	7.09%	0.844%
99	14.333	4032	4041	4054	rVB2	20251	31495	2.84%	0.338%
100	15.578	4426	4428	4430	rBV3	610	334	0.03%	0.004%




Sum of corrected areas: 9312563

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048201.D
Acq On : 22 Apr 2022 03:52
Operator : SY/MD
Sample : N2488-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

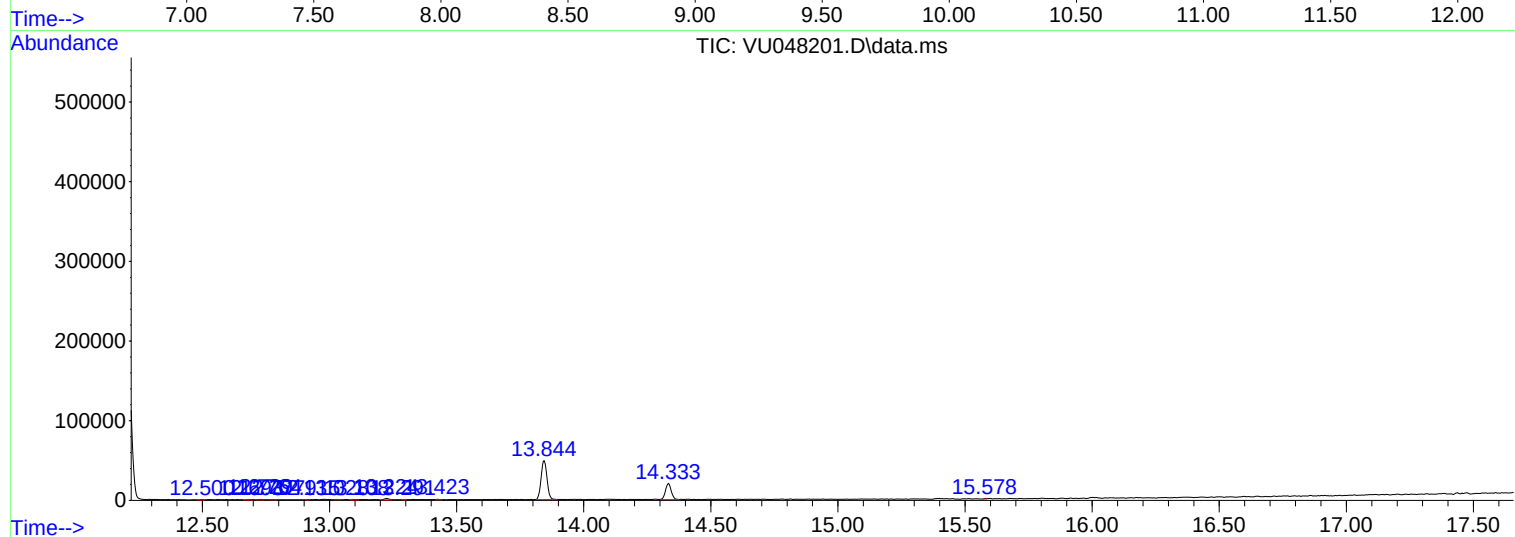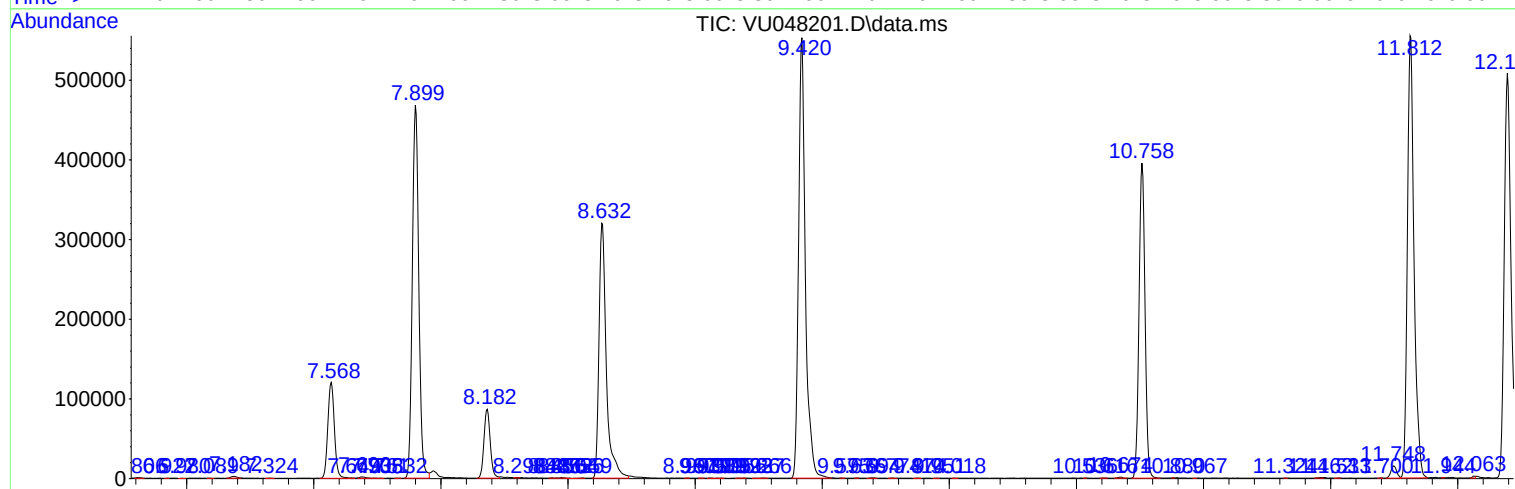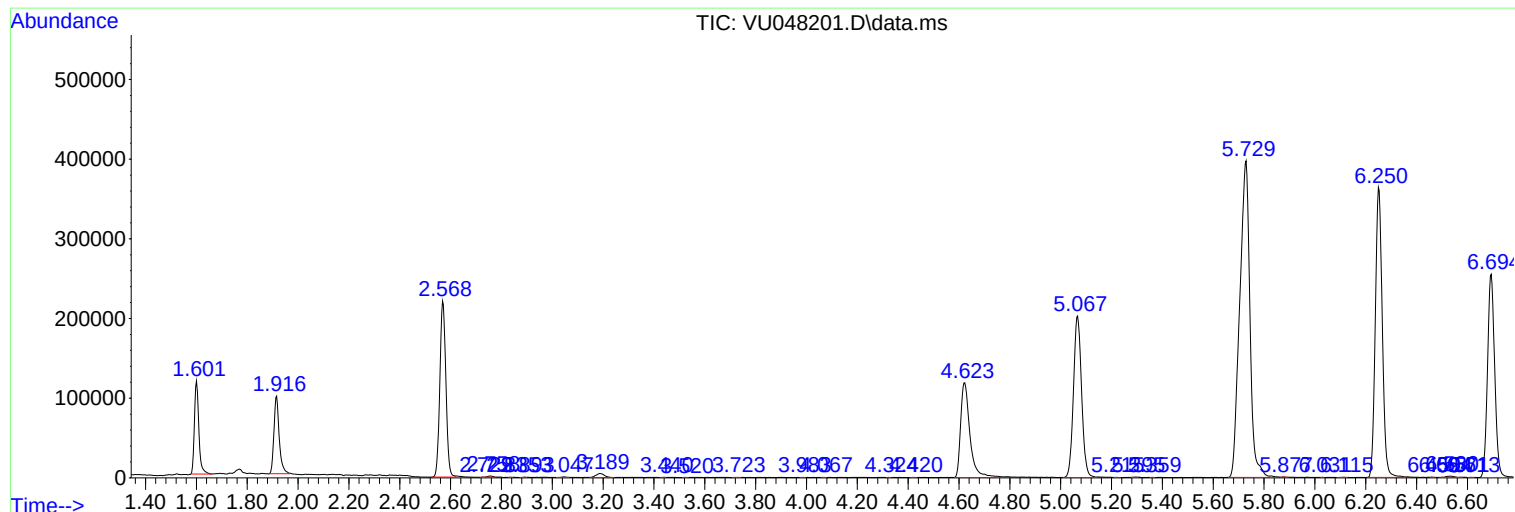

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048201.D
Acq On : 22 Apr 2022 03:52
Operator : SY/MD
Sample : N2488-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048201.D
Acq On : 22 Apr 2022 03:52
Operator : SY/MD
Sample : N2488-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------