

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048202.D
 Acq On : 22 Apr 2022 04:23
 Operator : SY/MD
 Sample : N2488-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	116563	141608	12.96%	1.586%
2	1.912	170	178	199	rVB	97211	139097	12.73%	1.558%
3	2.568	369	382	395	rBV	220419	361891	33.13%	4.052%
4	2.719	426	429	435	rBV3	459	338	0.03%	0.004%
5	2.764	438	443	448	rBV2	664	829	0.08%	0.009%
6	2.819	457	460	463	rVB2	326	241	0.02%	0.003%
7	2.835	463	465	470	rVB2	280	197	0.02%	0.002%
8	2.864	470	474	477	rBV2	380	227	0.02%	0.003%
9	2.903	484	486	489	rBV2	309	211	0.02%	0.002%
10	3.031	519	526	527	rBV2	435	473	0.04%	0.005%
11	3.041	527	529	532	rVV3	567	384	0.04%	0.004%
12	3.057	532	534	537	rVV2	554	353	0.03%	0.004%
13	3.089	541	544	549	rVV	352	317	0.03%	0.004%
14	3.128	553	556	562	rVV2	432	341	0.03%	0.004%
15	3.173	568	570	572	rVV	602	416	0.04%	0.005%
16	3.192	573	576	588	rVB2	1106	1292	0.12%	0.014%
17	3.279	600	603	606	rBV2	190	198	0.02%	0.002%
18	3.578	691	696	699	rBV2	287	321	0.03%	0.004%
19	3.735	740	745	747	rBV2	260	261	0.02%	0.003%
20	3.764	750	754	757	rVV	311	281	0.03%	0.003%
21	3.809	766	768	772	rVB	336	234	0.02%	0.003%
22	4.202	888	890	898	rVB2	238	213	0.02%	0.002%
23	4.350	930	936	940	rVB2	232	242	0.02%	0.003%
24	4.388	945	948	954	rVB3	278	244	0.02%	0.003%
25	4.623	1008	1021	1049	rBV	119354	298575	27.33%	3.343%
26	5.067	1143	1159	1181	rBV	202500	441608	40.43%	4.945%
27	5.215	1200	1205	1212	rVB4	406	551	0.05%	0.006%
28	5.288	1224	1228	1231	rBV2	758	708	0.06%	0.008%
29	5.359	1244	1250	1254	rVB2	286	321	0.03%	0.004%
30	5.382	1254	1257	1260	rBV	230	205	0.02%	0.002%
31	5.404	1260	1264	1273	rVB2	277	407	0.04%	0.005%
32	5.443	1273	1276	1279	rBV	202	201	0.02%	0.002%
33	5.481	1286	1288	1293	rBV2	287	268	0.02%	0.003%
34	5.514	1294	1298	1301	rVB2	215	190	0.02%	0.002%
35	5.610	1323	1328	1332	rBV2	263	303	0.03%	0.003%
36	5.726	1343	1364	1395	rBV2	397497	1092407	100.00%	12.232%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048202.D
 Acq On : 22 Apr 2022 04:23
 Operator : SY/MD
 Sample : N2488-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.131	1488	1490	1495	rVB2	453	345	0.03%	0.004%
38	6.189	1504	1508	1513	rVB	360	342	0.03%	0.004%
39	6.250	1513	1527	1550	rBV	361386	686568	62.85%	7.688%
40	6.420	1577	1580	1585	rBV3	282	233	0.02%	0.003%
41	6.446	1585	1588	1592	rBV3	387	327	0.03%	0.004%
42	6.478	1595	1598	1601	rVB	316	235	0.02%	0.003%
43	6.497	1601	1604	1607	rBV2	225	187	0.02%	0.002%
44	6.536	1607	1616	1626	rVB6	1910	3794	0.35%	0.042%
45	6.571	1626	1627	1631	rBV2	358	207	0.02%	0.002%
46	6.623	1641	1643	1650	rVB2	305	272	0.02%	0.003%
47	6.694	1650	1665	1686	rBV	252645	502123	45.96%	5.623%
48	6.813	1698	1702	1706	rVB3	921	648	0.06%	0.007%
49	7.112	1792	1795	1799	rBV2	254	207	0.02%	0.002%
50	7.131	1799	1801	1805	rVB	342	191	0.02%	0.002%
51	7.185	1809	1818	1827	rBV4	2485	4169	0.38%	0.047%
52	7.414	1883	1889	1892	rBV2	309	296	0.03%	0.003%
53	7.465	1900	1905	1906	rBV2	356	229	0.02%	0.003%
54	7.568	1925	1937	1952	rBV	120693	211104	19.32%	2.364%
55	7.694	1965	1976	1981	rBV5	1575	2555	0.23%	0.029%
56	7.742	1989	1991	1994	rBV	277	221	0.02%	0.002%
57	7.832	2014	2019	2025	rBV2	186	228	0.02%	0.003%
58	7.899	2026	2040	2057	rBV	465881	822082	75.25%	9.205%
59	8.182	2115	2128	2141	rBV	86236	147983	13.55%	1.657%
60	8.517	2228	2232	2236	rBV2	515	446	0.04%	0.005%
61	8.636	2256	2269	2306	rBV2	344370	662265	60.62%	7.416%
62	8.838	2329	2332	2335	rBV2	429	265	0.02%	0.003%
63	8.861	2337	2339	2344	rVB2	466	270	0.02%	0.003%
64	8.912	2353	2355	2359	rVB3	277	216	0.02%	0.002%
65	8.957	2365	2369	2372	rBV2	300	206	0.02%	0.002%
66	9.018	2385	2388	2391	rBV2	316	275	0.03%	0.003%
67	9.118	2416	2419	2422	rBV	214	201	0.02%	0.002%
68	9.253	2455	2461	2467	rBV3	421	540	0.05%	0.006%
69	9.359	2488	2494	2495	rBV3	503	376	0.03%	0.004%
70	9.420	2500	2513	2538	rBV	545642	934932	85.58%	10.469%
71	9.571	2558	2560	2567	rVB3	296	294	0.03%	0.003%
72	9.690	2593	2597	2599	rBV2	482	381	0.03%	0.004%
73	10.346	2796	2801	2802	rBV	331	191	0.02%	0.002%
74	10.375	2807	2810	2817	rVB	213	196	0.02%	0.002%
75	10.433	2825	2828	2834	rBV2	236	217	0.02%	0.002%
76	10.671	2898	2902	2908	rVB4	1041	1223	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048202.D
 Acq On : 22 Apr 2022 04:23
 Operator : SY/MD
 Sample : N2488-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.697	2908	2910	2915	rVB	253	188	0.02%	0.002%
78	10.758	2915	2929	2951	rBV	402050	652933	59.77%	7.311%
79	10.896	2967	2972	2976	rVV3	842	855	0.08%	0.010%
80	11.002	3003	3005	3009	rBV2	265	236	0.02%	0.003%
81	11.124	3041	3043	3047	rVB2	435	247	0.02%	0.003%
82	11.455	3141	3146	3148	rBV2	921	832	0.08%	0.009%
83	11.533	3166	3170	3175	rVB	260	250	0.02%	0.003%
84	11.639	3200	3203	3204	rBV2	323	190	0.02%	0.002%
85	11.693	3214	3220	3221	rBV3	925	652	0.06%	0.007%
86	11.748	3229	3237	3244	rBV5	2205	3710	0.34%	0.042%
87	11.812	3244	3257	3280	rVV	553889	897049	82.12%	10.045%
88	12.066	3323	3336	3349	rBV4	9093	17368	1.59%	0.194%
89	12.195	3362	3376	3398	rBV	508781	853172	78.10%	9.554%
90	12.327	3413	3417	3423	rBV3	548	648	0.06%	0.007%
91	12.378	3429	3433	3434	rBV2	271	189	0.02%	0.002%
92	12.893	3587	3593	3601	rBV7	2945	3868	0.35%	0.043%
93	12.954	3609	3612	3615	rBV2	344	279	0.03%	0.003%
94	13.121	3661	3664	3668	rBV3	290	256	0.02%	0.003%
95	13.150	3671	3673	3680	rBV3	282	322	0.03%	0.004%
96	13.307	3718	3722	3724	rBV2	286	240	0.02%	0.003%
97	13.481	3772	3776	3779	rBV	391	386	0.04%	0.004%
98	13.719	3847	3850	3853	rBV3	280	194	0.02%	0.002%
99	13.844	3879	3889	3901	rBV2	10728	16416	1.50%	0.184%
100	14.333	4034	4041	4051	rVB3	4397	6899	0.63%	0.077%


Sum of corrected areas: 8930372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048202.D
Acq On : 22 Apr 2022 04:23
Operator : SY/MD
Sample : N2488-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

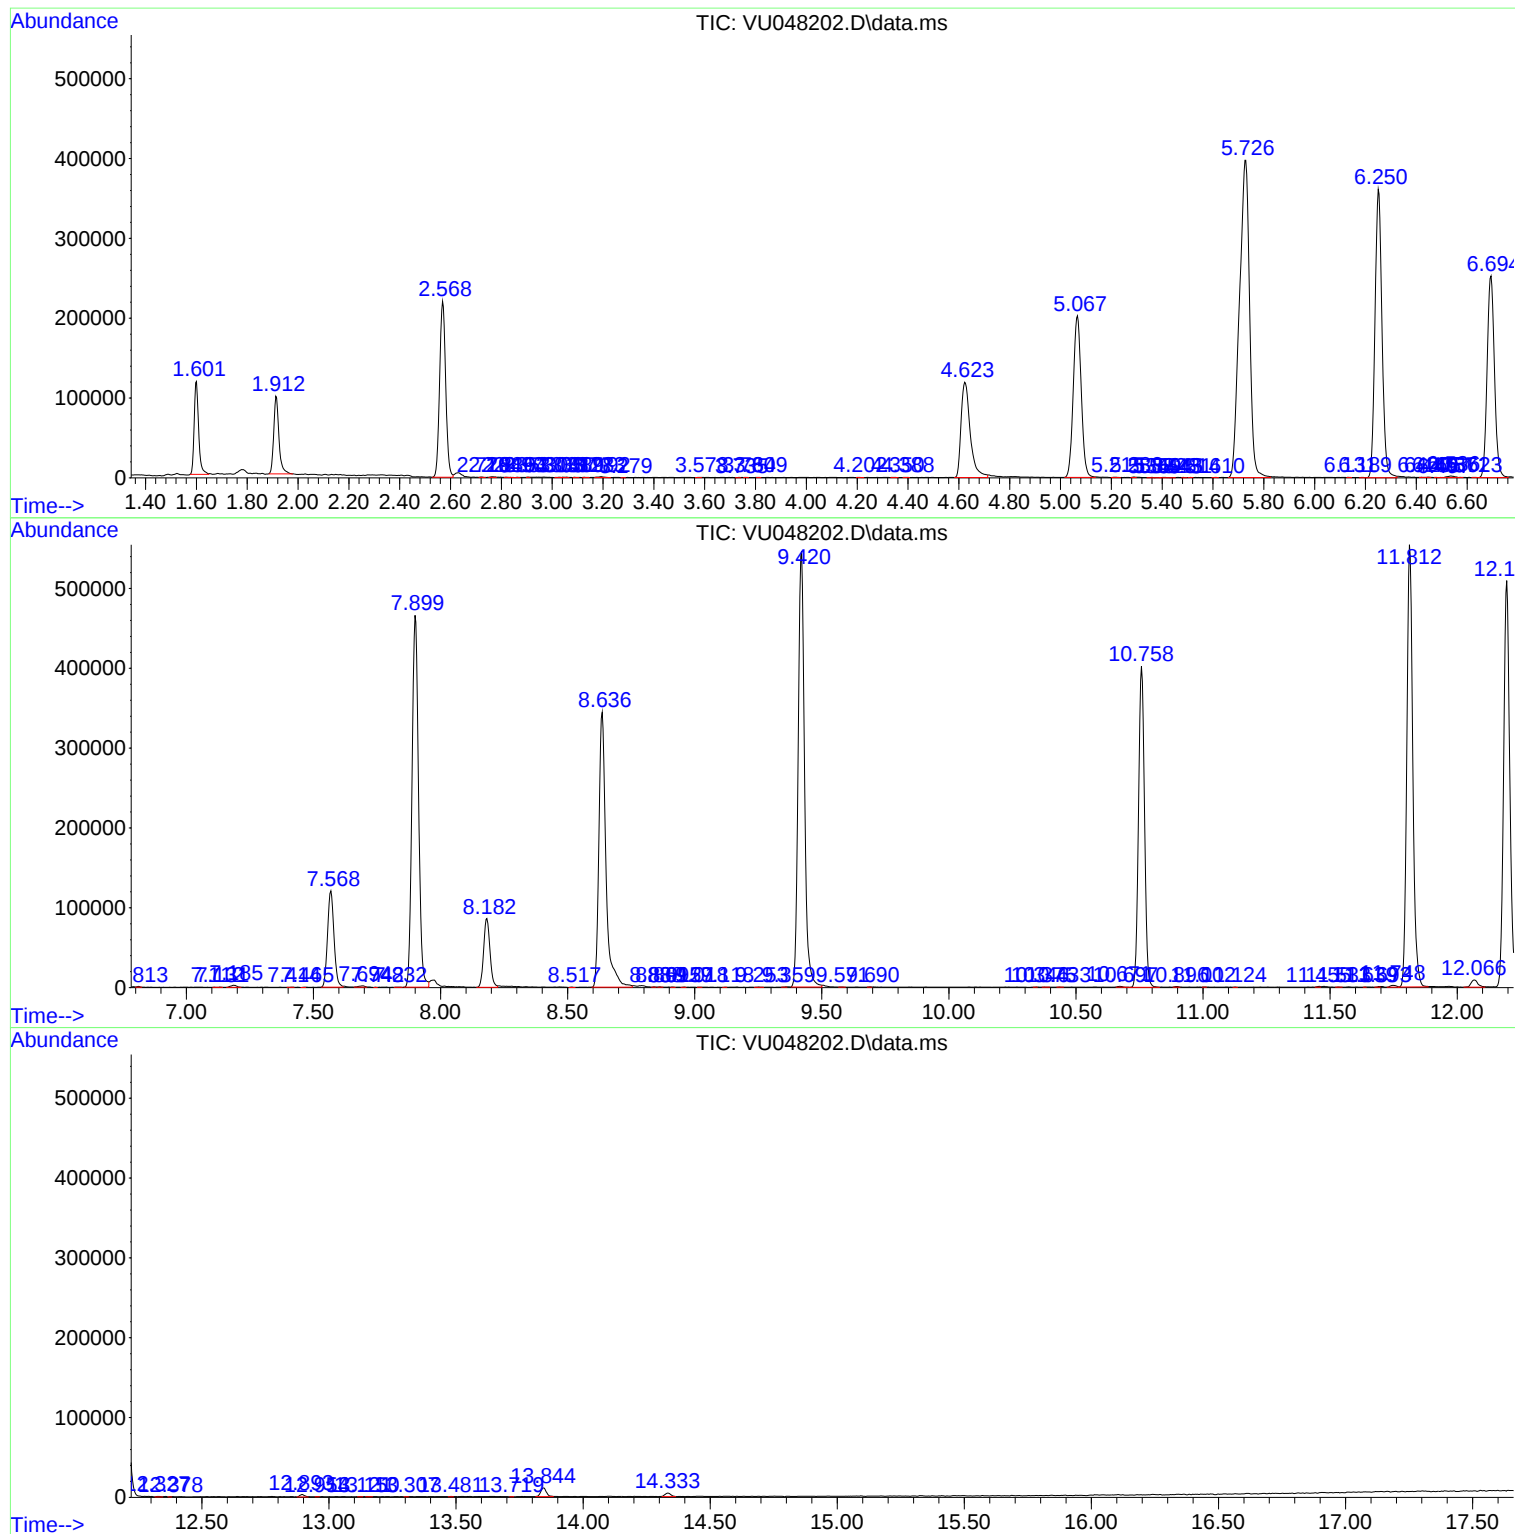

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048202.D
Acq On : 22 Apr 2022 04:23
Operator : SY/MD
Sample : N2488-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048202.D
Acq On : 22 Apr 2022 04:23
Operator : SY/MD
Sample : N2488-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------