

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048204.D
 Acq On : 22 Apr 2022 05:11
 Operator : SY/MD
 Sample : N2488-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	116921	142596	13.10%	1.597%
2	1.916	171	179	195	rVB	100549	141285	12.98%	1.582%
3	2.568	370	382	399	rBV	210715	358985	32.97%	4.021%
4	2.732	432	433	437	rVB3	337	192	0.02%	0.002%
5	2.790	446	451	454	rBV3	822	772	0.07%	0.009%
6	2.819	454	460	468	rBV5	1064	2000	0.18%	0.022%
7	3.006	515	518	521	rBV	460	228	0.02%	0.003%
8	3.044	527	530	533	rBV3	588	428	0.04%	0.005%
9	3.186	564	574	586	rBV2	1876	3860	0.35%	0.043%
10	3.318	612	615	617	rBV	285	228	0.02%	0.003%
11	3.330	617	619	620	rBV	292	162	0.01%	0.002%
12	3.363	623	629	630	rBV3	1535	1279	0.12%	0.014%
13	3.482	663	666	670	rBV2	266	163	0.01%	0.002%
14	3.601	698	703	705	rBV2	276	288	0.03%	0.003%
15	3.662	720	722	725	rBV2	304	174	0.02%	0.002%
16	3.697	728	733	738	rBV2	782	971	0.09%	0.011%
17	3.922	799	803	807	rBV2	235	210	0.02%	0.002%
18	4.266	905	910	913	rBV2	268	243	0.02%	0.003%
19	4.295	913	919	923	rVV2	275	320	0.03%	0.004%
20	4.385	944	947	952	rVB2	364	365	0.03%	0.004%
21	4.633	1010	1024	1062	rBV	117986	330254	30.33%	3.699%
22	5.067	1141	1159	1187	rBV	200746	453577	41.66%	5.080%
23	5.186	1194	1196	1200	rBV2	386	221	0.02%	0.002%
24	5.353	1246	1248	1253	rVB	315	203	0.02%	0.002%
25	5.375	1253	1255	1258	rBV	288	170	0.02%	0.002%
26	5.498	1285	1293	1299	rBV	396	808	0.07%	0.009%
27	5.726	1342	1364	1393	rBV2	400026	1088834	100.00%	12.195%
28	5.880	1409	1412	1416	rBV2	469	296	0.03%	0.003%
29	6.102	1479	1481	1485	rVB2	271	189	0.02%	0.002%
30	6.189	1506	1508	1513	rVB2	212	180	0.02%	0.002%
31	6.250	1513	1527	1554	rBV	361878	695327	63.86%	7.788%
32	6.517	1606	1610	1611	rBV3	737	519	0.05%	0.006%
33	6.533	1611	1615	1619	rVV2	1156	1316	0.12%	0.015%
34	6.552	1619	1621	1623	rVB	407	188	0.02%	0.002%
35	6.694	1650	1665	1687	rBV	256097	502052	46.11%	5.623%
36	6.787	1692	1694	1696	rBV2	378	218	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048204.D
 Acq On : 22 Apr 2022 05:11
 Operator : SY/MD
 Sample : N2488-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.041	1765	1773	1775	rBV2	236	322	0.03%	0.004%
38	7.108	1792	1794	1797	rVB	291	165	0.02%	0.002%
39	7.150	1802	1807	1809	rBV2	391	287	0.03%	0.003%
40	7.189	1809	1819	1828	rVV4	2280	3991	0.37%	0.045%
41	7.478	1905	1909	1912	rVB2	227	169	0.02%	0.002%
42	7.514	1916	1920	1923	rBV	297	286	0.03%	0.003%
43	7.568	1924	1937	1958	rBV	116339	213232	19.58%	2.388%
44	7.690	1969	1975	1984	rBV6	1588	2614	0.24%	0.029%
45	7.771	1991	2000	2004	rBV3	385	556	0.05%	0.006%
46	7.899	2027	2040	2056	rBV	466677	814358	74.79%	9.121%
47	8.179	2116	2127	2145	rBV2	83270	145927	13.40%	1.634%
48	8.398	2192	2195	2199	rBV2	299	236	0.02%	0.003%
49	8.449	2209	2211	2213	rVV	306	185	0.02%	0.002%
50	8.468	2216	2217	2227	rVB2	595	660	0.06%	0.007%
51	8.549	2237	2242	2243	rBV	340	221	0.02%	0.002%
52	8.639	2257	2270	2299	rBV2	355065	698366	64.14%	7.822%
53	8.845	2332	2334	2338	rVB4	499	330	0.03%	0.004%
54	8.874	2340	2343	2345	rBV2	401	231	0.02%	0.003%
55	8.957	2364	2369	2374	rVB2	392	376	0.03%	0.004%
56	8.989	2375	2379	2382	rVB	263	218	0.02%	0.002%
57	9.054	2393	2399	2409	rVB4	557	643	0.06%	0.007%
58	9.095	2409	2412	2416	rBV2	255	204	0.02%	0.002%
59	9.140	2423	2426	2429	rBV2	264	185	0.02%	0.002%
60	9.417	2499	2512	2550	rVV	536116	933864	85.77%	10.459%
61	9.565	2556	2558	2561	rBV3	376	206	0.02%	0.002%
62	9.584	2561	2564	2568	rVB2	216	169	0.02%	0.002%
63	9.694	2594	2598	2600	rBV2	358	299	0.03%	0.003%
64	9.951	2675	2678	2682	rBV	259	216	0.02%	0.002%
65	10.198	2751	2755	2760	rBV	196	198	0.02%	0.002%
66	10.600	2877	2880	2883	rVB	412	294	0.03%	0.003%
67	10.642	2884	2893	2895	rBV2	295	420	0.04%	0.005%
68	10.671	2895	2902	2912	rVV3	1030	1546	0.14%	0.017%
69	10.758	2916	2929	2953	rVV	395920	648418	59.55%	7.262%
70	10.880	2964	2967	2968	rBV	428	231	0.02%	0.003%
71	10.893	2968	2971	2975	rVB2	546	476	0.04%	0.005%
72	10.970	2991	2995	2997	rBV2	253	205	0.02%	0.002%
73	10.983	2997	2999	3006	rVB2	332	242	0.02%	0.003%
74	11.018	3006	3010	3013	rBV	380	295	0.03%	0.003%
75	11.247	3078	3081	3086	rBV3	214	162	0.01%	0.002%
76	11.465	3145	3149	3150	rBV3	428	313	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048204.D
 Acq On : 22 Apr 2022 05:11
 Operator : SY/MD
 Sample : N2488-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.661	3208	3210	3216	rBV3	222	207	0.02%	0.002%
78	11.693	3216	3220	3224	rBV2	340	349	0.03%	0.004%
79	11.748	3231	3237	3243	rBV4	1644	1914	0.18%	0.021%
80	11.812	3244	3257	3278	rBV	549173	885587	81.33%	9.919%
81	11.970	3303	3306	3313	rVB3	733	774	0.07%	0.009%
82	12.070	3328	3337	3345	rBV7	1993	3736	0.34%	0.042%
83	12.102	3345	3347	3354	rVB5	622	654	0.06%	0.007%
84	12.137	3355	3358	3362	rBV2	273	169	0.02%	0.002%
85	12.195	3362	3376	3396	rBV	493395	821188	75.42%	9.197%
86	12.308	3408	3411	3415	rVB3	422	317	0.03%	0.004%
87	12.362	3424	3428	3429	rBV2	320	195	0.02%	0.002%
88	12.372	3429	3431	3434	rVV2	265	154	0.01%	0.002%
89	12.443	3450	3453	3459	rBV2	478	563	0.05%	0.006%
90	12.520	3471	3477	3479	rBV2	408	394	0.04%	0.004%
91	12.539	3480	3483	3486	rVB	292	180	0.02%	0.002%
92	12.558	3486	3489	3494	rBV2	457	402	0.04%	0.005%
93	12.584	3494	3497	3503	rBV2	303	349	0.03%	0.004%
94	12.777	3554	3557	3560	rBV	428	210	0.02%	0.002%
95	13.102	3655	3658	3660	rBV2	387	261	0.02%	0.003%
96	13.774	3864	3867	3868	rBV	323	171	0.02%	0.002%
97	13.844	3883	3889	3900	rVB3	4671	7024	0.65%	0.079%
98	14.336	4035	4042	4050	rBV4	1763	2731	0.25%	0.031%
99	15.208	4310	4313	4315	rBV2	494	222	0.02%	0.002%
100	15.246	4323	4325	4328	rBV2	479	351	0.03%	0.004%




Sum of corrected areas: 8928519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048204.D
Acq On : 22 Apr 2022 05:11
Operator : SY/MD
Sample : N2488-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

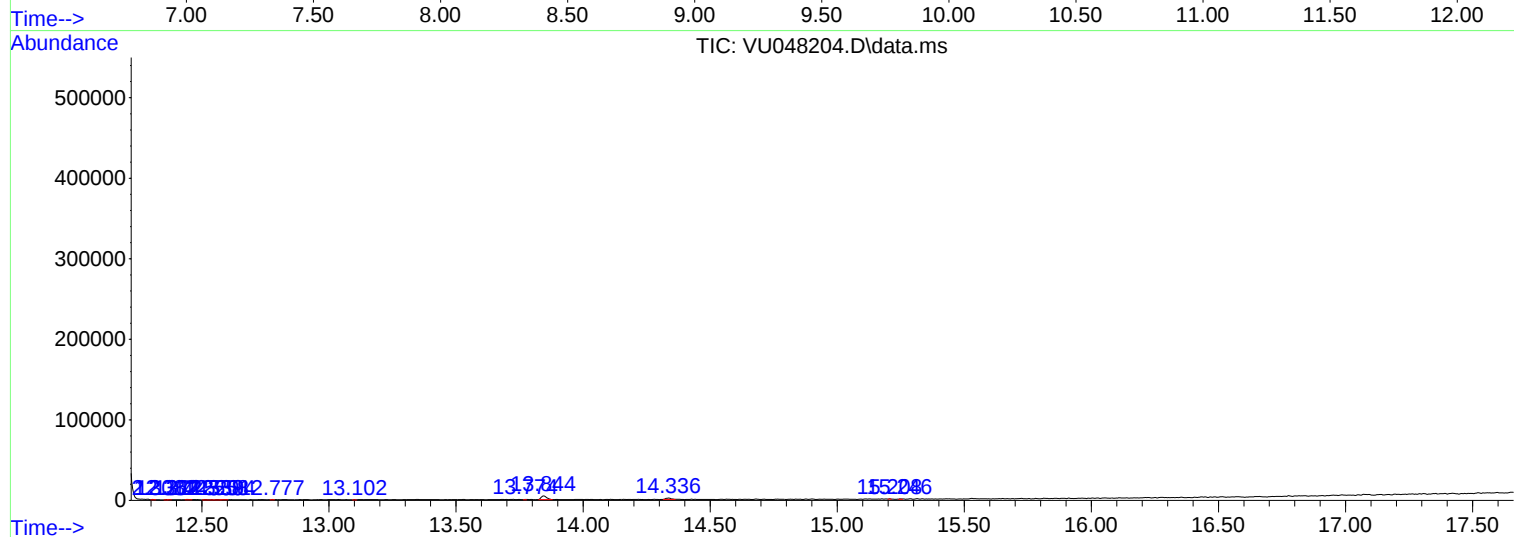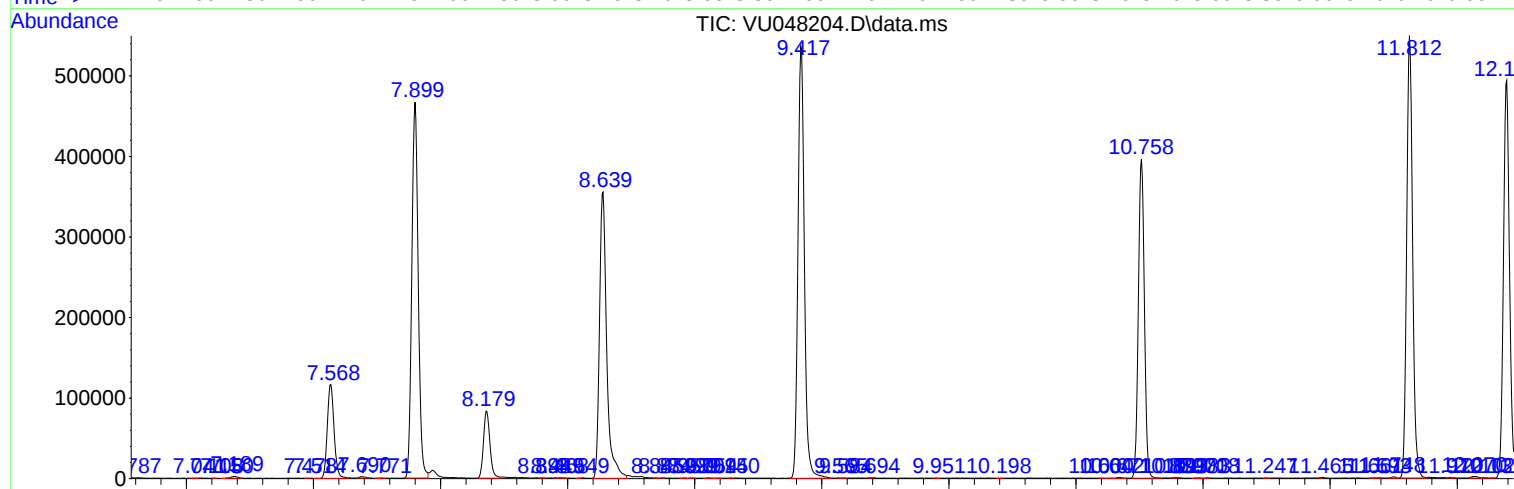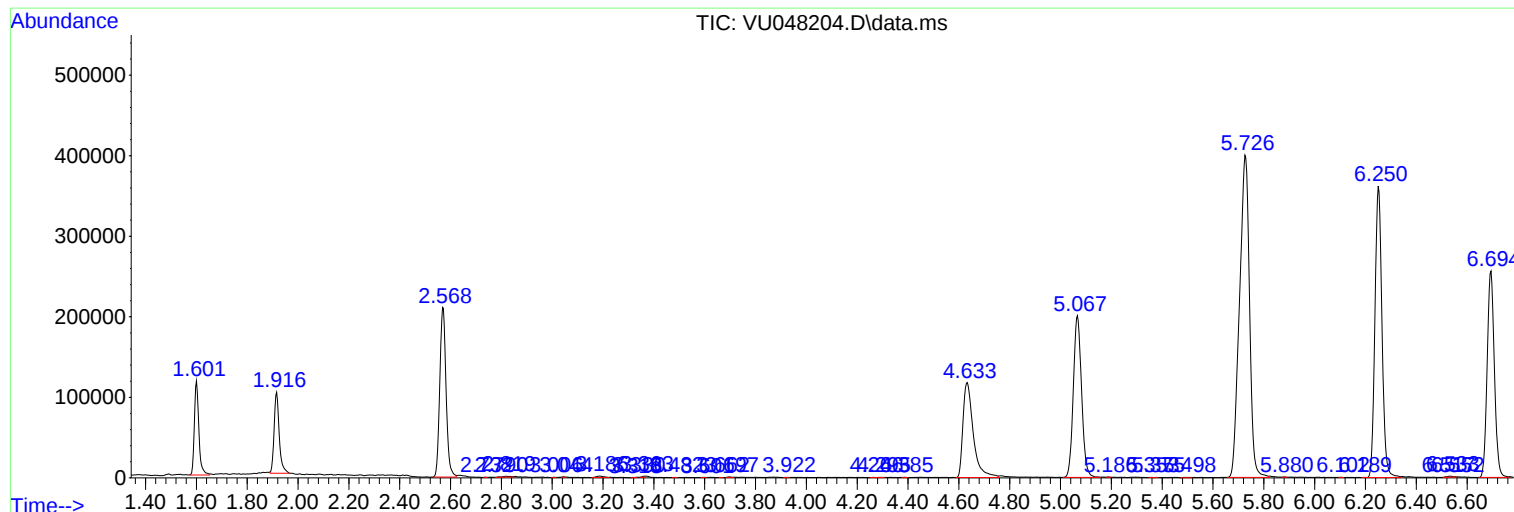

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048204.D
Acq On : 22 Apr 2022 05:11
Operator : SY/MD
Sample : N2488-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048204.D
Acq On : 22 Apr 2022 05:11
Operator : SY/MD
Sample : N2488-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc