

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048206.D
 Acq On : 22 Apr 2022 05:58
 Operator : SY/MD
 Sample : N2488-13 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	94	rBV	118499	139928	4.16%	1.013%
2	1.912	170	178	196	rBV	94340	135081	4.01%	0.978%
3	2.568	369	382	396	rBV	218449	358162	10.64%	2.593%
4	2.726	426	431	434	rBV3	373	362	0.01%	0.003%
5	2.758	434	441	442	rBV2	1269	1240	0.04%	0.009%
6	2.832	463	464	467	rBV2	283	178	0.01%	0.001%
7	2.896	480	484	488	rBV2	579	497	0.01%	0.004%
8	2.938	492	497	498	rBV	270	176	0.01%	0.001%
9	3.022	520	523	525	rBV2	291	181	0.01%	0.001%
10	3.044	525	530	543	rVB4	1633	2798	0.08%	0.020%
11	3.189	559	575	596	rBV	61196	140018	4.16%	1.014%
12	3.324	612	617	619	rBV2	226	213	0.01%	0.002%
13	3.523	674	679	682	rVB2	251	301	0.01%	0.002%
14	3.549	682	687	690	rBV2	276	268	0.01%	0.002%
15	3.774	752	757	760	rVB2	484	441	0.01%	0.003%
16	3.800	761	765	767	rBV	279	257	0.01%	0.002%
17	4.067	844	848	852	rBV2	346	396	0.01%	0.003%
18	4.108	858	861	866	rVB	250	205	0.01%	0.001%
19	4.260	905	908	912	rBV2	173	178	0.01%	0.001%
20	4.620	1006	1020	1054	rBV	138207	342191	10.17%	2.477%
21	5.067	1142	1159	1182	rBV	201254	463217	13.77%	3.353%
22	5.205	1199	1202	1207	rVB4	431	404	0.01%	0.003%
23	5.234	1207	1211	1214	rVB2	210	207	0.01%	0.001%
24	5.256	1214	1218	1222	rBV2	232	239	0.01%	0.002%
25	5.285	1222	1227	1228	rBV2	379	298	0.01%	0.002%
26	5.333	1237	1242	1243	rBV2	318	246	0.01%	0.002%
27	5.372	1252	1254	1257	rVB	301	190	0.01%	0.001%
28	5.398	1257	1262	1267	rBV2	301	392	0.01%	0.003%
29	5.530	1293	1303	1314	rVB3	2777	5505	0.16%	0.040%
30	5.726	1342	1364	1374	rBV2	399401	1111743	33.04%	8.047%
31	5.915	1421	1423	1426	rVB2	435	269	0.01%	0.002%
32	5.973	1437	1441	1447	rVB3	841	769	0.02%	0.006%
33	6.009	1447	1452	1456	rBV3	320	375	0.01%	0.003%
34	6.044	1459	1463	1468	rVB4	499	470	0.01%	0.003%
35	6.070	1468	1471	1477	rVB3	213	168	0.00%	0.001%
36	6.115	1480	1485	1487	rBV2	250	237	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048206.D
 Acq On : 22 Apr 2022 05:58
 Operator : SY/MD
 Sample : N2488-13 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.150	1491	1496	1498	rVB2	213	181	0.01%	0.001%
38	6.250	1513	1527	1556	rBV	391063	742176	22.06%	5.372%
39	6.526	1607	1613	1614	rBV3	1581	1242	0.04%	0.009%
40	6.610	1633	1639	1644	rVB2	306	365	0.01%	0.003%
41	6.690	1650	1664	1685	rBV	255482	499612	14.85%	3.616%
42	6.796	1695	1697	1698	rBV	512	252	0.01%	0.002%
43	6.841	1707	1711	1714	rBV2	367	221	0.01%	0.002%
44	6.976	1750	1753	1756	rBV	254	206	0.01%	0.001%
45	6.993	1756	1758	1760	rVV	288	177	0.01%	0.001%
46	7.028	1766	1769	1773	rVV	211	223	0.01%	0.002%
47	7.054	1774	1777	1783	rVV2	372	424	0.01%	0.003%
48	7.182	1806	1817	1826	rBV6	2557	4782	0.14%	0.035%
49	7.346	1863	1868	1870	rBV	233	201	0.01%	0.001%
50	7.565	1923	1936	1961	rBV	119271	212870	6.33%	1.541%
51	7.655	1961	1964	1968	rVB4	243	179	0.01%	0.001%
52	7.690	1968	1975	1979	rBV5	1625	2108	0.06%	0.015%
53	7.748	1991	1993	1997	rVB2	287	168	0.00%	0.001%
54	7.899	2023	2040	2056	rBV	478052	828709	24.63%	5.999%
55	8.111	2103	2106	2109	rBV3	253	166	0.00%	0.001%
56	8.179	2114	2127	2142	rBV	85953	145545	4.33%	1.054%
57	8.317	2168	2170	2176	rBV2	327	287	0.01%	0.002%
58	8.372	2185	2187	2192	rVB2	362	212	0.01%	0.002%
59	8.446	2206	2210	2211	rBV3	276	193	0.01%	0.001%
60	8.632	2253	2268	2303	rBV	340993	643543	19.13%	4.658%
61	8.864	2337	2340	2344	rBV	233	204	0.01%	0.001%
62	8.890	2344	2348	2351	rVB2	266	224	0.01%	0.002%
63	8.941	2360	2364	2367	rVB2	276	256	0.01%	0.002%
64	8.963	2367	2371	2374	rBV2	309	222	0.01%	0.002%
65	9.156	2426	2431	2432	rBV	316	209	0.01%	0.002%
66	9.198	2442	2444	2448	rVB2	344	192	0.01%	0.001%
67	9.343	2483	2489	2493	rBV3	172	216	0.01%	0.002%
68	9.446	2499	2521	2564	rVV2	1456713	3364712	100.00%	24.355%
69	9.664	2587	2589	2593	rVB2	315	177	0.01%	0.001%
70	9.690	2593	2597	2600	rBV2	613	599	0.02%	0.004%
71	9.809	2631	2634	2640	rVB4	395	367	0.01%	0.003%
72	10.099	2721	2724	2728	rBV2	179	174	0.01%	0.001%
73	10.250	2768	2771	2778	rVB2	253	252	0.01%	0.002%
74	10.285	2778	2782	2785	rBV	249	173	0.01%	0.001%
75	10.671	2898	2902	2909	rVB3	860	965	0.03%	0.007%
76	10.758	2915	2929	2947	rBV	402749	649808	19.31%	4.704%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048206.D
 Acq On : 22 Apr 2022 05:58
 Operator : SY/MD
 Sample : N2488-13 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.870	2959	2964	2969	rBV3	443	468	0.01%	0.003%
78	10.931	2980	2983	2986	rBV2	259	174	0.01%	0.001%
79	11.105	3032	3037	3040	rBV2	368	277	0.01%	0.002%
80	11.221	3070	3073	3076	rBV2	244	192	0.01%	0.001%
81	11.291	3090	3095	3100	rBV2	276	288	0.01%	0.002%
82	11.449	3140	3144	3145	rBV	454	274	0.01%	0.002%
83	11.697	3216	3221	3225	rBV3	261	253	0.01%	0.002%
84	11.745	3225	3236	3246	rBV	81457	130603	3.88%	0.945%
85	11.815	3246	3258	3260	rBV	663747	912284	27.11%	6.604%
86	11.973	3302	3307	3315	rVB7	837	1269	0.04%	0.009%
87	12.147	3357	3361	3363	rBV2	396	345	0.01%	0.002%
88	12.208	3363	3380	3406	rVV2	1002390	2231216	66.31%	16.151%
89	12.385	3432	3435	3439	rBV3	409	329	0.01%	0.002%
90	12.478	3462	3464	3467	rBV	256	169	0.01%	0.001%
91	12.619	3504	3508	3510	rBV2	345	317	0.01%	0.002%
92	12.674	3521	3525	3527	rBV	390	355	0.01%	0.003%
93	12.973	3612	3618	3631	rVB5	2173	3019	0.09%	0.022%
94	13.221	3691	3695	3703	rVB4	1585	1664	0.05%	0.012%
95	13.327	3722	3728	3729	rBV4	839	670	0.02%	0.005%
96	13.841	3876	3888	3905	rBV	340861	536794	15.95%	3.886%
97	14.330	4029	4040	4055	rBV2	113903	180671	5.37%	1.308%
98	14.568	4110	4114	4116	rBV2	437	308	0.01%	0.002%
99	15.105	4279	4281	4283	rBV	443	252	0.01%	0.002%
100	15.426	4373	4381	4386	rBV7	1367	2287	0.07%	0.017%




Sum of corrected areas: 13815070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048206.D
Acq On : 22 Apr 2022 05:58
Operator : SY/MD
Sample : N2488-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

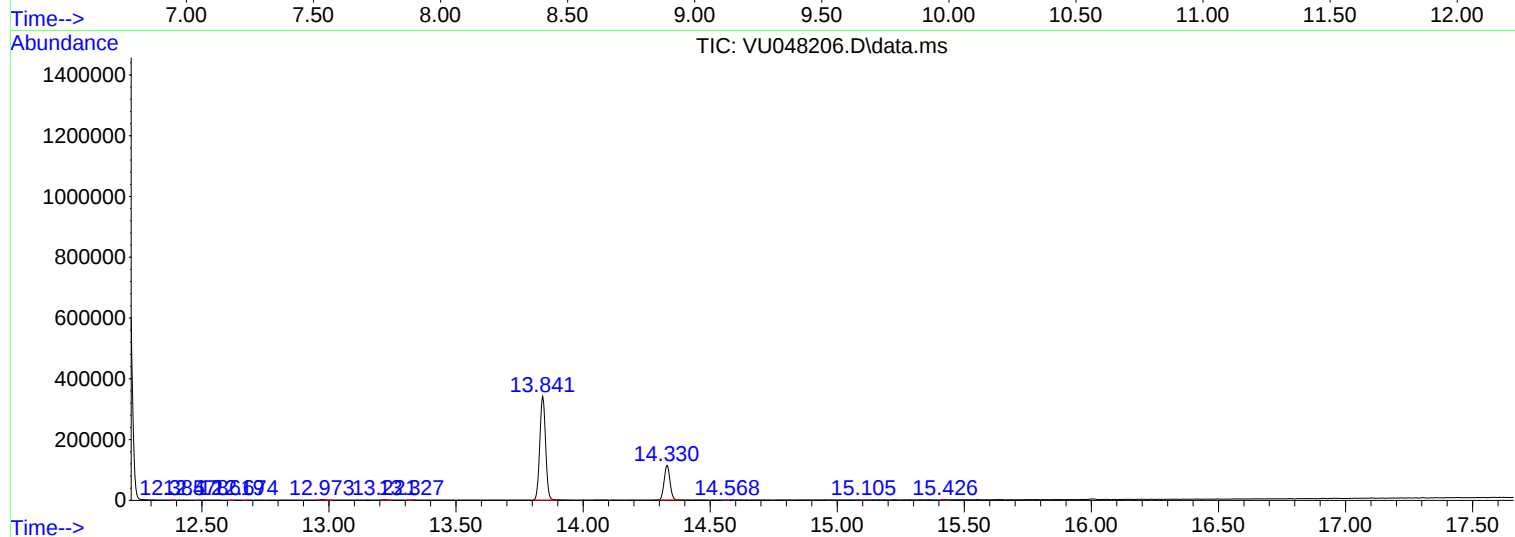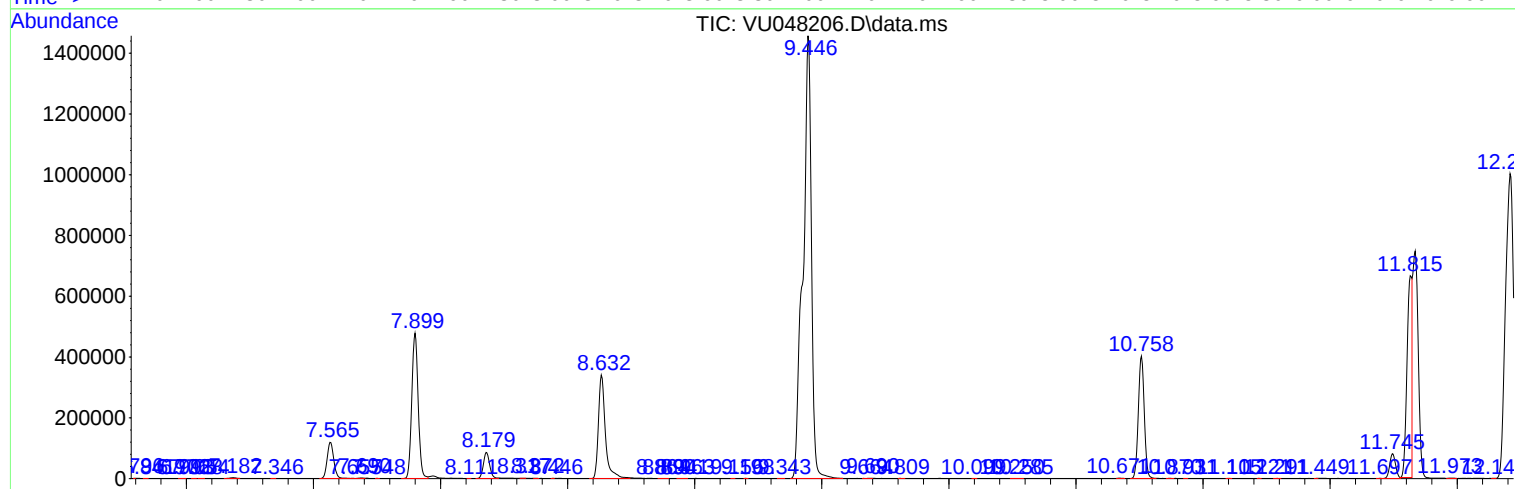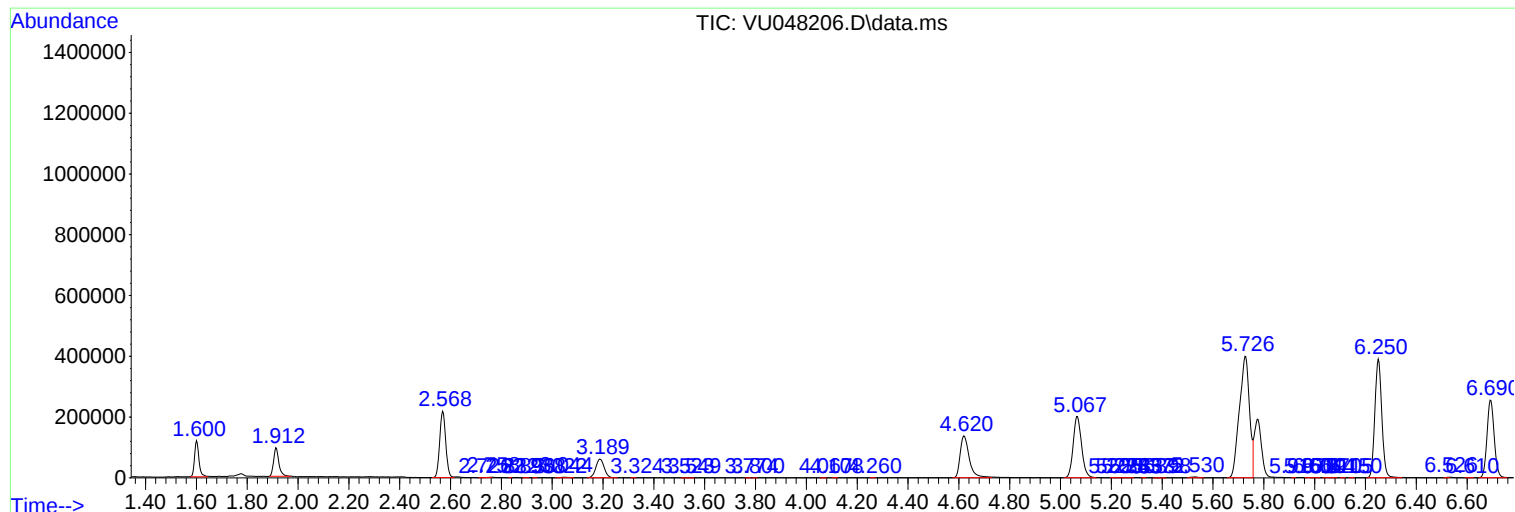

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048206.D
Acq On : 22 Apr 2022 05:58
Operator : SY/MD
Sample : N2488-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048206.D
Acq On : 22 Apr 2022 05:58
Operator : SY/MD
Sample : N2488-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc