

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048207.D
 Acq On : 22 Apr 2022 06:22
 Operator : SY/MD
 Sample : N2488-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	117523	136619	1.33%	0.444%
2	1.916	171	179	195	rVB	92202	131364	1.28%	0.427%
3	2.569	370	382	395	rBV	212532	350040	3.42%	1.137%
4	2.710	424	426	430	rBV2	482	383	0.00%	0.001%
5	2.832	460	464	467	rBV2	290	251	0.00%	0.001%
6	2.887	478	481	486	rBV2	427	264	0.00%	0.001%
7	3.048	523	531	543	rBV6	2099	4331	0.04%	0.014%
8	3.189	554	575	594	rBV	61842	143695	1.40%	0.467%
9	3.276	598	602	607	rVB3	477	451	0.00%	0.001%
10	3.298	607	609	610	rBV3	151	72	0.00%	0.000%
11	3.382	632	635	639	rBV2	310	197	0.00%	0.001%
12	3.504	671	673	675	rBV	179	102	0.00%	0.000%
13	3.533	679	682	684	rBV	209	121	0.00%	0.000%
14	3.559	689	690	692	rBV	119	56	0.00%	0.000%
15	3.617	704	708	710	rBV	254	176	0.00%	0.001%
16	3.694	729	732	733	rBV	209	137	0.00%	0.000%
17	3.716	737	739	744	rVB2	330	197	0.00%	0.001%
18	3.742	744	747	752	rVB2	171	185	0.00%	0.001%
19	3.781	756	759	761	rBV	258	160	0.00%	0.001%
20	3.823	770	772	776	rBV2	119	95	0.00%	0.000%
21	3.871	784	787	789	rBV	112	58	0.00%	0.000%
22	3.996	822	826	831	rBV2	282	279	0.00%	0.001%
23	4.080	850	852	855	rVB2	197	127	0.00%	0.000%
24	4.105	855	860	862	rBV2	267	295	0.00%	0.001%
25	4.215	890	894	897	rBV2	167	148	0.00%	0.000%
26	4.308	920	923	928	rBV2	195	195	0.00%	0.001%
27	4.421	957	958	960	rVB	168	63	0.00%	0.000%
28	4.523	984	990	991	rBV	825	629	0.01%	0.002%
29	4.620	1007	1020	1066	rBV	139793	350587	3.42%	1.138%
30	5.067	1142	1159	1185	rBV	199446	452662	4.42%	1.470%
31	5.183	1192	1195	1197	rBV3	281	143	0.00%	0.000%
32	5.292	1221	1229	1235	rBV3	715	909	0.01%	0.003%
33	5.334	1240	1242	1246	rVB2	208	138	0.00%	0.000%
34	5.353	1246	1248	1251	rBV	109	65	0.00%	0.000%
35	5.379	1251	1256	1258	rBV3	445	408	0.00%	0.001%
36	5.482	1284	1288	1291	rBV3	186	134	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048207.D
 Acq On : 22 Apr 2022 06:22
 Operator : SY/MD
 Sample : N2488-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.527	1291	1302	1317	rVB3	5719	12093	0.12%	0.039%
38	5.626	1330	1333	1336	rBV	172	128	0.00%	0.000%
39	5.729	1343	1365	1371	rBV2	394402	1062289	10.37%	3.449%
40	6.250	1513	1527	1548	rBV	396403	742557	7.25%	2.411%
41	6.408	1573	1576	1580	rBV	468	282	0.00%	0.001%
42	6.523	1608	1612	1616	rBV4	1442	1634	0.02%	0.005%
43	6.691	1650	1664	1685	rBV	252576	494318	4.83%	1.605%
44	6.810	1698	1701	1704	rBV	488	323	0.00%	0.001%
45	6.845	1710	1712	1716	rBV2	198	117	0.00%	0.000%
46	6.906	1728	1731	1734	rBV2	151	105	0.00%	0.000%
47	6.925	1735	1737	1739	rVV2	330	184	0.00%	0.001%
48	6.938	1740	1741	1744	rVB2	294	96	0.00%	0.000%
49	7.105	1791	1793	1795	rBV	123	69	0.00%	0.000%
50	7.182	1810	1817	1825	rBV4	2625	4042	0.04%	0.013%
51	7.301	1847	1854	1858	rBV	222	319	0.00%	0.001%
52	7.388	1879	1881	1885	rBV	183	119	0.00%	0.000%
53	7.404	1885	1886	1888	rVB	162	60	0.00%	0.000%
54	7.443	1896	1898	1900	rBV	139	90	0.00%	0.000%
55	7.565	1924	1936	1962	rBV	119865	212865	2.08%	0.691%
56	7.655	1962	1964	1967	rBV3	567	274	0.00%	0.001%
57	7.687	1969	1974	1983	rVB6	1468	2271	0.02%	0.007%
58	7.761	1996	1997	1999	rBV6	208	77	0.00%	0.000%
59	7.832	2017	2019	2021	rVB	531	185	0.00%	0.001%
60	7.900	2021	2040	2056	rBV	467191	812475	7.93%	2.638%
61	8.179	2116	2127	2144	rBV	82549	141627	1.38%	0.460%
62	8.507	2227	2229	2231	rBV2	131	54	0.00%	0.000%
63	8.578	2248	2251	2252	rBV2	188	93	0.00%	0.000%
64	8.633	2255	2268	2295	rBV	354582	666080	6.50%	2.163%
65	8.867	2340	2341	2344	rVB2	359	167	0.00%	0.001%
66	8.887	2344	2347	2348	rBV	231	157	0.00%	0.001%
67	9.067	2401	2403	2405	rBV2	275	148	0.00%	0.000%
68	9.170	2432	2435	2438	rBV2	200	157	0.00%	0.001%
69	9.231	2451	2454	2455	rBV2	234	140	0.00%	0.000%
70	9.256	2460	2462	2467	rVB	254	150	0.00%	0.000%
71	9.285	2467	2471	2473	rBV2	228	180	0.00%	0.001%
72	9.327	2481	2484	2486	rBV	218	107	0.00%	0.000%
73	9.340	2486	2488	2491	rVB2	189	79	0.00%	0.000%
74	9.446	2499	2521	2560	rBV	5631538	10241489	100.00%	33.256%
75	9.858	2648	2649	2653	rVB3	335	156	0.00%	0.001%
76	9.880	2653	2656	2658	rBV2	345	184	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048207.D
 Acq On : 22 Apr 2022 06:22
 Operator : SY/MD
 Sample : N2488-09 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.967	2681	2683	2687	rBV2	298	157	0.00%	0.001%
78	10.006	2694	2695	2702	rBV2	170	102	0.00%	0.000%
79	10.060	2708	2712	2714	rBV	242	178	0.00%	0.001%
80	10.096	2720	2723	2725	rBV	321	230	0.00%	0.001%
81	10.282	2779	2781	2782	rBV	218	101	0.00%	0.000%
82	10.324	2790	2794	2797	rBV2	301	260	0.00%	0.001%
83	10.475	2839	2841	2842	rBV	226	120	0.00%	0.000%
84	10.507	2848	2851	2857	rBV2	202	197	0.00%	0.001%
85	10.674	2895	2903	2909	rVB4	1238	1544	0.02%	0.005%
86	10.758	2916	2929	2949	rBV	384602	635866	6.21%	2.065%
87	10.870	2961	2964	2969	rBV3	437	450	0.00%	0.001%
88	11.070	3023	3026	3027	rBV	211	121	0.00%	0.000%
89	11.292	3092	3095	3096	rBV	136	69	0.00%	0.000%
90	11.301	3096	3098	3105	rBV3	385	491	0.00%	0.002%
91	11.620	3194	3197	3205	rVB2	343	361	0.00%	0.001%
92	11.652	3205	3207	3211	rVB	375	271	0.00%	0.001%
93	11.674	3211	3214	3217	rBV	386	324	0.00%	0.001%
94	11.745	3224	3236	3246	rBV	356658	565406	5.52%	1.836%
95	11.835	3247	3264	3288	rVB2	3288289	6052408	59.10%	19.653%
96	12.211	3363	3381	3402	rBV2	3348863	5953738	58.13%	19.333%
97	12.970	3610	3617	3628	rVB5	5904	9040	0.09%	0.029%
98	13.330	3721	3729	3737	rBV7	3088	4910	0.05%	0.016%
99	13.841	3875	3888	3917	rBV	792510	1253537	12.24%	4.070%
100	14.330	4028	4040	4057	rBV	211947	342133	3.34%	1.111%




Sum of corrected areas: 30795690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048207.D
Acq On : 22 Apr 2022 06:22
Operator : SY/MD
Sample : N2488-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

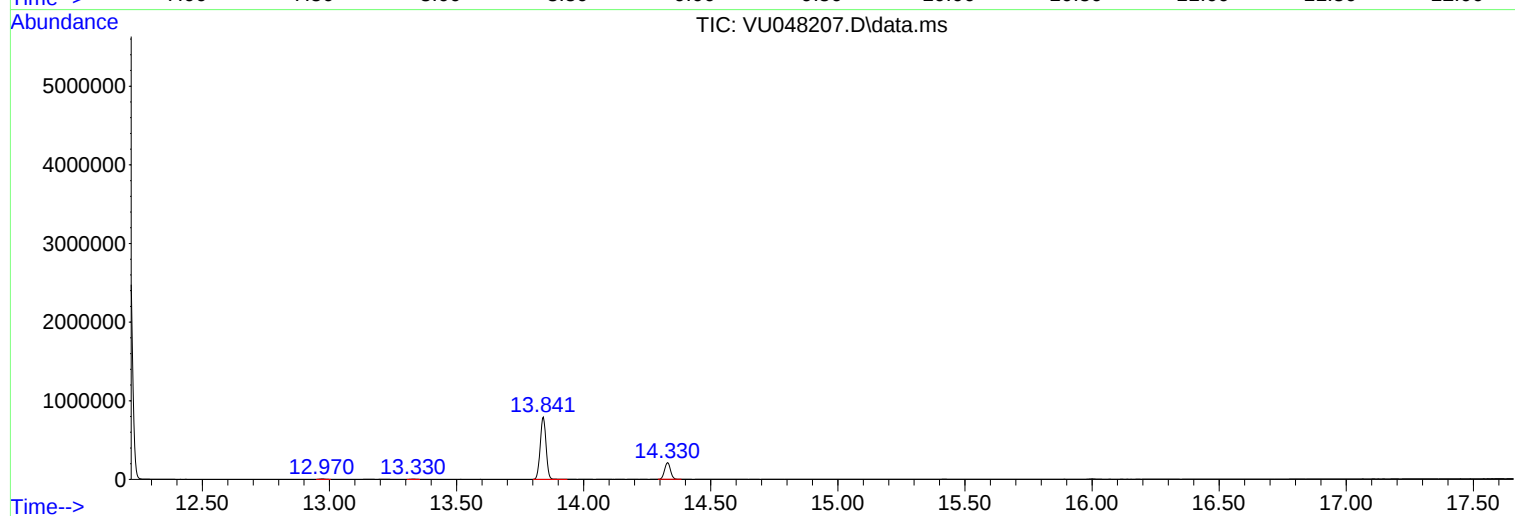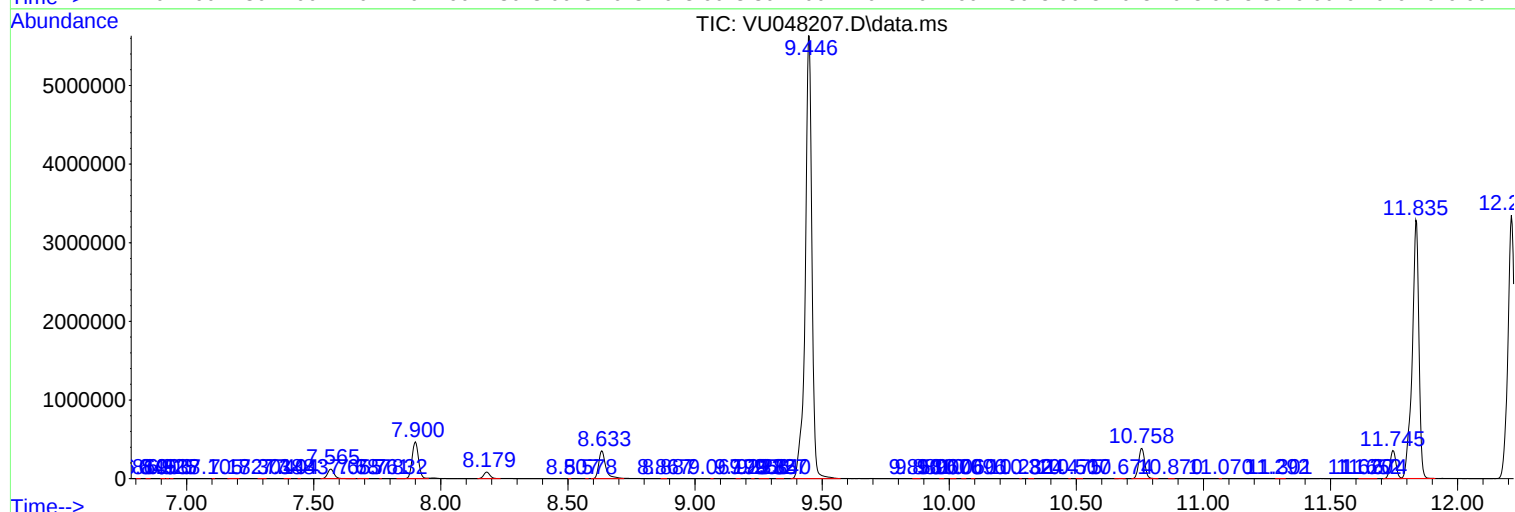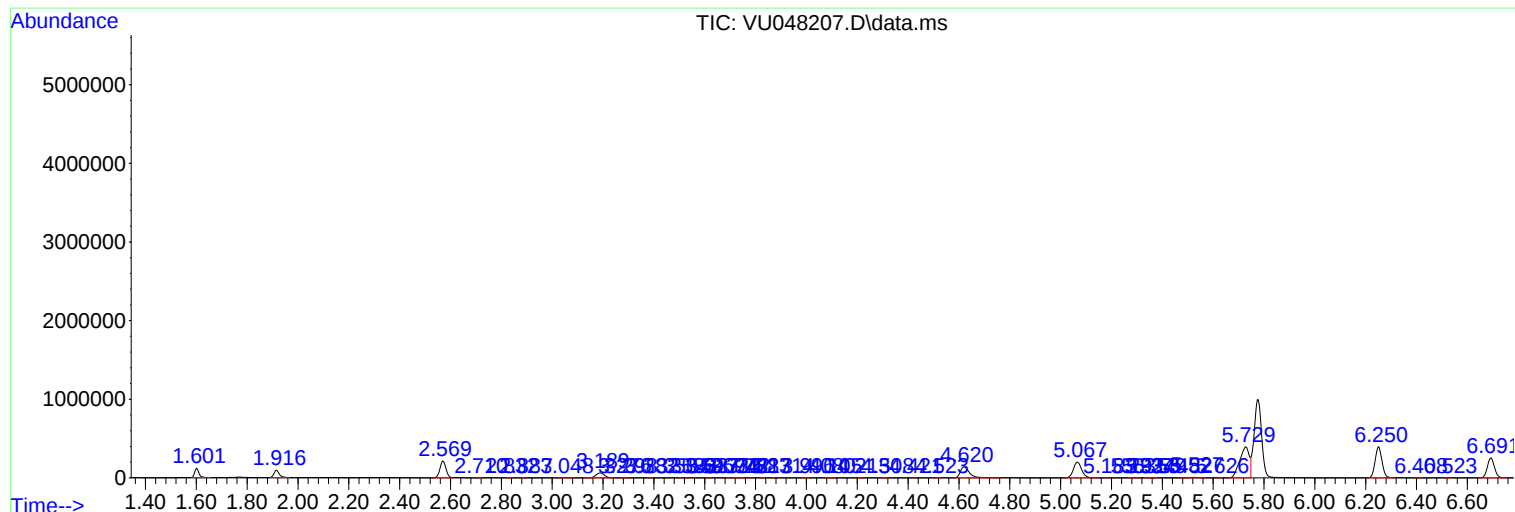

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048207.D
Acq On : 22 Apr 2022 06:22
Operator : SY/MD
Sample : N2488-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048207.D
Acq On : 22 Apr 2022 06:22
Operator : SY/MD
Sample : N2488-09 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------