

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048209.D
 Acq On : 22 Apr 2022 07:09
 Operator : SY/MD
 Sample : N2488-11 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rBV	116747	140574	6.87%	1.316%
2	1.912	170	178	199	rVB	98324	138690	6.78%	1.299%
3	2.568	369	382	397	rBV	216158	357474	17.47%	3.347%
4	2.826	460	462	467	rVB3	636	331	0.02%	0.003%
5	2.919	488	491	495	rBV2	318	285	0.01%	0.003%
6	2.999	513	516	520	rVB2	307	220	0.01%	0.002%
7	3.051	525	532	544	rVB6	1604	3065	0.15%	0.029%
8	3.102	544	548	551	rBV2	289	241	0.01%	0.002%
9	3.189	560	575	594	rVB	15173	36609	1.79%	0.343%
10	3.260	594	597	599	rBV	359	223	0.01%	0.002%
11	3.633	709	713	717	rBV2	353	347	0.02%	0.003%
12	3.951	809	812	819	rVB	382	345	0.02%	0.003%
13	4.089	849	855	857	rBV2	265	221	0.01%	0.002%
14	4.118	857	864	870	rBV2	203	380	0.02%	0.004%
15	4.498	973	982	984	rBV3	351	361	0.02%	0.003%
16	4.626	1008	1022	1050	rBV2	149604	390184	19.07%	3.653%
17	4.874	1097	1099	1106	rVB4	368	274	0.01%	0.003%
18	4.935	1115	1118	1128	rVB4	527	689	0.03%	0.006%
19	5.067	1141	1159	1184	rBV	204046	445713	21.79%	4.173%
20	5.292	1222	1229	1236	rBV3	501	669	0.03%	0.006%
21	5.520	1294	1300	1308	rBV3	390	574	0.03%	0.005%
22	5.565	1311	1314	1321	rVB2	251	235	0.01%	0.002%
23	5.726	1342	1364	1375	rBV2	402712	1115260	54.52%	10.442%
24	5.919	1420	1424	1430	rVB4	359	367	0.02%	0.003%
25	6.060	1463	1468	1471	rVV3	294	334	0.02%	0.003%
26	6.250	1512	1527	1547	rBV	369169	703950	34.41%	6.591%
27	6.485	1593	1600	1604	rVB2	350	531	0.03%	0.005%
28	6.526	1604	1613	1624	rBV4	1908	3578	0.17%	0.034%
29	6.584	1628	1631	1636	rVB2	238	209	0.01%	0.002%
30	6.610	1636	1639	1644	rBV2	414	309	0.02%	0.003%
31	6.690	1649	1664	1686	rVV	259891	506311	24.75%	4.741%
32	6.780	1689	1692	1695	rVV2	625	536	0.03%	0.005%
33	6.809	1695	1701	1709	rVB3	915	1446	0.07%	0.014%
34	7.121	1796	1798	1801	rVB2	360	196	0.01%	0.002%
35	7.189	1806	1819	1827	rBV3	2355	4214	0.21%	0.039%
36	7.247	1834	1837	1841	rVB	282	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048209.D
 Acq On : 22 Apr 2022 07:09
 Operator : SY/MD
 Sample : N2488-11 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.276	1841	1846	1850	rBV2	332	388	0.02%	0.004%
38	7.391	1878	1882	1887	rBV2	316	296	0.01%	0.003%
39	7.565	1924	1936	1952	rBV	118660	213117	10.42%	1.995%
40	7.694	1968	1976	1987	rVV5	1810	2936	0.14%	0.027%
41	7.790	2004	2006	2010	rVB2	348	214	0.01%	0.002%
42	7.899	2025	2040	2056	rBV	457060	803051	39.26%	7.519%
43	8.179	2114	2127	2141	rBV	84042	144060	7.04%	1.349%
44	8.385	2187	2191	2194	rBV3	307	274	0.01%	0.003%
45	8.462	2211	2215	2217	rBV2	439	331	0.02%	0.003%
46	8.501	2225	2227	2232	rVB2	239	196	0.01%	0.002%
47	8.558	2242	2245	2251	rVB3	228	221	0.01%	0.002%
48	8.636	2256	2269	2300	rBV	345131	662639	32.39%	6.204%
49	8.874	2341	2343	2348	rVB2	585	420	0.02%	0.004%
50	8.915	2353	2356	2361	rBV	587	506	0.02%	0.005%
51	8.986	2369	2378	2382	rBV2	440	650	0.03%	0.006%
52	9.005	2382	2384	2388	rVB2	484	285	0.01%	0.003%
53	9.054	2393	2399	2400	rBV2	275	203	0.01%	0.002%
54	9.214	2443	2449	2453	rBV	278	337	0.02%	0.003%
55	9.295	2469	2474	2476	rBV2	423	314	0.02%	0.003%
56	9.417	2495	2512	2517	rBV	560598	952730	46.57%	8.921%
57	9.578	2560	2562	2565	rVB2	470	194	0.01%	0.002%
58	9.600	2566	2569	2575	rVB2	297	261	0.01%	0.002%
59	9.690	2592	2597	2604	rVB2	719	904	0.04%	0.008%
60	9.767	2617	2621	2623	rBV	380	293	0.01%	0.003%
61	10.025	2697	2701	2708	rBV2	259	379	0.02%	0.004%
62	10.063	2710	2713	2716	rVV	322	214	0.01%	0.002%
63	10.108	2725	2727	2731	rVB2	473	292	0.01%	0.003%
64	10.263	2771	2775	2782	rVV2	311	403	0.02%	0.004%
65	10.320	2790	2793	2797	rVB3	334	278	0.01%	0.003%
66	10.346	2797	2801	2804	rBV2	313	216	0.01%	0.002%
67	10.369	2804	2808	2811	rVB2	257	213	0.01%	0.002%
68	10.388	2811	2814	2819	rBV2	345	390	0.02%	0.004%
69	10.671	2895	2902	2909	rVB5	1034	1289	0.06%	0.012%
70	10.758	2916	2929	2951	rBV	401995	651817	31.86%	6.103%
71	11.089	3028	3032	3035	rBV	292	240	0.01%	0.002%
72	11.140	3043	3048	3050	rBV2	372	340	0.02%	0.003%
73	11.234	3073	3077	3080	rVB3	273	210	0.01%	0.002%
74	11.253	3080	3083	3087	rBV2	244	198	0.01%	0.002%
75	11.401	3123	3129	3131	rBV2	291	257	0.01%	0.002%
76	11.452	3139	3145	3148	rBV3	460	587	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048209.D
 Acq On : 22 Apr 2022 07:09
 Operator : SY/MD
 Sample : N2488-11 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.587	3182	3187	3190	rBV3	377	371	0.02%	0.003%
78	11.645	3201	3205	3208	rBV	282	226	0.01%	0.002%
79	11.671	3208	3213	3216	rBV3	246	275	0.01%	0.003%
80	11.748	3226	3237	3245	rBV	41106	64970	3.18%	0.608%
81	11.816	3245	3258	3260	rBV	615499	869581	42.51%	8.142%
82	12.208	3361	3380	3401	rBV2	889534	2045704	100.00%	19.154%
83	12.327	3416	3417	3422	rVB2	601	238	0.01%	0.002%
84	12.362	3423	3428	3431	rBV3	787	803	0.04%	0.008%
85	12.465	3457	3460	3461	rBV	402	214	0.01%	0.002%
86	12.507	3469	3473	3475	rBV3	452	426	0.02%	0.004%
87	12.565	3487	3491	3495	rBV3	385	271	0.01%	0.003%
88	12.742	3542	3546	3550	rVB3	377	312	0.02%	0.003%
89	12.771	3550	3555	3559	rBV3	869	827	0.04%	0.008%
90	12.812	3565	3568	3570	rBV2	385	195	0.01%	0.002%
91	13.025	3630	3634	3639	rVV3	427	388	0.02%	0.004%
92	13.333	3727	3730	3733	rVB2	681	481	0.02%	0.005%
93	13.664	3829	3833	3837	rBV3	403	504	0.02%	0.005%
94	13.841	3876	3888	3906	rBV	205001	326793	15.97%	3.060%
95	14.176	3990	3992	3997	rVB2	431	299	0.01%	0.003%
96	14.330	4029	4040	4051	rBV3	42942	67157	3.28%	0.629%
97	14.815	4188	4191	4193	rBV	491	292	0.01%	0.003%
98	15.015	4251	4253	4257	rBV3	479	249	0.01%	0.002%
99	15.417	4369	4378	4379	rBV5	1273	1533	0.07%	0.014%
100	16.073	4578	4582	4584	rBV3	885	750	0.04%	0.007%




Sum of corrected areas: 10680174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048209.D
Acq On : 22 Apr 2022 07:09
Operator : SY/MD
Sample : N2488-11 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

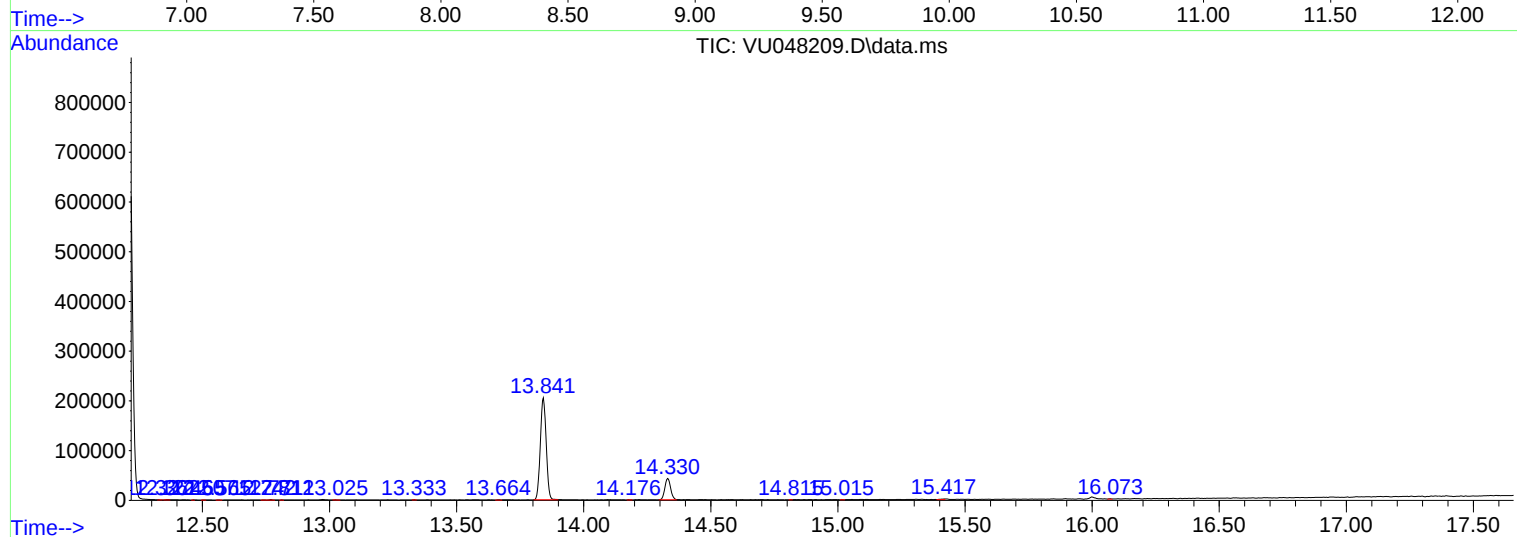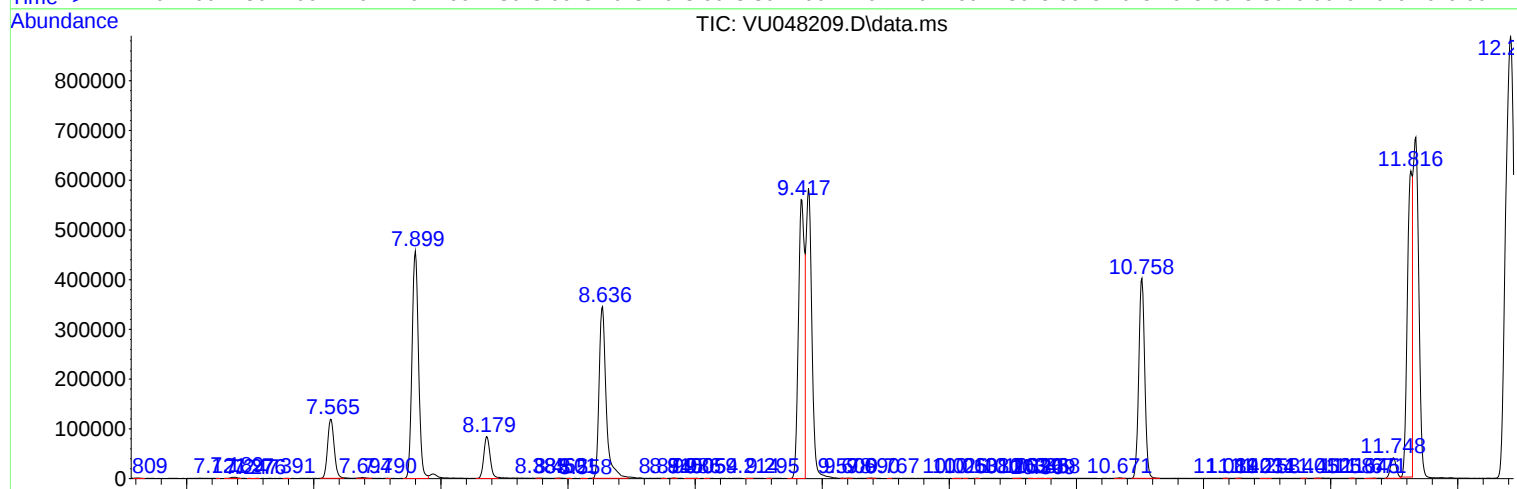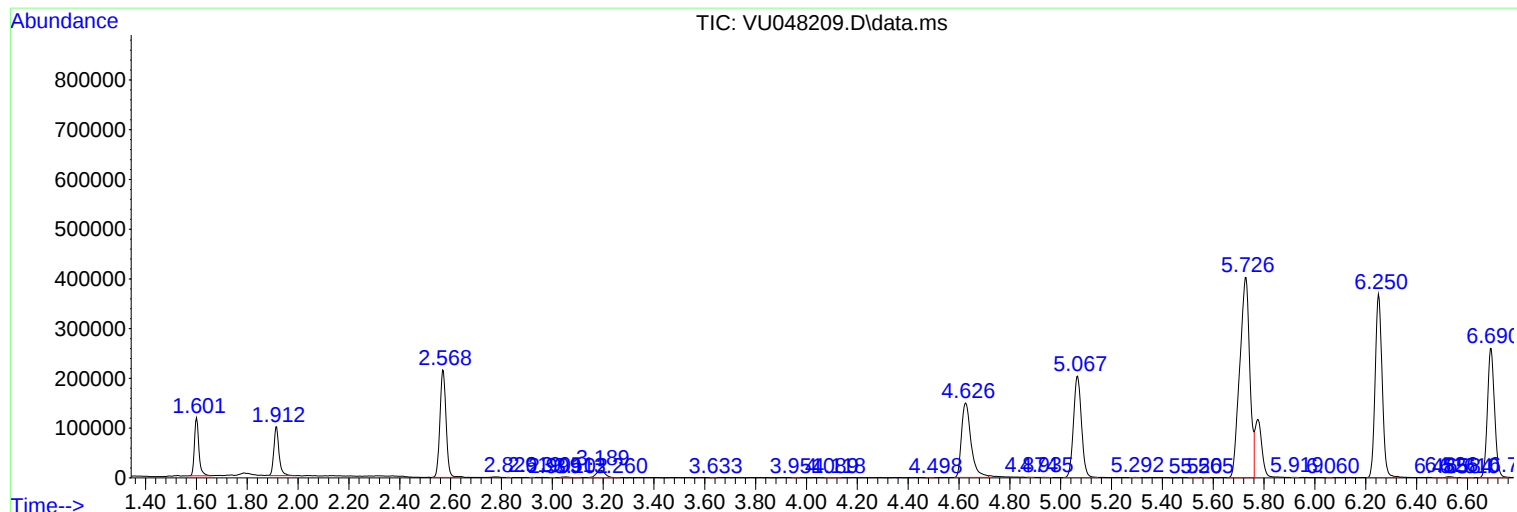

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048209.D
Acq On : 22 Apr 2022 07:09
Operator : SY/MD
Sample : N2488-11 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
Data File : VU048209.D
Acq On : 22 Apr 2022 07:09
Operator : SY/MD
Sample : N2488-11 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc