


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042122\
 Data File : VU048161.D
 Acq On : 21 Apr 2022 09:02
 Operator : SY/MD
 Sample : BFB069
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB069

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 25 01:24:32 2022

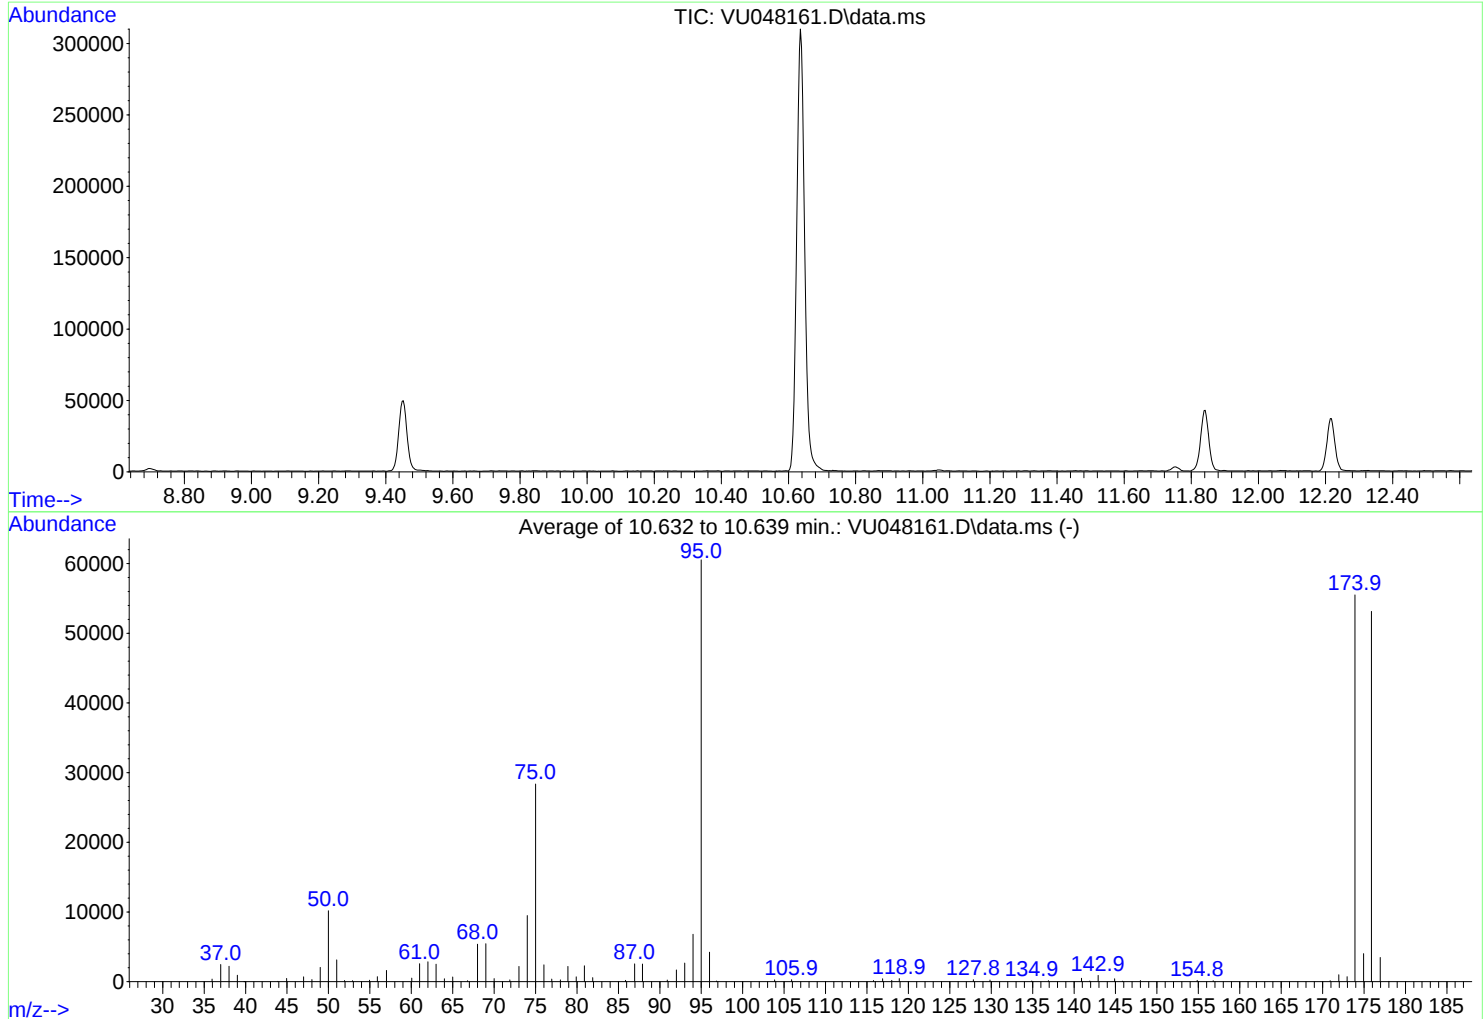

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	10168	PASS
75	95	30	80	46.8	28352	PASS
95	95	100	100	100.0	60541	PASS
96	95	5	9	7.0	4236	PASS
173	174	0.00	2	1.3	723	PASS
174	95	50	120	91.7	55507	PASS
175	174	5	9	7.2	4012	PASS
176	174	95	101	95.8	53149	PASS
177	176	5	9	6.5	3473	PASS

m/z	Abundance
39.80	214.0
43.90	568.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
36.00	399.0
37.00	2544.0
38.00	2182.0
39.00	902.0
39.80	236.0
43.90	681.0
45.00	439.0
47.00	691.0
48.00	311.0
49.00	1980.0
50.00	10297.0
51.00	2996.0
51.90	156.0
52.90	128.0
54.90	222.0
55.90	717.0
57.00	1617.0
60.00	532.0
61.00	2550.0
62.00	2914.0
63.00	2390.0
64.00	438.0
65.00	663.0
66.80	134.0
68.00	5113.0
69.00	5486.0
70.00	420.0
71.90	250.0
73.00	2324.0
74.00	9508.0
75.00	28184.0
76.00	2391.0
76.90	348.0
78.00	223.0
78.90	2198.0
79.90	679.0
80.90	2317.0
81.90	550.0
85.80	191.0
86.90	2425.0
87.90	2405.0
90.90	225.0
92.00	1581.0
93.00	2625.0
94.00	6800.0
95.00	59416.0
96.00	4214.0
103.90	232.0
105.90	268.0
115.80	160.0
116.90	399.0
118.00	202.0
118.90	405.0
127.90	283.0
129.90	230.0
134.90	148.0
136.90	105.0
140.90	449.0
141.90	124.0
142.90	852.0
145.00	423.0
148.00	164.0
154.90	156.0
156.80	150.0
170.90	163.0
172.00	875.0
172.90	719.0
173.90	53576.0
175.00	3953.0
175.90	51184.0
176.90	3307.0
178.00	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
36.00	355.0
37.00	2567.0
38.00	2286.0
39.00	962.0
39.90	206.0
43.90	577.0
45.00	485.0
47.00	723.0
48.00	296.0
49.00	2058.0
50.00	10519.0
51.00	3269.0
52.00	181.0
52.90	150.0
55.00	215.0
55.90	750.0
57.00	1712.0
60.10	518.0
61.00	2649.0
62.00	2963.0
63.00	2597.0
64.00	439.0
65.00	671.0
66.80	153.0
68.00	5505.0
69.00	5490.0
70.00	446.0
71.90	255.0
73.00	2220.0
74.00	9838.0
75.00	29160.0
76.00	2509.0
77.00	368.0
78.00	268.0
78.90	2246.0
79.90	723.0
80.90	2352.0
81.90	607.0
85.90	193.0
87.00	2641.0
87.90	2618.0
90.90	235.0
92.00	1718.0
93.00	2802.0
94.00	7062.0
95.00	62432.0
96.00	4399.0
96.80	133.0
103.90	259.0
105.90	281.0
115.80	172.0
116.90	445.0
118.00	176.0
118.90	461.0
127.90	285.0
129.80	223.0
134.90	111.0
136.90	124.0
140.90	511.0
141.90	128.0
142.90	920.0
144.90	410.0
145.90	107.0
148.00	171.0
154.80	194.0
156.80	158.0
170.90	143.0
172.00	1043.0
173.00	714.0
173.90	57048.0
174.90	4107.0
175.90	54832.0
176.90	3560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	356.0
37.00	2278.0
38.00	2136.0
39.00	869.0
39.90	214.0
43.90	568.0
44.90	464.0
47.00	633.0
48.00	256.0
49.00	2104.0
50.00	9687.0
51.00	3130.0
52.00	181.0
52.90	133.0
55.00	181.0
55.90	708.0
57.00	1502.0
60.00	472.0
61.00	2495.0
62.00	2684.0
63.00	2503.0
64.00	395.0
65.00	651.0
66.80	154.0
68.00	5502.0
69.00	5348.0
70.00	433.0
71.90	276.0
73.00	2034.0
74.00	9093.0
75.00	27712.0
76.00	2321.0
77.00	383.0
78.00	265.0
78.90	2130.0
79.90	674.0
80.90	2139.0
81.90	589.0
85.90	137.0
87.00	2565.0
87.90	2536.0
90.90	204.0
92.00	1729.0
93.00	2577.0
94.00	6532.0
95.00	59776.0
96.00	4094.0
96.90	167.0
103.80	261.0
105.90	257.0
115.80	182.0
116.90	430.0
118.00	149.0
118.90	419.0
127.80	265.0
129.80	216.0
136.90	159.0
140.90	524.0
142.90	906.0
144.80	386.0
145.80	122.0
148.00	132.0
154.80	191.0
156.80	118.0
170.90	130.0
171.90	1070.0
173.00	735.0
173.90	55896.0
174.90	3975.0
175.90	53432.0
177.00	3551.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069