


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042123\
Data File : VU053820.D
Acq On : 21 Apr 2023 09:03
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U041923DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Apr 21 09:18:21 2023

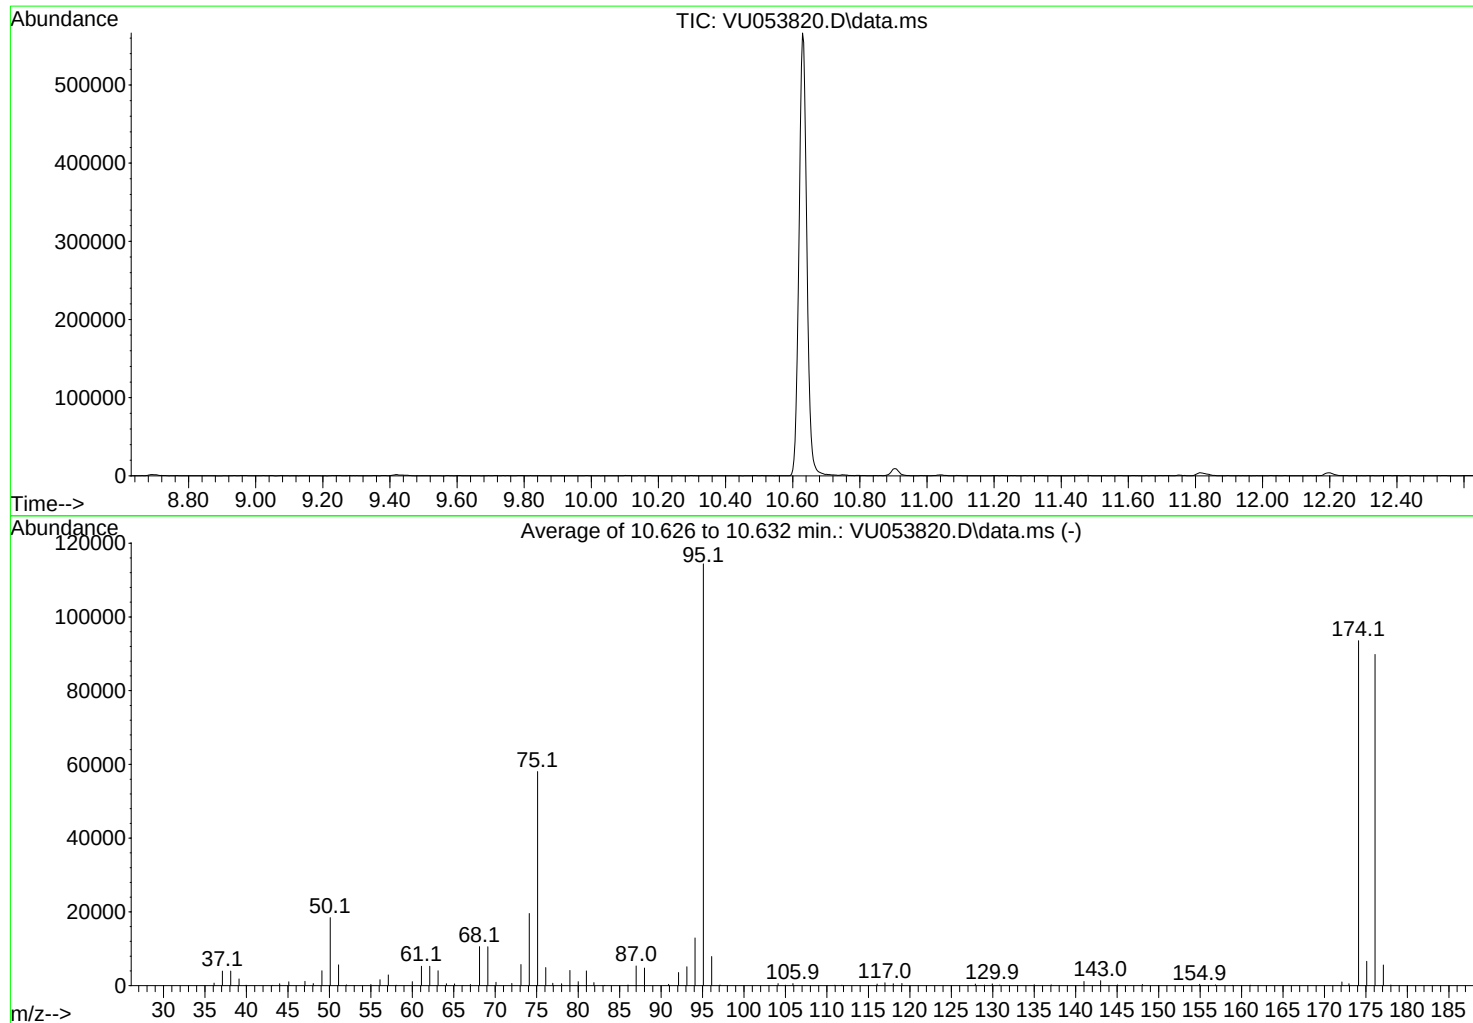

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	18445	PASS
75	95	30	60	50.7	58048	PASS
95	95	100	100	100.0	114395	PASS
96	95	5	9	6.9	7895	PASS
173	174	0.00	2	0.6	517	PASS
174	95	50	100	81.8	93563	PASS
175	174	5	9	7.1	6613	PASS
176	174	95	101	96.0	89840	PASS
177	176	5	9	6.2	5592	PASS