

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031392.D
 Acq On : 22 Apr 2019 14:31
 Operator : JC/SP
 Sample : K2428-15DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X16DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB2	15110	14043	0.76%	0.094%
2	1.283	55	60	66	rBV3	25846	27266	1.48%	0.182%
3	1.396	88	95	108	rVB	249947	269037	14.65%	1.799%
4	1.682	176	184	195	rBV	199453	251572	13.70%	1.682%
5	1.884	241	247	259	rVB2	29307	41520	2.26%	0.278%
6	2.270	356	367	381	rVB	416333	644723	35.11%	4.311%
7	2.450	419	423	425	rBV3	938	620	0.03%	0.004%
8	2.556	454	456	460	rVB2	679	381	0.02%	0.003%
9	2.666	487	490	494	rBV2	465	430	0.02%	0.003%
10	2.695	494	499	501	rBV4	1981	1746	0.10%	0.012%
11	2.826	536	540	543	rVB4	903	676	0.04%	0.005%
12	2.849	543	547	551	rBV4	615	597	0.03%	0.004%
13	3.183	647	651	658	rVB2	1143	1225	0.07%	0.008%
14	3.334	692	698	700	rBV2	811	695	0.04%	0.005%
15	3.360	704	706	711	rBV	695	465	0.03%	0.003%
16	3.428	721	727	732	rVB3	652	642	0.03%	0.004%
17	3.473	739	741	747	rVB3	648	525	0.03%	0.004%
18	3.553	764	766	772	rVB	847	770	0.04%	0.005%
19	3.797	837	842	844	rBV2	505	397	0.02%	0.003%
20	3.820	844	849	852	rBV2	681	631	0.03%	0.004%
21	4.013	906	909	912	rBV2	535	378	0.02%	0.003%
22	4.048	918	920	924	rVB	626	383	0.02%	0.003%
23	4.193	951	965	1009	rBV2	167974	586636	31.95%	3.922%
24	4.524	1066	1068	1070	rBV3	910	595	0.03%	0.004%
25	4.643	1089	1105	1131	rBV	298053	709054	38.61%	4.741%
26	4.945	1196	1199	1200	rBV2	753	424	0.02%	0.003%
27	5.045	1227	1230	1233	rBV2	586	580	0.03%	0.004%
28	5.151	1258	1263	1265	rBV2	631	599	0.03%	0.004%
29	5.334	1298	1320	1352	rBV2	599801	1836387	100.00%	12.278%
30	5.563	1389	1391	1396	rVB2	980	672	0.04%	0.004%
31	5.749	1446	1449	1453	rVB3	725	596	0.03%	0.004%
32	5.775	1454	1457	1468	rVB4	1416	1874	0.10%	0.013%
33	5.826	1471	1473	1477	rVB3	596	371	0.02%	0.002%
34	5.884	1477	1491	1522	rBV	704298	1450475	78.99%	9.698%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031392.D
 Acq On : 22 Apr 2019 14:31
 Operator : JC/SP
 Sample : K2428-15DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X16DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

35	6.183	1570	1584	1615	rBV	659168	1352887	73.67%	9.046%
36	6.328	1616	1629	1654	rVB	389259	804800	43.83%	5.381%
37	6.791	1768	1773	1782	rVB4	767	1035	0.06%	0.007%
38	6.891	1800	1804	1805	rBV	611	467	0.03%	0.003%
39	6.968	1825	1828	1831	rBV2	672	434	0.02%	0.003%
40	6.987	1831	1834	1838	rVB2	731	503	0.03%	0.003%
41	7.013	1838	1842	1851	rVB4	1025	1697	0.09%	0.011%
42	7.051	1851	1854	1859	rBV4	913	725	0.04%	0.005%
43	7.135	1876	1880	1886	rVB2	662	784	0.04%	0.005%
44	7.170	1886	1891	1896	rBV4	930	980	0.05%	0.007%
45	7.225	1896	1908	1935	rBV2	164617	318113	17.32%	2.127%
46	7.373	1949	1954	1955	rBV3	627	507	0.03%	0.003%
47	7.440	1973	1975	1980	rVB4	605	477	0.03%	0.003%
48	7.563	1999	2013	2044	rBV	600884	1103630	60.10%	7.379%
49	7.849	2092	2102	2124	rBV	108489	205796	11.21%	1.376%
50	8.042	2158	2162	2164	rBV2	587	451	0.02%	0.003%
51	8.116	2182	2185	2189	rBV2	1186	942	0.05%	0.006%
52	8.148	2189	2195	2196	rVV	902	777	0.04%	0.005%
53	8.177	2196	2204	2209	rVV3	2994	4195	0.23%	0.028%
54	8.225	2209	2219	2235	rVB2	84368	143348	7.81%	0.958%
55	8.312	2235	2246	2280	rBV	482470	909322	49.52%	6.080%
56	8.620	2340	2342	2345	rVB3	829	370	0.02%	0.002%
57	8.730	2373	2376	2380	rVB2	882	669	0.04%	0.004%
58	8.900	2423	2429	2432	rBV4	701	704	0.04%	0.005%
59	9.045	2467	2474	2475	rBV3	997	974	0.05%	0.007%
60	9.087	2475	2487	2523	rBV	776474	1338757	72.90%	8.951%
61	9.273	2541	2545	2551	rBV3	685	599	0.03%	0.004%
62	9.328	2559	2562	2565	rVB2	721	505	0.03%	0.003%
63	9.357	2565	2571	2572	rBV2	714	513	0.03%	0.003%
64	9.392	2576	2582	2585	rBV3	598	617	0.03%	0.004%
65	9.463	2602	2604	2608	rVB	932	529	0.03%	0.004%
66	9.495	2608	2614	2618	rBV5	792	749	0.04%	0.005%
67	9.556	2630	2633	2636	rVB2	772	417	0.02%	0.003%
68	9.636	2656	2658	2661	rBV	693	414	0.02%	0.003%
69	9.653	2661	2663	2668	rVB2	706	575	0.03%	0.004%
70	9.688	2668	2674	2675	rBV2	705	667	0.04%	0.004%
71	9.871	2727	2731	2734	rBV2	694	581	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031392.D
 Acq On : 22 Apr 2019 14:31
 Operator : JC/SP
 Sample : K2428-15DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X16DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

72	9.903	2739	2741	2745	rVV	853	570	0.03%	0.004%
73	9.926	2746	2748	2752	rVB2	755	496	0.03%	0.003%
74	9.980	2761	2765	2768	rBV4	715	601	0.03%	0.004%
75	10.087	2795	2798	2802	rBV	799	729	0.04%	0.005%
76	10.328	2871	2873	2876	rBV2	679	362	0.02%	0.002%
77	10.427	2891	2904	2923	rBV	480702	772802	42.08%	5.167%
78	10.607	2949	2960	2965	rBV4	2326	3699	0.20%	0.025%
79	10.672	2975	2980	2981	rBV2	629	622	0.03%	0.004%
80	10.707	2989	2991	2995	rBV2	539	384	0.02%	0.003%
81	11.177	3133	3137	3140	rBV	926	698	0.04%	0.005%
82	11.228	3151	3153	3157	rVB3	585	442	0.02%	0.003%
83	11.267	3162	3165	3169	rVV2	680	534	0.03%	0.004%
84	11.296	3170	3174	3178	rVB2	546	460	0.03%	0.003%
85	11.405	3204	3208	3211	rBV2	1070	742	0.04%	0.005%
86	11.479	3219	3231	3256	rBV	712889	1165243	63.45%	7.791%
87	11.855	3336	3348	3367	rBV	570429	949054	51.68%	6.346%
88	12.099	3422	3424	3431	rVV6	974	1039	0.06%	0.007%
89	12.353	3497	3503	3505	rBV3	873	795	0.04%	0.005%
90	12.476	3535	3541	3543	rBV4	1619	1885	0.10%	0.013%
91	12.601	3573	3580	3583	rBV3	698	984	0.05%	0.007%
92	12.659	3593	3598	3601	rBV4	831	930	0.05%	0.006%
93	12.771	3630	3633	3635	rBV2	749	424	0.02%	0.003%
94	12.922	3676	3680	3687	rVB4	986	1044	0.06%	0.007%
95	12.961	3687	3692	3695	rBV3	1115	976	0.05%	0.007%
96	13.247	3777	3781	3785	rBV2	654	719	0.04%	0.005%
97	13.620	3895	3897	3900	rVB2	1151	652	0.04%	0.004%
98	13.791	3946	3950	3954	rBV4	1505	1630	0.09%	0.011%
99	14.112	4047	4050	4052	rBV2	1081	602	0.03%	0.004%
100	14.430	4146	4149	4151	rBV2	1247	694	0.04%	0.005%


Sum of corrected areas: 14956307

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042219\
Data File : VU031392.D
Acq On : 22 Apr 2019 14:31
Operator : JC/SP
Sample : K2428-15DL 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X16DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

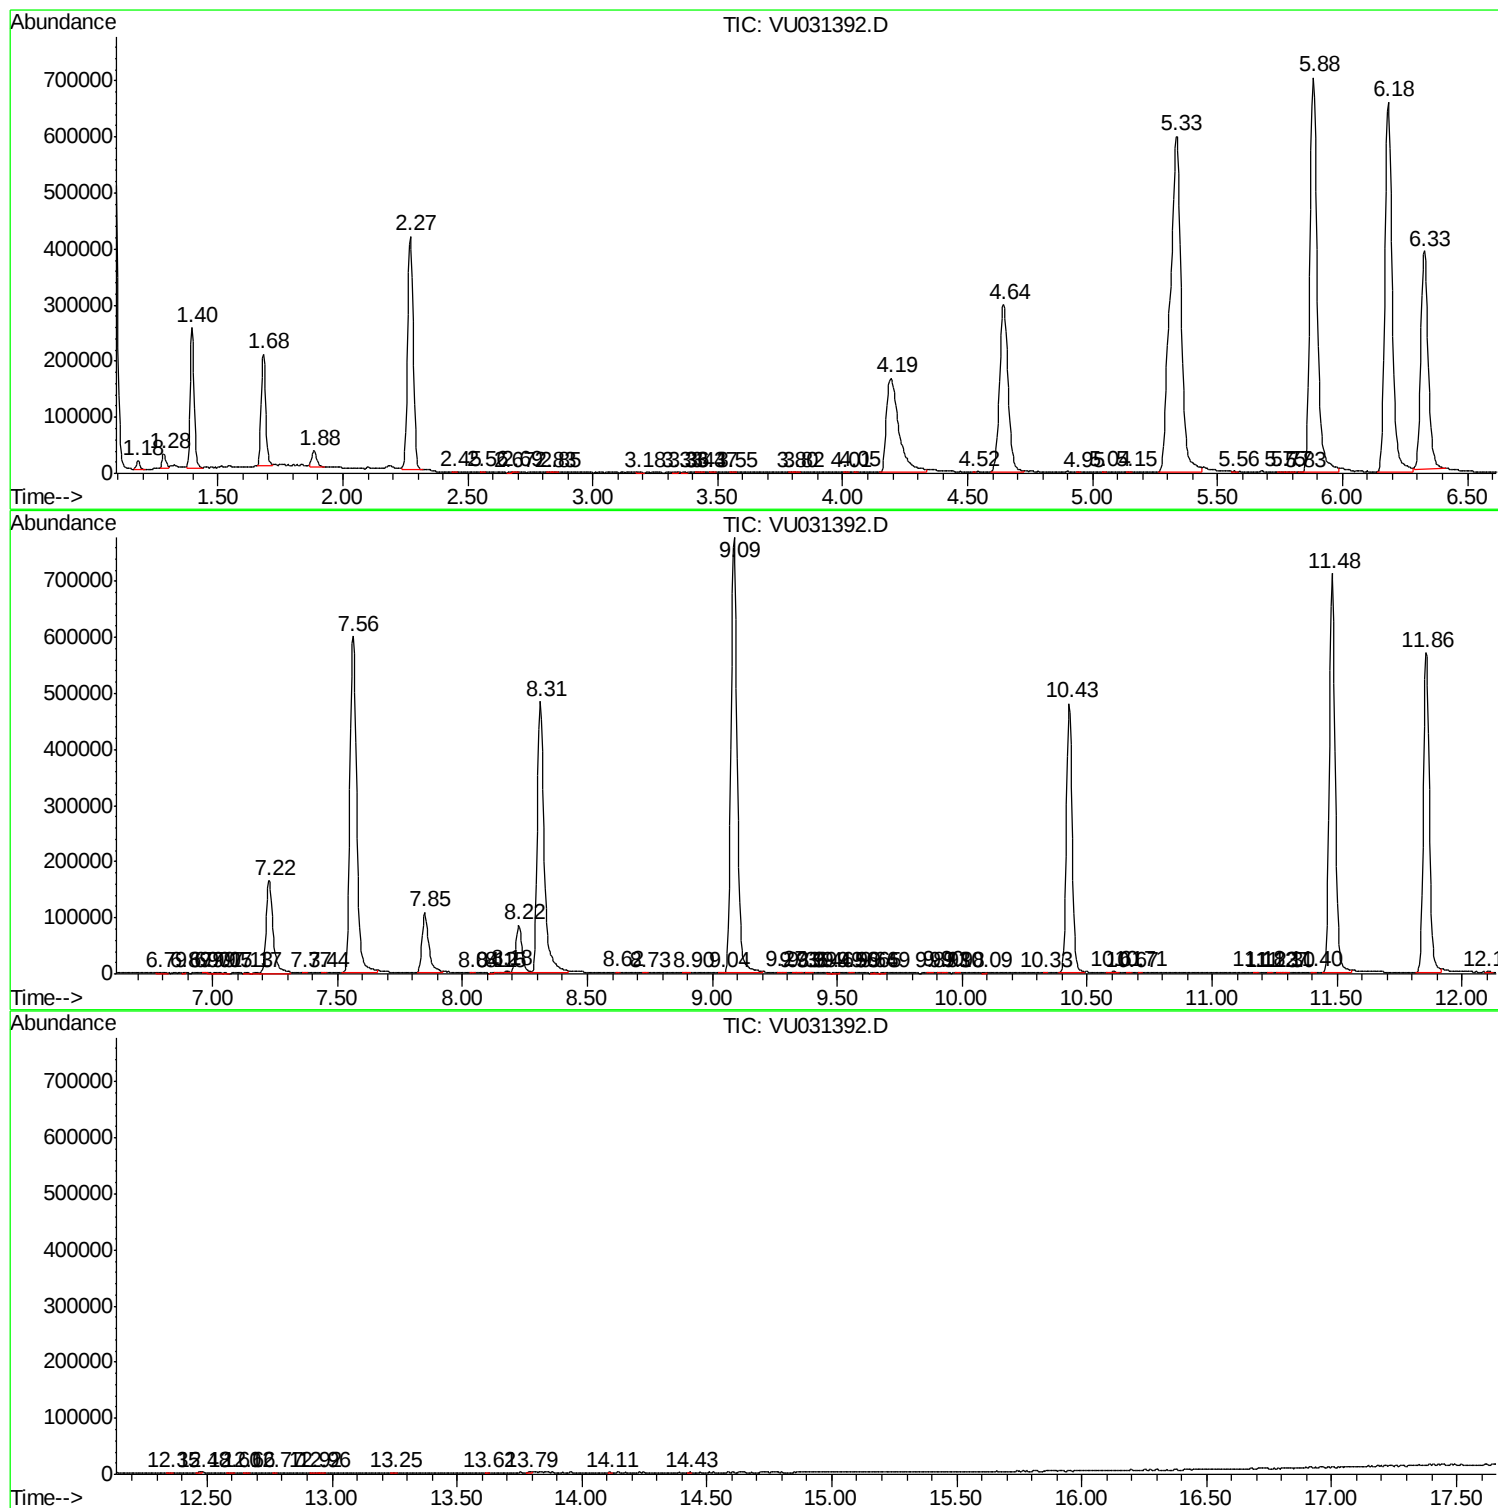

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031392.D
Acq On : 22 Apr 2019 14:31
Operator : JC/SP
Sample : K2428-15DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X16DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042219\
Data File : VU031392.D
Acq On : 22 Apr 2019 14:31
Operator : JC/SP
Sample : K2428-15DL 50X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0X16DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc