

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031393.D
 Acq On : 22 Apr 2019 14:54
 Operator : JC/SP
 Sample : K2403-22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5133

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rVB3	14599	14172	0.81%	0.098%
2	1.396	88	95	108	rVB	230453	241672	13.84%	1.663%
3	1.682	176	184	197	rBV	193995	244487	14.00%	1.683%
4	2.270	357	367	378	rBV	378833	571919	32.74%	3.937%
5	2.344	379	390	415	rVB	109920	287176	16.44%	1.977%
6	2.531	439	448	450	rBV6	4181	6431	0.37%	0.044%
7	2.701	492	501	510	rVB4	16132	28776	1.65%	0.198%
8	2.791	526	529	531	rBV2	983	607	0.03%	0.004%
9	2.817	534	537	540	rVV3	1777	1548	0.09%	0.011%
10	2.836	540	543	550	rVB5	1945	2478	0.14%	0.017%
11	2.907	562	565	568	rBV2	1085	561	0.03%	0.004%
12	2.990	587	591	598	rBV6	1280	1113	0.06%	0.008%
13	3.045	605	608	613	rVB2	711	552	0.03%	0.004%
14	3.103	620	626	632	rBV3	1199	1491	0.09%	0.010%
15	3.206	656	658	662	rVV3	1005	628	0.04%	0.004%
16	3.273	675	679	683	rBV3	797	894	0.05%	0.006%
17	3.531	756	759	762	rBV2	720	622	0.04%	0.004%
18	3.833	850	853	858	rVB3	683	576	0.03%	0.004%
19	4.090	929	933	937	rBV4	807	709	0.04%	0.005%
20	4.138	943	948	950	rBV	838	854	0.05%	0.006%
21	4.190	951	964	984	rBV	184473	576081	32.98%	3.965%
22	4.643	1089	1105	1139	rBV5	394816	998435	57.16%	6.872%
23	4.971	1201	1207	1210	rBV5	1177	1345	0.08%	0.009%
24	5.186	1271	1274	1278	rBV3	942	808	0.05%	0.006%
25	5.338	1297	1321	1355	rBV2	568273	1746631	100.00%	12.023%
26	5.637	1412	1414	1419	rVB2	897	600	0.03%	0.004%
27	5.666	1419	1423	1424	rBV3	1595	950	0.05%	0.007%
28	5.727	1440	1442	1446	rVB4	1181	599	0.03%	0.004%
29	5.884	1476	1491	1526	rBV	659427	1360488	77.89%	9.365%
30	6.186	1572	1585	1600	rBV7	31695	72065	4.13%	0.496%
31	6.270	1608	1611	1614	rBV4	1025	668	0.04%	0.005%
32	6.328	1615	1629	1651	rBV	377092	794907	45.51%	5.472%
33	6.630	1720	1723	1728	rBV5	951	885	0.05%	0.006%
34	6.730	1749	1754	1758	rBV3	616	692	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031393.D
 Acq On : 22 Apr 2019 14:54
 Operator : JC/SP
 Sample : K2403-22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5133

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

35	6.862	1793	1795	1798	rVB	1230	670	0.04%	0.005%
36	6.887	1798	1803	1807	rBV6	1267	1563	0.09%	0.011%
37	6.923	1811	1814	1818	rVB3	1042	708	0.04%	0.005%
38	7.048	1847	1853	1856	rVV6	516	703	0.04%	0.005%
39	7.064	1856	1858	1862	rVB2	1351	698	0.04%	0.005%
40	7.090	1862	1866	1871	rBV3	509	554	0.03%	0.004%
41	7.225	1895	1908	1930	rBV	199421	394363	22.58%	2.715%
42	7.421	1966	1969	1972	rBV3	1130	736	0.04%	0.005%
43	7.476	1976	1986	2000	rVB8	3961	8014	0.46%	0.055%
44	7.563	2000	2013	2042	rBV	703053	1288239	73.76%	8.867%
45	7.797	2083	2086	2090	rVB4	1197	770	0.04%	0.005%
46	7.849	2090	2102	2121	rBV	133141	249514	14.29%	1.717%
47	8.026	2155	2157	2160	rVB2	983	583	0.03%	0.004%
48	8.090	2175	2177	2180	rVB2	1152	678	0.04%	0.005%
49	8.174	2192	2203	2214	rBV2	23490	41610	2.38%	0.286%
50	8.222	2214	2218	2219	rBV3	2135	1506	0.09%	0.010%
51	8.309	2234	2245	2281	rBV	647569	1245345	71.30%	8.572%
52	8.473	2289	2296	2310	rVB6	16271	31085	1.78%	0.214%
53	8.604	2334	2337	2341	rBV5	1388	1248	0.07%	0.009%
54	8.636	2345	2347	2353	rVB5	1757	1541	0.09%	0.011%
55	8.736	2374	2378	2381	rBV2	933	687	0.04%	0.005%
56	8.804	2396	2399	2405	rVB3	948	905	0.05%	0.006%
57	8.845	2408	2412	2420	rBV5	1130	1152	0.07%	0.008%
58	8.881	2420	2423	2429	rBV5	899	880	0.05%	0.006%
59	9.087	2473	2487	2509	rBV	892719	1537345	88.02%	10.582%
60	9.373	2574	2576	2579	rBV3	968	620	0.04%	0.004%
61	9.392	2579	2582	2589	rVB5	964	1095	0.06%	0.008%
62	9.624	2649	2654	2657	rBV3	853	861	0.05%	0.006%
63	9.714	2675	2682	2685	rBV4	1096	1130	0.06%	0.008%
64	9.926	2744	2748	2751	rBV2	1035	763	0.04%	0.005%
65	9.977	2760	2764	2767	rVB3	987	718	0.04%	0.005%
66	10.003	2767	2772	2776	rBV2	754	656	0.04%	0.005%
67	10.042	2776	2784	2794	rBV10	2127	4354	0.25%	0.030%
68	10.128	2806	2811	2816	rVB2	1003	1029	0.06%	0.007%
69	10.164	2816	2822	2825	rBV3	946	1101	0.06%	0.008%
70	10.247	2840	2848	2852	rBV5	3333	5585	0.32%	0.038%
71	10.344	2873	2878	2884	rBV3	778	1045	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031393.D
 Acq On : 22 Apr 2019 14:54
 Operator : JC/SP
 Sample : K2403-22
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A5133

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

72	10.427	2891	2904	2927	rVV	463245	751429	43.02%	5.172%
73	10.601	2946	2958	2971	rVB2	19122	32700	1.87%	0.225%
74	10.961	3067	3070	3075	rVB3	1435	1216	0.07%	0.008%
75	10.997	3075	3081	3082	rBV	856	704	0.04%	0.005%
76	11.032	3088	3092	3097	rVB3	645	702	0.04%	0.005%
77	11.161	3127	3132	3136	rBV7	1809	2144	0.12%	0.015%
78	11.183	3137	3139	3142	rVV4	878	541	0.03%	0.004%
79	11.270	3163	3166	3170	rVB3	939	724	0.04%	0.005%
80	11.292	3170	3173	3177	rVB4	912	775	0.04%	0.005%
81	11.386	3194	3202	3203	rBV3	2396	2054	0.12%	0.014%
82	11.479	3219	3231	3255	rBV	630017	1028243	58.87%	7.078%
83	11.755	3308	3317	3333	rBV6	9811	25141	1.44%	0.173%
84	11.858	3337	3349	3377	rVV	515933	869884	49.80%	5.988%
85	11.955	3377	3379	3385	rVB5	1654	1062	0.06%	0.007%
86	12.160	3440	3443	3447	rBV4	1272	960	0.05%	0.007%
87	12.222	3458	3462	3464	rBV5	1410	1214	0.07%	0.008%
88	12.395	3513	3516	3519	rBV2	1319	799	0.05%	0.005%
89	12.469	3533	3539	3542	rBV5	4230	4659	0.27%	0.032%
90	12.951	3684	3689	3692	rBV4	1243	1164	0.07%	0.008%
91	12.974	3693	3696	3699	rVB3	1110	666	0.04%	0.005%
92	13.196	3761	3765	3766	rBV2	1018	718	0.04%	0.005%
93	13.382	3817	3823	3826	rBV5	1833	1699	0.10%	0.012%
94	13.540	3870	3872	3880	rVB5	993	1011	0.06%	0.007%
95	13.971	4003	4006	4010	rBV3	768	797	0.05%	0.005%
96	14.260	4093	4096	4099	rBV2	1321	865	0.05%	0.006%
97	14.627	4207	4210	4213	rBV3	1335	947	0.05%	0.007%
98	14.807	4264	4266	4270	rVB3	1285	739	0.04%	0.005%
99	14.829	4270	4273	4275	rBV2	1186	810	0.05%	0.006%
100	15.305	4417	4421	4425	rVB3	1405	1140	0.07%	0.008%


Sum of corrected areas: 14527981

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042219\
Data File : VU031393.D
Acq On : 22 Apr 2019 14:54
Operator : JC/SP
Sample : K2403-22
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5133

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

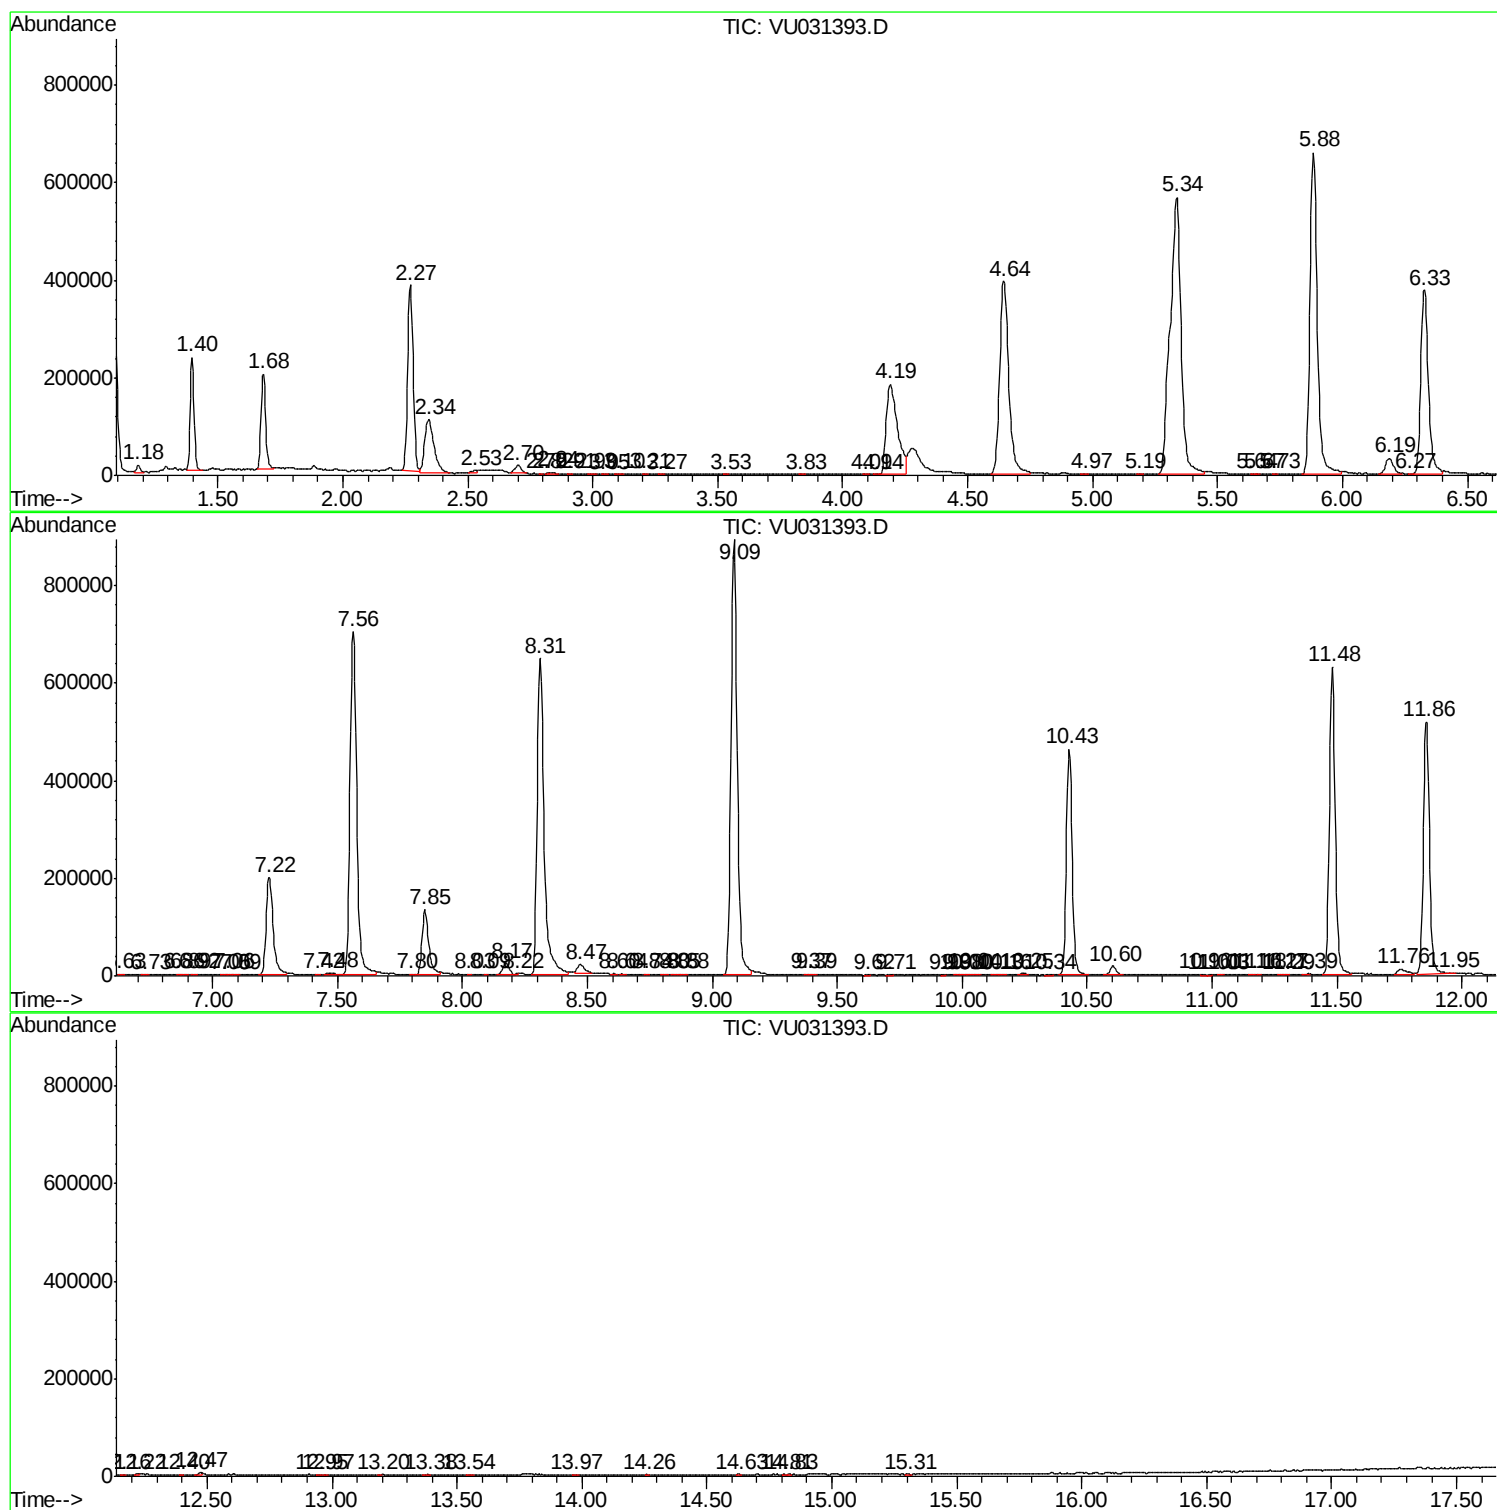

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031393.D
Acq On : 22 Apr 2019 14:54
Operator : JC/SP
Sample : K2403-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5133

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031393.D
Acq On : 22 Apr 2019 14:54
Operator : JC/SP
Sample : K2403-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A5133

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc