

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031394.D
 Acq On : 22 Apr 2019 15:17
 Operator : JC/SP
 Sample : K2428-13DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X13DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rBV	14404	15053	0.64%	0.092%
2	1.395	88	95	109	rVB	302804	325620	13.91%	1.989%
3	1.682	175	184	197	rBV	256160	330409	14.12%	2.018%
4	2.270	356	367	382	rBV	527502	811442	34.67%	4.957%
5	2.505	437	440	443	rBV3	851	587	0.03%	0.004%
6	2.543	450	452	457	rVB4	1275	845	0.04%	0.005%
7	2.691	495	498	501	rBV4	1715	1615	0.07%	0.010%
8	2.749	513	516	522	rVB3	1135	1032	0.04%	0.006%
9	3.051	606	610	617	rBV3	2277	2788	0.12%	0.017%
10	3.084	617	620	622	rBV2	728	533	0.02%	0.003%
11	3.257	670	674	677	rVB3	743	588	0.03%	0.004%
12	3.328	692	696	700	rBV4	612	640	0.03%	0.004%
13	3.411	720	722	725	rBV2	693	510	0.02%	0.003%
14	3.566	766	770	772	rBV2	1250	642	0.03%	0.004%
15	3.585	772	776	778	rBV	615	487	0.02%	0.003%
16	3.662	797	800	802	rBV	673	514	0.02%	0.003%
17	3.884	866	869	874	rBV3	763	761	0.03%	0.005%
18	3.961	888	893	895	rBV2	634	664	0.03%	0.004%
19	4.190	951	964	1009	rBV	202921	681427	29.11%	4.162%
20	4.646	1089	1106	1129	rBV2	388476	910716	38.91%	5.563%
21	4.791	1148	1151	1153	rBV3	1013	795	0.03%	0.005%
22	4.865	1171	1174	1176	rVB3	1034	593	0.03%	0.004%
23	4.929	1190	1194	1197	rBV3	1287	1088	0.05%	0.007%
24	4.984	1208	1211	1215	rVB3	1099	968	0.04%	0.006%
25	5.006	1215	1218	1223	rVB3	997	730	0.03%	0.004%
26	5.157	1262	1265	1267	rBV3	788	483	0.02%	0.003%
27	5.202	1276	1279	1281	rVB3	847	472	0.02%	0.003%
28	5.238	1282	1290	1294	rBV7	985	1401	0.06%	0.009%
29	5.337	1298	1321	1346	rBV2	784511	2340493	100.00%	14.297%
30	5.704	1433	1435	1440	rVB2	1548	1012	0.04%	0.006%
31	5.746	1440	1448	1451	rBV4	937	1083	0.05%	0.007%
32	5.813	1466	1469	1474	rBV2	714	557	0.02%	0.003%
33	5.884	1476	1491	1526	rBV	536153	1126598	48.14%	6.882%
34	6.103	1557	1559	1565	rVB3	845	801	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031394.D
 Acq On : 22 Apr 2019 15:17
 Operator : JC/SP
 Sample : K2428-13DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X13DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

35	6.183	1567	1584	1615	rBV	553610	1120984	47.90%	6.847%
36	6.328	1615	1629	1654	rVV	378612	783278	33.47%	4.785%
37	6.540	1693	1695	1698	rBV2	866	604	0.03%	0.004%
38	6.849	1788	1791	1795	rBV	558	491	0.02%	0.003%
39	6.923	1812	1814	1819	rVB3	894	701	0.03%	0.004%
40	6.955	1819	1824	1825	rBV2	699	600	0.03%	0.004%
41	7.038	1845	1850	1854	rBV3	931	818	0.03%	0.005%
42	7.106	1867	1871	1873	rBV3	629	486	0.02%	0.003%
43	7.157	1878	1887	1889	rBV3	422	641	0.03%	0.004%
44	7.225	1896	1908	1937	rBV	219506	420419	17.96%	2.568%
45	7.440	1969	1975	1978	rVB4	616	648	0.03%	0.004%
46	7.562	1995	2013	2040	rBV	786503	1424565	60.87%	8.702%
47	7.788	2079	2083	2086	rBV3	785	599	0.03%	0.004%
48	7.849	2091	2102	2121	rBV	140481	260012	11.11%	1.588%
49	8.000	2147	2149	2153	rVB4	826	516	0.02%	0.003%
50	8.083	2171	2175	2178	rBV2	686	558	0.02%	0.003%
51	8.141	2188	2193	2194	rBV2	720	566	0.02%	0.003%
52	8.170	2194	2202	2204	rBV4	3025	2935	0.13%	0.018%
53	8.228	2210	2220	2235	rBV3	22125	40168	1.72%	0.245%
54	8.312	2235	2246	2275	rBV	585377	1103506	47.15%	6.741%
55	8.775	2386	2390	2393	rBV2	698	551	0.02%	0.003%
56	8.794	2394	2396	2403	rVB4	664	617	0.03%	0.004%
57	8.852	2411	2414	2419	rVB3	793	682	0.03%	0.004%
58	8.877	2419	2422	2425	rBV2	916	757	0.03%	0.005%
59	8.929	2433	2438	2441	rBV2	673	505	0.02%	0.003%
60	8.958	2444	2447	2452	rVB2	765	519	0.02%	0.003%
61	9.086	2474	2487	2512	rBV	768628	1308280	55.90%	7.992%
62	9.315	2554	2558	2563	rVB5	889	839	0.04%	0.005%
63	9.337	2563	2565	2569	rBV3	754	592	0.03%	0.004%
64	9.357	2569	2571	2575	rVB5	1077	699	0.03%	0.004%
65	9.382	2575	2579	2582	rVB2	821	627	0.03%	0.004%
66	9.418	2583	2590	2592	rBV3	806	757	0.03%	0.005%
67	9.524	2621	2623	2629	rVB3	678	550	0.02%	0.003%
68	9.572	2633	2638	2642	rVV3	927	959	0.04%	0.006%
69	9.595	2642	2645	2650	rVB2	647	635	0.03%	0.004%
70	9.681	2669	2672	2675	rVV2	816	626	0.03%	0.004%
71	9.771	2695	2700	2703	rBV3	554	666	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031394.D
 Acq On : 22 Apr 2019 15:17
 Operator : JC/SP
 Sample : K2428-13DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X13DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

72	10.183	2824	2828	2833	rVB4	773	654	0.03%	0.004%
73	10.212	2833	2837	2843	rBV	459	547	0.02%	0.003%
74	10.427	2891	2904	2925	rBV	573007	926886	39.60%	5.662%
75	10.601	2953	2958	2971	rVB5	3043	5186	0.22%	0.032%
76	10.694	2982	2987	2993	rBV4	909	1163	0.05%	0.007%
77	10.787	3011	3016	3021	rVB3	621	849	0.04%	0.005%
78	10.826	3026	3028	3033	rVB2	709	533	0.02%	0.003%
79	10.961	3067	3070	3074	rVB2	835	504	0.02%	0.003%
80	10.993	3077	3080	3087	rVB3	702	707	0.03%	0.004%
81	11.054	3097	3099	3104	rVB2	884	668	0.03%	0.004%
82	11.083	3104	3108	3112	rBV3	952	866	0.04%	0.005%
83	11.225	3147	3152	3156	rBV2	1040	1194	0.05%	0.007%
84	11.273	3162	3167	3172	rBV2	949	1054	0.05%	0.006%
85	11.337	3184	3187	3192	rBV2	913	699	0.03%	0.004%
86	11.479	3220	3231	3251	rBV	702737	1156325	49.41%	7.063%
87	11.639	3279	3281	3286	rBV4	1077	983	0.04%	0.006%
88	11.858	3334	3349	3374	rBV	705471	1217002	52.00%	7.434%
89	12.106	3424	3426	3429	rBV2	933	547	0.02%	0.003%
90	12.173	3443	3447	3449	rBV3	931	758	0.03%	0.005%
91	12.373	3507	3509	3515	rVB3	1083	968	0.04%	0.006%
92	12.565	3565	3569	3572	rVB4	568	480	0.02%	0.003%
93	12.588	3572	3576	3579	rBV2	1013	668	0.03%	0.004%
94	12.868	3660	3663	3666	rBV	908	677	0.03%	0.004%
95	13.572	3878	3882	3885	rBV	1256	971	0.04%	0.006%
96	13.778	3941	3946	3947	rBV	918	755	0.03%	0.005%
97	14.247	4089	4092	4096	rBV3	1003	779	0.03%	0.005%
98	14.572	4191	4193	4197	rBV2	882	622	0.03%	0.004%
99	14.745	4244	4247	4251	rBV2	1290	964	0.04%	0.006%
100	14.893	4290	4293	4297	rBV3	995	857	0.04%	0.005%


Sum of corrected areas: 16370769

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042219\
Data File : VU031394.D
Acq On : 22 Apr 2019 15:17
Operator : JC/SP
Sample : K2428-13DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X13DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

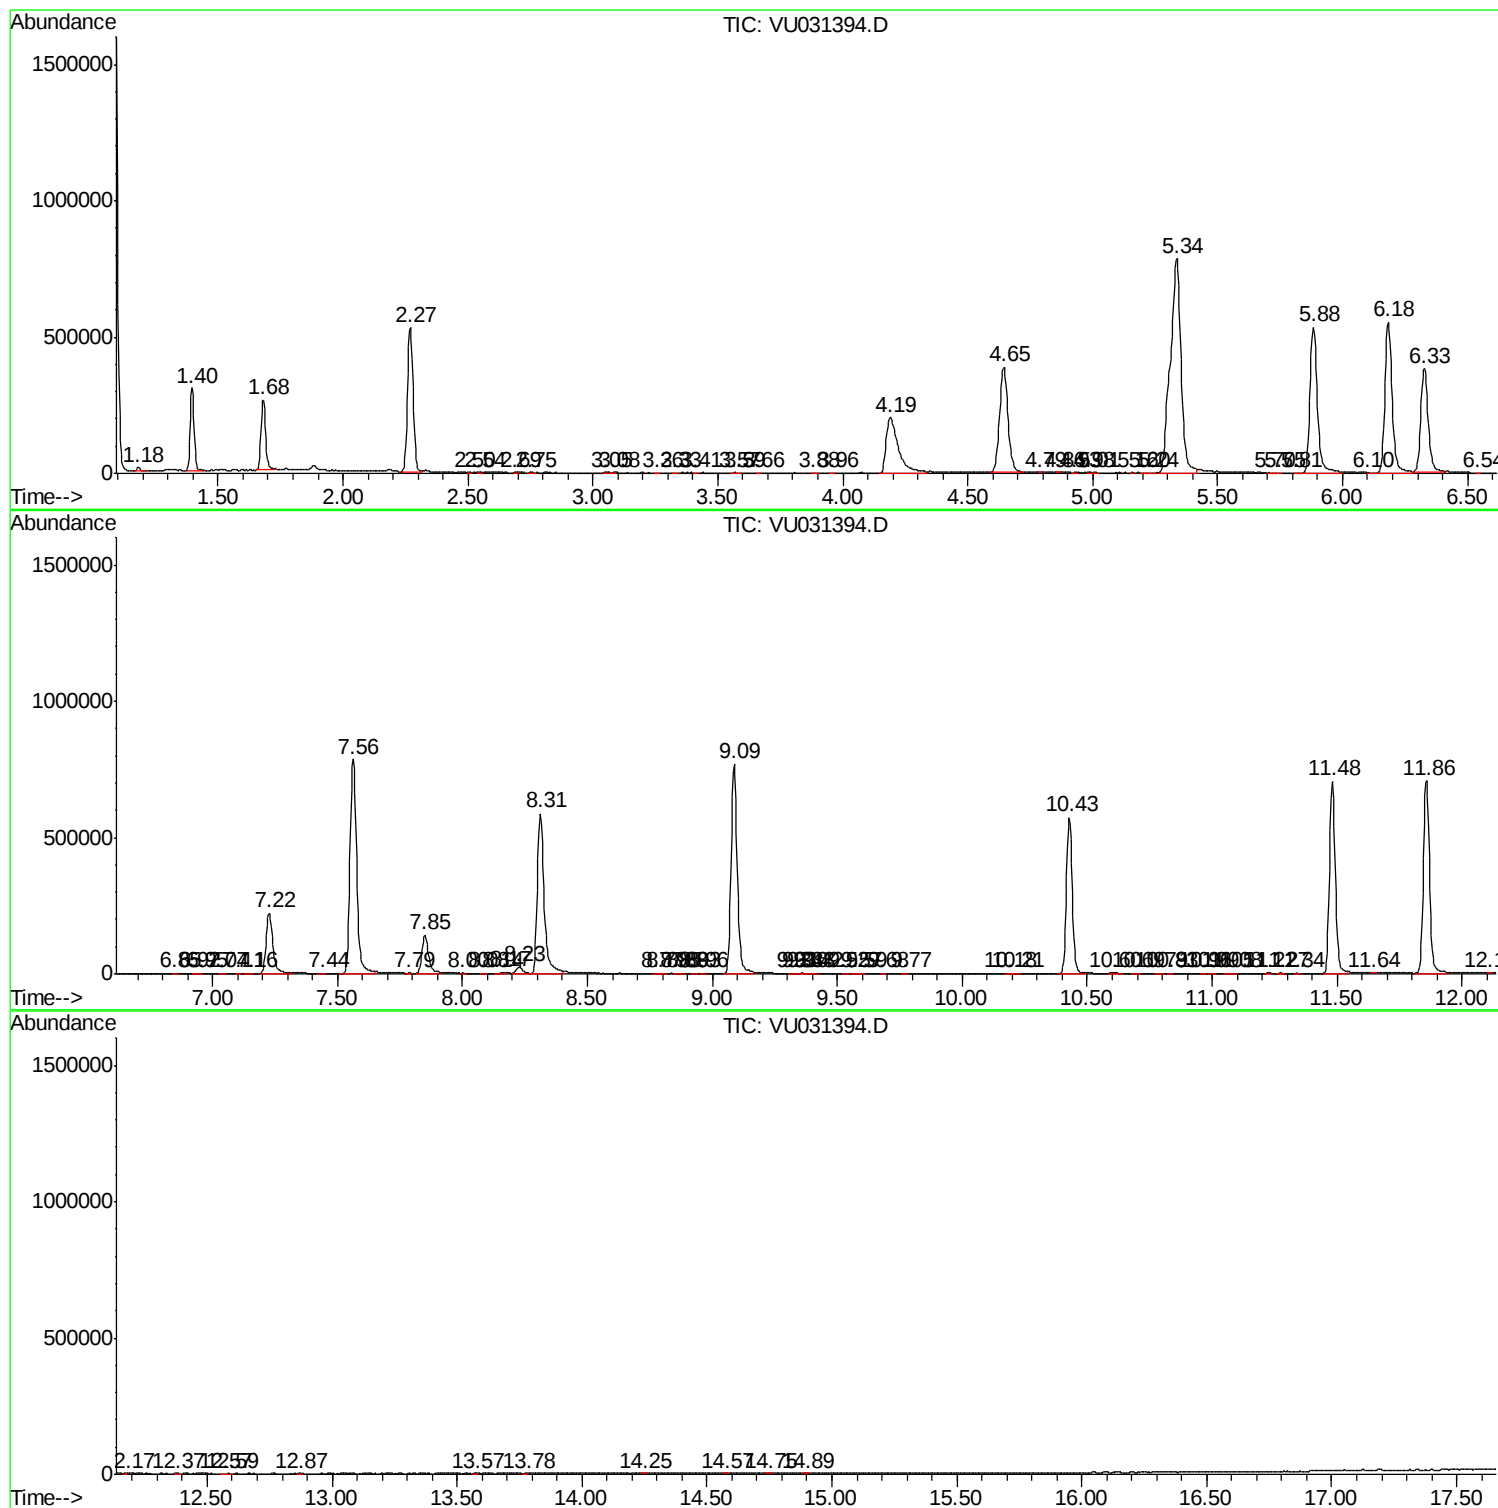

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031394.D
Acq On : 22 Apr 2019 15:17
Operator : JC/SP
Sample : K2428-13DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X13DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031394.D
Acq On : 22 Apr 2019 15:17
Operator : JC/SP
Sample : K2428-13DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X13DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc