

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031395.D
 Acq On : 22 Apr 2019 15:39
 Operator : JC/SP
 Sample : K2428-14DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X14DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rBV2	13483	13053	0.55%	0.068%
2	1.396	88	95	108	rVB	304940	331095	13.95%	1.724%
3	1.682	176	184	197	rBV	261426	335465	14.14%	1.747%
4	1.881	241	246	254	rVB5	14408	18283	0.77%	0.095%
5	2.270	356	367	381	rVB	539694	821618	34.63%	4.278%
6	2.547	450	453	454	rBV3	1222	570	0.02%	0.003%
7	2.617	472	475	477	rBV4	1103	862	0.04%	0.004%
8	2.701	490	501	503	rBV5	2600	3673	0.15%	0.019%
9	2.775	520	524	527	rVB4	929	631	0.03%	0.003%
10	2.797	527	531	537	rBV5	784	650	0.03%	0.003%
11	2.913	563	567	570	rBV3	717	501	0.02%	0.003%
12	3.039	602	606	611	rVB3	760	686	0.03%	0.004%
13	3.122	628	632	635	rBV	958	891	0.04%	0.005%
14	3.138	635	637	642	rVB2	1068	721	0.03%	0.004%
15	3.441	728	731	734	rBV2	901	575	0.02%	0.003%
16	3.714	811	816	818	rBV2	675	491	0.02%	0.003%
17	3.765	827	832	835	rBV2	752	773	0.03%	0.004%
18	4.103	933	937	940	rBV2	627	500	0.02%	0.003%
19	4.138	945	948	950	rBV2	741	505	0.02%	0.003%
20	4.190	951	964	1006	rBV	212139	680680	28.69%	3.544%
21	4.643	1089	1105	1130	rBV	389130	915947	38.60%	4.769%
22	4.871	1174	1176	1182	rBV3	1004	1205	0.05%	0.006%
23	4.942	1193	1198	1200	rBV2	618	525	0.02%	0.003%
24	4.987	1206	1212	1213	rBV4	1158	1109	0.05%	0.006%
25	5.244	1289	1292	1297	rBV2	1218	1351	0.06%	0.007%
26	5.338	1297	1321	1350	rBV2	789575	2372821	100.00%	12.354%
27	5.746	1444	1448	1450	rBV2	909	754	0.03%	0.004%
28	5.884	1477	1491	1515	rBV	705023	1449252	61.08%	7.546%
29	6.112	1557	1562	1565	rBV5	1364	1179	0.05%	0.006%
30	6.183	1570	1584	1615	rBV	886375	1786485	75.29%	9.301%
31	6.328	1616	1629	1650	rVV	510177	1036026	43.66%	5.394%
32	6.534	1691	1693	1697	rVV5	886	498	0.02%	0.003%
33	6.601	1712	1714	1719	rVB3	1060	663	0.03%	0.003%
34	6.653	1723	1730	1732	rVV4	781	955	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031395.D
 Acq On : 22 Apr 2019 15:39
 Operator : JC/SP
 Sample : K2428-14DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X14DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

35	6.688	1736	1741	1746	rVB5	1524	1699	0.07%	0.009%
36	6.727	1746	1753	1756	rBV5	1436	1804	0.08%	0.009%
37	6.768	1761	1766	1770	rBV4	799	952	0.04%	0.005%
38	6.852	1789	1792	1794	rVV2	947	677	0.03%	0.004%
39	6.900	1805	1807	1810	rVV	718	506	0.02%	0.003%
40	6.929	1814	1816	1821	rVV2	707	597	0.03%	0.003%
41	6.971	1827	1829	1833	rVB3	1250	743	0.03%	0.004%
42	7.022	1843	1845	1848	rBV3	864	543	0.02%	0.003%
43	7.141	1879	1882	1884	rBV2	770	489	0.02%	0.003%
44	7.170	1887	1891	1895	rBV3	791	567	0.02%	0.003%
45	7.225	1895	1908	1936	rBV	285251	547482	23.07%	2.850%
46	7.563	2000	2013	2055	rBV	1016363	1871899	78.89%	9.746%
47	7.849	2091	2102	2125	rBV	184490	344303	14.51%	1.793%
48	8.061	2165	2168	2174	rBV5	1433	1569	0.07%	0.008%
49	8.225	2209	2219	2235	rBV2	42508	78152	3.29%	0.407%
50	8.312	2235	2246	2282	rBV	787437	1513446	63.78%	7.880%
51	8.749	2379	2382	2386	rBV3	964	751	0.03%	0.004%
52	8.836	2407	2409	2413	rVB3	1071	716	0.03%	0.004%
53	8.871	2418	2420	2424	rBV2	605	496	0.02%	0.003%
54	8.964	2445	2449	2452	rVV3	616	672	0.03%	0.003%
55	9.026	2464	2468	2469	rBV3	1216	766	0.03%	0.004%
56	9.087	2471	2487	2521	rBV	981830	1714752	72.27%	8.928%
57	9.411	2585	2588	2590	rBV3	1443	956	0.04%	0.005%
58	9.463	2600	2604	2607	rBV4	701	613	0.03%	0.003%
59	9.669	2665	2668	2673	rVB2	687	760	0.03%	0.004%
60	9.788	2700	2705	2708	rVB2	910	881	0.04%	0.005%
61	9.849	2720	2724	2729	rVB2	1060	916	0.04%	0.005%
62	9.878	2729	2733	2735	rBV2	1048	884	0.04%	0.005%
63	10.141	2810	2815	2820	rBV2	692	683	0.03%	0.004%
64	10.273	2852	2856	2862	rVB3	939	935	0.04%	0.005%
65	10.312	2863	2868	2871	rVB3	753	681	0.03%	0.004%
66	10.331	2871	2874	2879	rVB3	637	525	0.02%	0.003%
67	10.427	2889	2904	2924	rBV	583736	938462	39.55%	4.886%
68	10.604	2952	2959	2963	rVV4	1756	2276	0.10%	0.012%
69	10.640	2967	2970	2974	rVV2	849	705	0.03%	0.004%
70	10.659	2974	2976	2980	rVV3	748	511	0.02%	0.003%
71	10.678	2980	2982	2986	rVV3	887	529	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042219\
 Data File : VU031395.D
 Acq On : 22 Apr 2019 15:39
 Operator : JC/SP
 Sample : K2428-14DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X14DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

72	10.704	2986	2990	2995	rVB3	678	720	0.03%	0.004%
73	10.800	3014	3020	3023	rBV2	727	589	0.02%	0.003%
74	10.826	3023	3028	3031	rBV	657	557	0.02%	0.003%
75	10.974	3071	3074	3078	rVB2	689	505	0.02%	0.003%
76	11.090	3107	3110	3114	rVB2	710	505	0.02%	0.003%
77	11.122	3114	3120	3123	rBV2	1080	898	0.04%	0.005%
78	11.479	3219	3231	3262	rBV	716254	1164920	49.09%	6.065%
79	11.669	3288	3290	3296	rVB5	944	743	0.03%	0.004%
80	11.855	3335	3348	3366	rBV	733716	1206698	50.85%	6.283%
81	12.144	3435	3438	3443	rBV4	1092	887	0.04%	0.005%
82	12.302	3483	3487	3491	rBV4	1173	1074	0.05%	0.006%
83	12.369	3502	3508	3511	rBV3	596	672	0.03%	0.003%
84	12.607	3578	3582	3586	rVV2	954	776	0.03%	0.004%
85	12.672	3597	3602	3604	rVV2	749	654	0.03%	0.003%
86	12.781	3633	3636	3641	rVB2	812	693	0.03%	0.004%
87	12.884	3665	3668	3672	rBV2	814	563	0.02%	0.003%
88	13.064	3720	3724	3726	rBV2	926	744	0.03%	0.004%
89	13.498	3856	3859	3864	rVB2	953	817	0.03%	0.004%
90	13.691	3917	3919	3922	rBV	764	544	0.02%	0.003%
91	13.726	3928	3930	3933	rBV	1098	759	0.03%	0.004%
92	13.794	3948	3951	3953	rBV2	1293	936	0.04%	0.005%
93	13.900	3981	3984	3990	rVB2	844	588	0.02%	0.003%
94	14.022	4020	4022	4027	rVB4	908	679	0.03%	0.004%
95	14.324	4113	4116	4118	rBV2	951	599	0.03%	0.003%
96	14.418	4142	4145	4149	rBV3	838	571	0.02%	0.003%
97	14.556	4184	4188	4196	rVB5	1164	1707	0.07%	0.009%
98	14.662	4218	4221	4224	rVB3	1386	812	0.03%	0.004%
99	14.897	4291	4294	4298	rVB4	1135	915	0.04%	0.005%
100	14.938	4305	4307	4309	rBV	1164	785	0.03%	0.004%


Sum of corrected areas: 19206801

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042219\
Data File : VU031395.D
Acq On : 22 Apr 2019 15:39
Operator : JC/SP
Sample : K2428-14DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X14DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

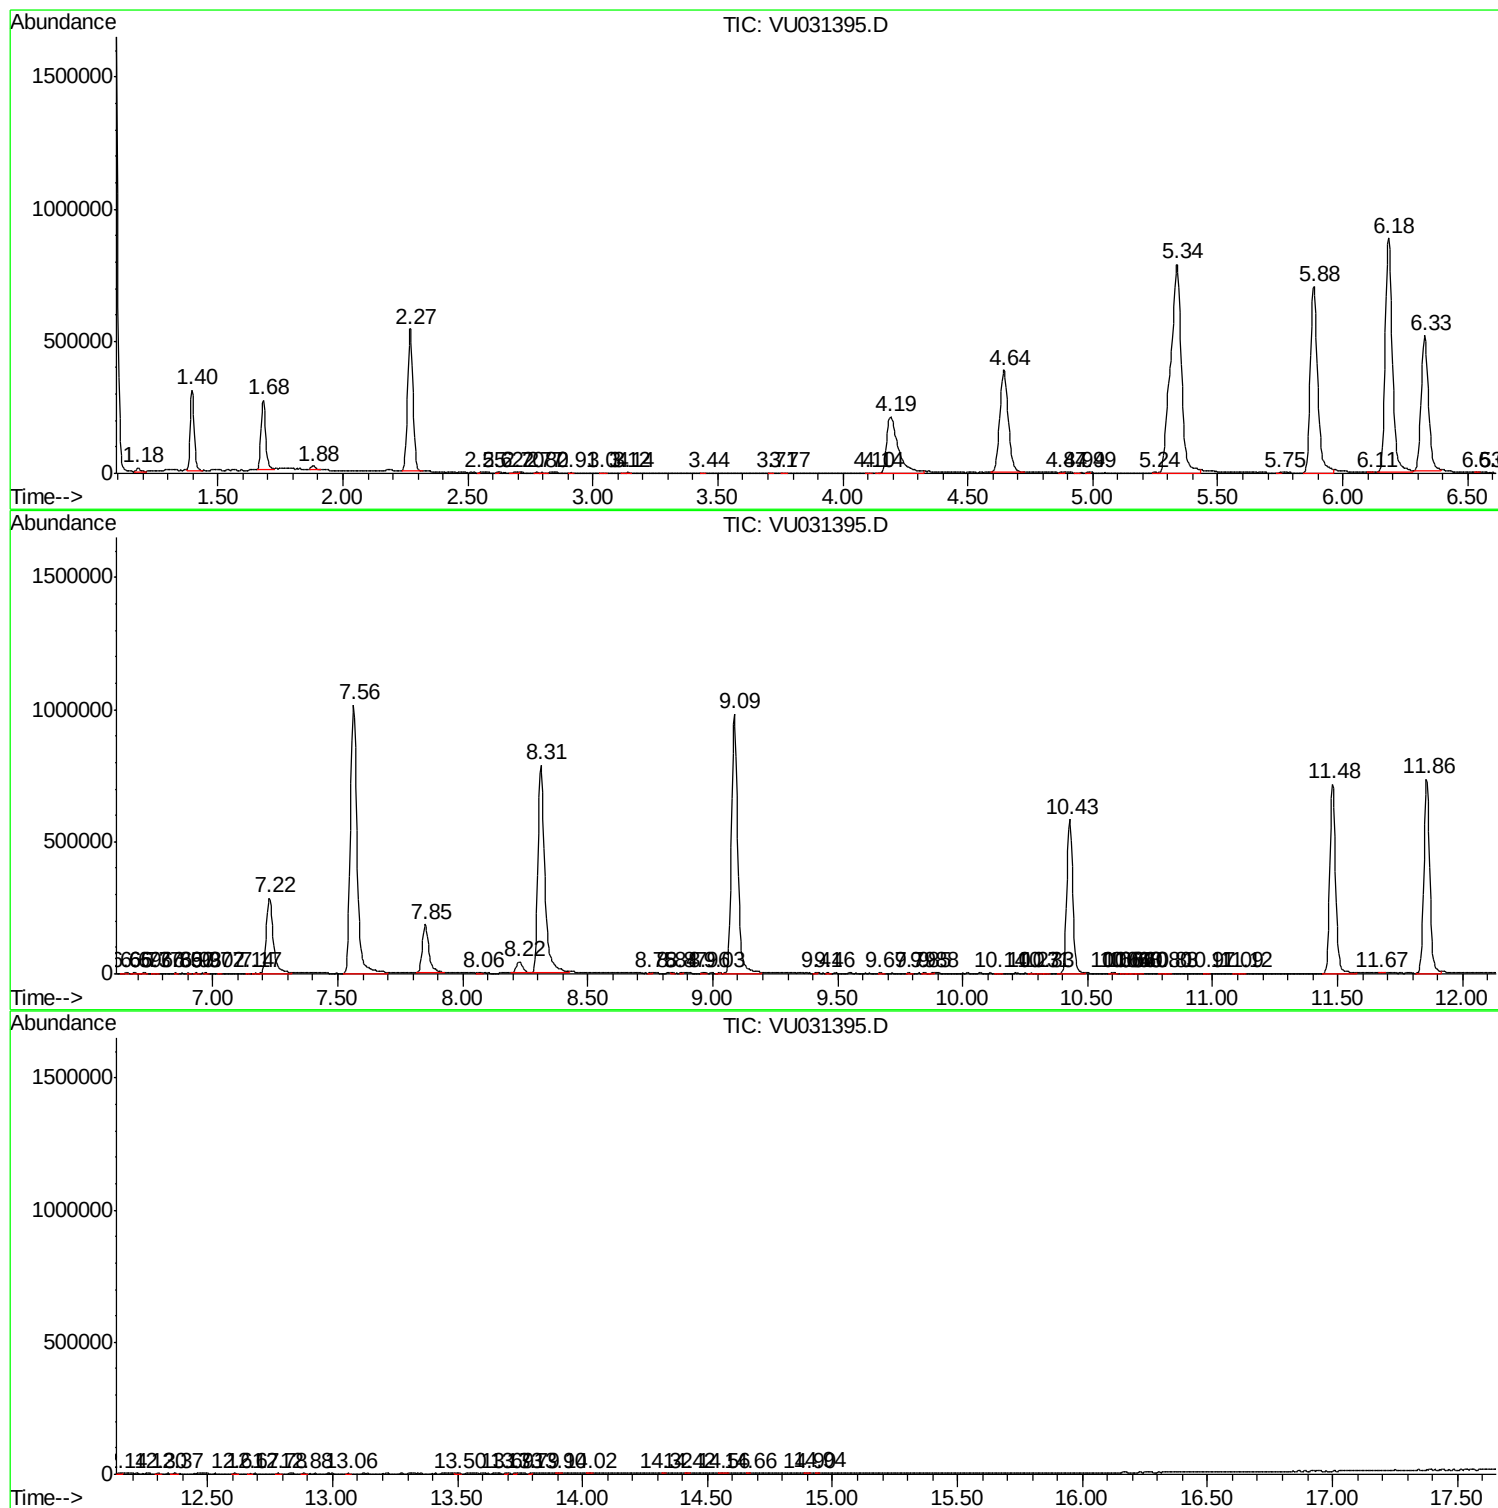

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031395.D
Acq On : 22 Apr 2019 15:39
Operator : JC/SP
Sample : K2428-14DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X14DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042219\
Data File : VU031395.D
Acq On : 22 Apr 2019 15:39
Operator : JC/SP
Sample : K2428-14DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X14DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
