


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042219\
 Data File : VU031381.D
 Acq On : 22 Apr 2019 08:20
 Operator : JC/SP
 Sample : BFB60
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 23 02:53:18 2019

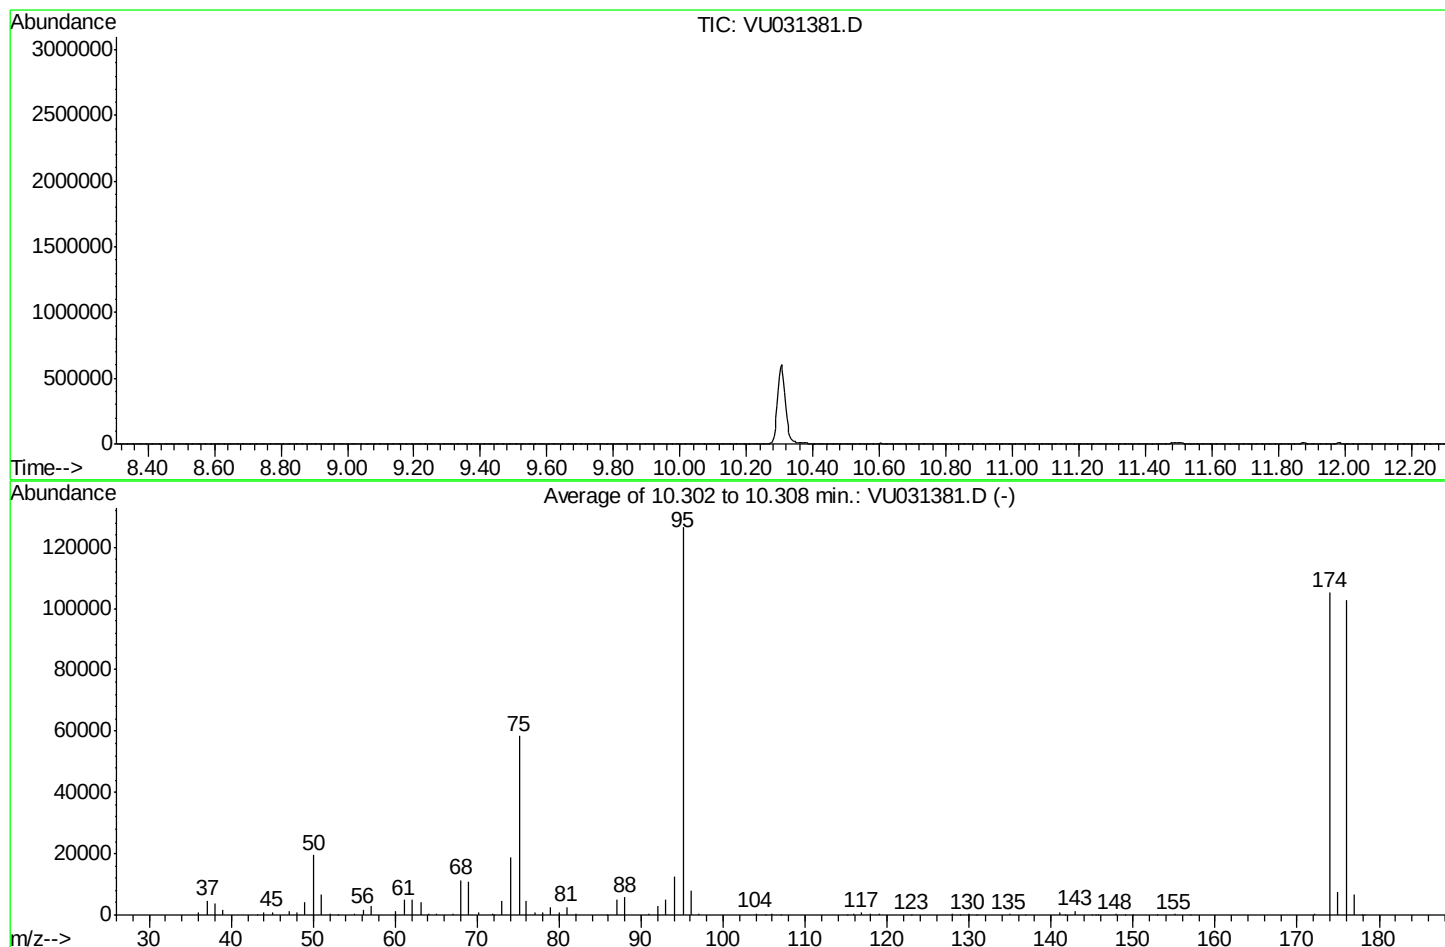

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	19568	PASS
75	95	30	80	46.2	58424	PASS
95	95	100	100	100.0	126493	PASS
96	95	5	9	6.3	8027	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.2	105184	PASS
175	174	5	9	7.1	7493	PASS
176	174	95	101	97.9	102965	PASS
177	176	5	9	6.6	6817	PASS

Scan 2853 (10.263 min): VU031381.D
BFB60

m/z	Abundance
35.10	122.0
36.00	920.0
38.00	321.0
40.00	950.0
41.00	122.0
44.00	560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	1521.0
37.10	5042.0
38.00	4696.0
39.00	1942.0
39.90	896.0
43.20	174.0
44.00	1350.0
45.00	838.0
47.10	1459.0
48.00	830.0
49.00	3915.0
50.10	19712.0
51.00	6295.0
52.00	283.0
52.90	135.0
55.00	339.0
56.10	1806.0
57.10	3300.0
60.10	1142.0
61.10	4971.0
62.00	4820.0
63.10	4016.0
64.10	655.0
64.90	514.0
67.00	455.0
68.00	11382.0
69.00	11205.0
70.20	888.0
71.90	450.0
73.00	4746.0
74.10	18880.0
75.10	59632.0
76.00	4509.0
77.10	911.0
78.00	612.0
78.90	2645.0
80.00	1065.0
80.90	2756.0
82.00	552.0
85.80	176.0
87.00	5532.0
88.00	5479.0
91.00	363.0
92.00	3429.0
93.00	5181.0
94.10	12691.0
95.10	128184.0
96.10	8253.0
96.90	292.0
104.00	481.0
105.10	156.0
106.00	491.0
115.10	152.0
115.90	344.0
116.90	561.0
117.90	438.0
119.10	419.0
122.90	124.0
128.00	397.0
128.80	176.0
129.90	309.0
131.00	192.0
135.00	314.0
137.00	266.0
141.10	767.0
141.70	123.0
143.00	1221.0
144.90	226.0
145.80	267.0
147.80	160.0
150.00	105.0
155.10	381.0
156.90	211.0
172.10	685.0
174.00	103776.0
175.00	7004.0
176.00	102040.0
177.00	6759.0
178.20	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.10	1697.0
37.10	4930.0
38.00	4395.0
39.00	1885.0
39.90	957.0
43.20	225.0
44.00	1297.0
45.00	924.0
47.10	1542.0
48.00	728.0
49.00	4133.0
50.10	19968.0
51.00	6794.0
52.00	253.0
53.00	121.0
55.00	319.0
56.10	1787.0
57.10	3045.0
60.10	1089.0
61.00	5176.0
62.00	5007.0
63.10	4058.0
64.10	494.0
65.00	544.0
67.00	462.0
68.00	11934.0
69.00	11367.0
70.10	989.0
71.90	455.0
73.10	4754.0
74.10	19352.0
75.10	60272.0
76.00	4922.0
77.10	769.0
77.90	635.0
78.90	2718.0
80.10	1017.0
80.90	2652.0
82.00	495.0
85.80	175.0
87.00	5348.0
88.00	5950.0
90.90	400.0
92.00	3162.0
93.00	5315.0
94.10	13043.0
95.10	130280.0
96.10	8367.0
96.90	216.0
104.00	486.0
105.10	145.0
106.00	472.0
115.10	128.0
115.90	390.0
116.90	675.0
117.90	477.0
119.10	541.0
123.00	136.0
128.00	351.0
128.90	182.0
129.90	408.0
130.80	177.0
135.00	336.0
136.90	207.0
141.10	762.0
143.00	1377.0
145.00	176.0
145.80	229.0
147.90	213.0
152.90	118.0
155.10	381.0
157.00	162.0
172.10	643.0
174.00	108448.0
175.00	7688.0
176.00	106432.0
177.00	7118.0
177.90	101.0
178.20	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.10	1706.0
37.10	4451.0
38.00	3721.0
39.00	1717.0
39.90	955.0
41.20	157.0
43.20	231.0
44.00	1123.0
45.00	921.0
47.10	1349.0
48.00	727.0
49.00	4261.0
50.10	19024.0
51.00	6774.0
52.00	182.0
55.10	245.0
56.10	1467.0
57.00	2686.0
60.10	997.0
61.10	4645.0
62.00	4689.0
63.10	3993.0
64.10	308.0
65.00	486.0
67.10	398.0
68.10	11031.0
69.00	10434.0
70.10	973.0
72.10	542.0
73.10	4710.0
74.10	18272.0
75.10	55368.0
76.00	4863.0
77.10	638.0
78.00	700.0
78.90	2571.0
80.10	917.0
81.00	2291.0
82.00	465.0
85.90	132.0
87.00	4496.0
88.00	5651.0
90.90	387.0
92.00	2849.0
93.00	4957.0
94.10	12360.0
95.10	121016.0
96.10	7463.0
97.00	176.0
104.00	460.0
105.10	134.0
106.00	351.0
107.00	110.0
115.90	409.0
116.90	702.0
118.00	441.0
119.00	585.0
128.00	396.0
128.90	247.0
129.90	482.0
130.80	134.0
134.90	286.0
136.80	126.0
140.90	750.0
142.90	1357.0
145.00	168.0
145.40	132.0
145.80	158.0
147.90	321.0
149.00	101.0
149.90	131.0
152.90	139.0
155.00	278.0
157.10	158.0
172.10	589.0
174.00	103328.0
175.00	7787.0
176.00	100424.0
177.00	6574.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60