

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042220\
 Data File : VU037843.D
 Acq On : 22 Apr 2020 15:13
 Operator : JC/MD
 Sample : L2388-01
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFS99

Quant Time: Apr 23 02:16:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 23 01:37:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	265782	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	256384	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	130738	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	70774	3.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.40%
7) Chloroethane-d5	1.93	69	71389	4.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.20%
11) 1,1-Dichloroethene-d2	2.59	63	93904	2.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.60%#
20) 2-Butanone-d5	4.66	46	316237	57.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.50%
24) Chloroform-d	5.10	84	153409	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.74	65	94930	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	5.76	84	303418	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
36) 1,2-Dichloropropane-d6	6.72	67	109168	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.92	98	270105	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
43) trans-1,3-Dichloropropene-	8.20	79	44683	4.41	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.20%
46) 2-Hexanone-d5	8.65	63	277082	53.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.90%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	93390	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	107945	4.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.60%


Target Compounds					Ovalue
13) Acetone	2.66	43	3542	0.973 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042220\
Data File : VU037843.D
Acq On : 22 Apr 2020 15:13
Operator : JC/MD
Sample : L2388-01
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFS99

Quant Time: Apr 23 02:16:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 23 01:37:32 2020
Response via : Initial Calibration

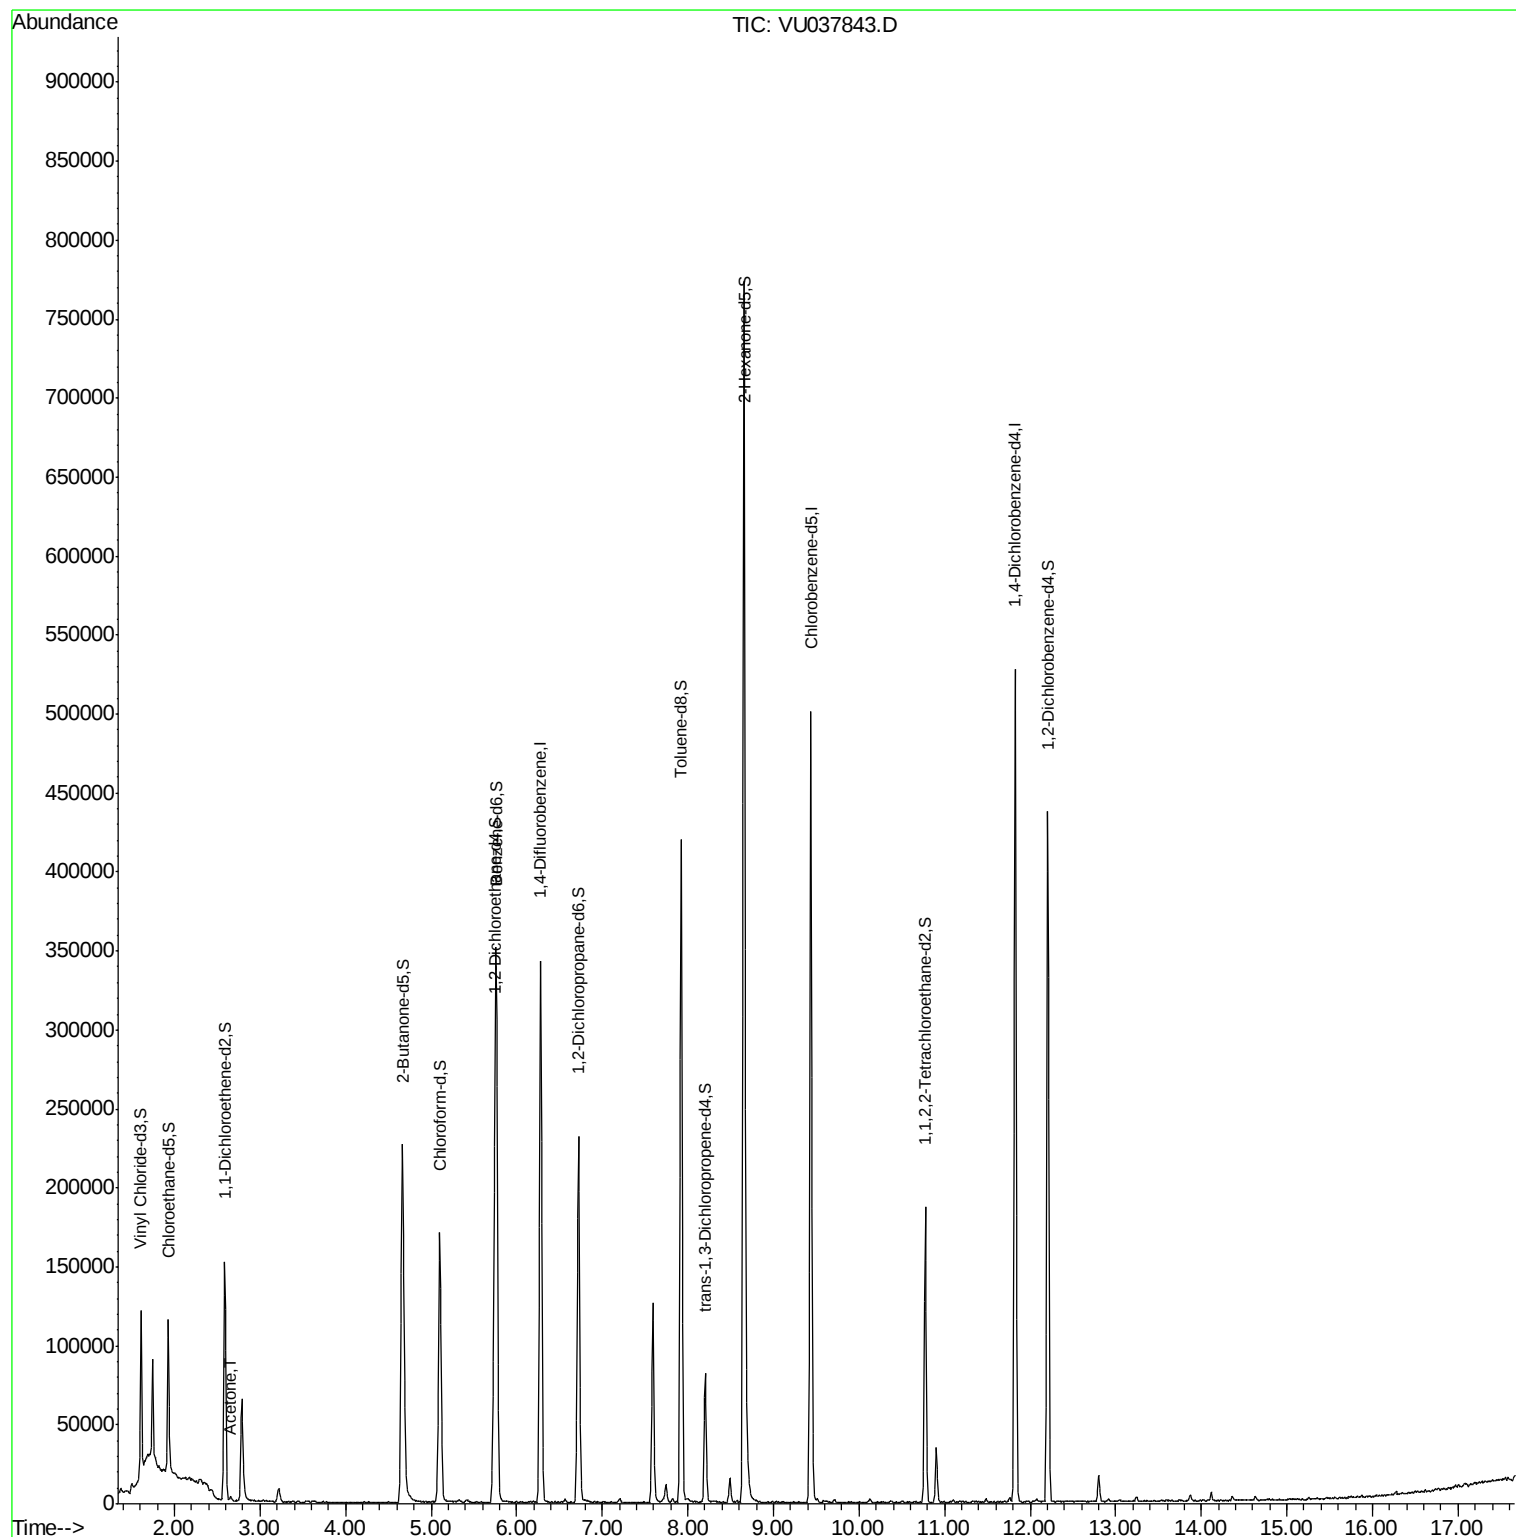

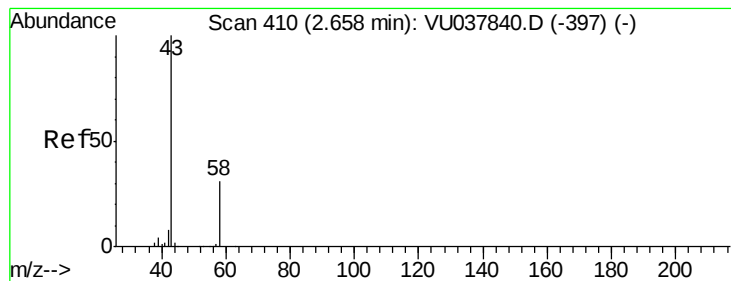

#13
 Acetone
 Concen: 0.973 ug/L
 RT: 2.66 min Scan# 409
 Delta R.T. -0.00 min
 Lab File: VU037843.D
 Acq: 22 Apr 2020 15:13

Instrument :
 MSVOA_U
 ClientSampleId :
 BFS99

Tot Ion: 43 Resp: 3542
 Ion Ratio Lower Upper
 43 100
 58 24.7 0.0 64.8

